

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00925	Calib. Date: 06/27/2011
Certification File No.:	00926	Calib. No.: 00013
Linearity File No.:	00927	Cert. Date: 06/27/2011
Solution File No.:	00986	Cert. No.: 00010
Sequential File No.:	00986	Lin. Date: 06/27/2011
		Lin. No.: 00010
		Soln. Date: 10/09/2011
		Soln. No.: 00103
		File Date: 10/09/2011

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0311
Control Solution %: 0.100%		Expires: 03/10/2012
Solution Control Lot: 10C077		Bottle No.: 1020

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:50D		
Control 1 EC	0.099%	09:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52D		
Control 2 EC	0.098%	09:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53D		
Control 3 EC	0.098%	09:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

OFC. Armstrong #93

Badge No.: 93

Date: 10/09/2011

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00925	Calib. Date: 06/27/2011
Certification File No.:	00926	Calib. No.: 00013
Linearity File No.:	00927	Cert. Date: 06/27/2011
Solution File No.:	00975	Cert. No.: 00010
Sequential File No.:	00975	Lin. Date: 06/27/2011
		Lin. No.: 00010
		Soln. Date: 09/23/2011
		Soln. No.: 00102
		File Date: 09/23/2011

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0311
Control Solution %:	0.100%			Expires:	03/10/2012
Solution Control Lot:	10C077			Bottle No.:	1015

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:38D		
Control 1 EC	0.099%	10:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40D		
Control 2 EC	0.098%	10:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41D		
Control 3 EC	0.098%	10:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 09/23/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00925 Calib. Date: 06/27/2011 Calib. No.: 00013
Certification File No.: 00926 Cert. Date: 06/27/2011 Cert. No.: 00010
Linearity File No.: 00927 Lin. Date: 06/27/2011 Lin. No.: 00010
Solution File No.: 00963 Soln. Date: 09/03/2011 Soln. No.: 00101
Sequential File No.: 00963 File Date: 09/03/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0311
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1014

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:09D		
Control 1 EC	0.099%	12:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:11D		
Control 2 EC	0.098%	12:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:12D		
Control 3 EC	0.099%	12:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 09/03/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00925	Calib. Date: 06/27/2011
Certification File No.:	00926	Calib. No.: 00013
Linearity File No.:	00927	Cert. Date: 06/27/2011
Solution File No.:	00950	Cert. No.: 00010
Sequential File No.:	00950	Lin. Date: 06/27/2011
		Lin. No.: 00010
		Soln. Date: 08/09/2011
		Soln. No.: 00100
		File Date: 08/09/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0311
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1013

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:59D		
Control 1 EC	0.099%	07:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00D		
Control 2 EC	0.099%	08:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:01D		
Control 3 EC	0.098%	08:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

OPC Jack Armstrong #93

Badge No.: 93

Date: 08/09/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00013
Calibration File No.:	00925	Cert. Date:	06/27/2011
Certification File No.:	00926	Lin. Date:	06/27/2011
Linearity File No.:	00927	Soln. Date:	07/20/2011
Solution File No.:	00941	File Date:	07/20/2011
Sequential File No.:	00941		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1011

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:13D		
Control 1 EC	0.099%	09:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14D		
Control 2 EC	0.099%	09:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15D		
Control 3 EC	0.099%	09:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____




Badge No.: 31

Date: 07/20/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00838	Calib. Date:	01/11/2011
Certification File No.:	00839	Cert. Date:	01/11/2011
Linearity File No.:	00840	Lin. Date:	01/11/2011
Solution File No.:	00898	Soln. Date:	05/06/2011
Sequential File No.:	00898	File Date:	05/06/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1007

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:26D		
Control 1 EC	0.099%	20:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:27D		
Control 2 EC	0.099%	20:28D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:28D		
Control 3 EC	0.099%	20:29D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

J.F. Armstrong #93

Badge No.: 93

Date: 05/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00011
Calibration File No.:	00738	Cert. Date:	07/26/2010
Certification File No.:	00739	Lin. Date:	07/26/2010
Linearity File No.:	00740	Soln. Date:	12/22/2010
Solution File No.:	00828	File Date:	12/22/2010
Sequential File No.:	00828		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1001

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:10S		
Control 1 EC	0.101%	13:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:11S		
Control 2 EC	0.101%	13:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:13S		
Control 3 EC	0.100%	13:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 12/22/2010



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.


MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 3/24/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10C077


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1198 to 0.1202 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 10, 2012

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 6th day of April, 2010.


 Notary

Linda L. DiCenzo
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable



Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00738	Calib. Date: 07/26/2010
Certification File No.:	00739	Calib. No.: 00011
Linearity File No.:	00740	Cert. Date: 07/26/2010
Solution File No.:	00820	Cert. No.: 00008
Sequential File No.:	00820	Lin. Date: 07/26/2010
		Lin. No.: 00008
		Soln. Date: 12/03/2010
		Soln. No.: 00088
		File Date: 12/03/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0311
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0956

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:12S		
Control 1 EC	0.097%	00:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	00:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:13S		
Control 2 EC	0.097%	00:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	00:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:14S		
Control 3 EC	0.097%	00:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: TEW

First Name: JOHN

MI: A

Signature: _____



Badge No.: 33

Date: 12/03/2010



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.


MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 3/24/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10C077


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1198 to 0.1202 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 10, 2012

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalck, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 6th day of April, 2010.


 Notary

Paula L. Dow
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00738	Calib. Date: 07/26/2010
Certification File No.:	00739	Calib. No.: 00011
Linearity File No.:	00740	Cert. Date: 07/26/2010
Solution File No.:	00791	Cert. No.: 00008
Sequential File No.:	00791	Lin. Date: 07/26/2010
		Lin. No.: 00008
		Soln. Date: 11/03/2010
		Soln. No.: 00085
		File Date: 11/03/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0311
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0958

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:23S		
Control 1 EC	0.098%	10:24S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:24S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:25S		
Control 2 EC	0.099%	10:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:26S		
Control 3 EC	0.099%	10:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



11/3/10

Badge No.: 31

Date: 11/03/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00738	Calib. Date: 07/26/2010
Certification File No.:	00739	Calib. No.: 00011
Linearity File No.:	00740	Cert. Date: 07/26/2010
Solution File No.:	00768	Cert. No.: 00008
Sequential File No.:	00768	Lin. Date: 07/26/2010
		Lin. No.: 00008
		Soln. Date: 09/09/2010
		Soln. No.: 00082
		File Date: 09/09/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0311
Control Solution %: 0.100%		Expires: 02/02/2011
Solution Control Lot: 09B063		Bottle No.: 0957

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:43D		
Control 1 EC	0.100%	09:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		
Control 2 EC	0.099%	09:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45D		
Control 3 EC	0.100%	09:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 09/09/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00738	Calib. Date: 07/26/2010
Certification File No.:	00739	Calib. No.: 00011
Linearity File No.:	00740	Cert. Date: 07/26/2010
Solution File No.:	00757	Cert. No.: 00008
Sequential File No.:	00757	Lin. Date: 07/26/2010
		Lin. No.: 00008
		Soln. Date: 08/13/2010
		Soln. No.: 00081
		File Date: 08/13/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0311
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0959

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:51D		
Control 1 EC	0.100%	09:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53D		
Control 2 EC	0.100%	09:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		
Control 3 EC	0.100%	09:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____

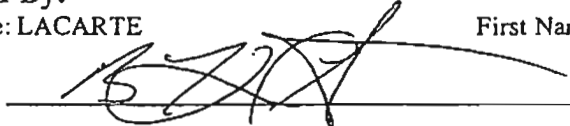

Badge No.: 31

Date: 08/13/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00738	Calib. Date:	07/26/2010
Certification File No.:	00739	Cert. No.:	00011
Linearity File No.:	00740	Cert. Date:	07/26/2010
Solution File No.:	00741	Lin. Date:	07/26/2010
Sequential File No.:	00741	Soln. Date:	07/26/2010
		File Date:	07/26/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	0953

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:17D		
Control 1 EC	0.101%	15:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18D		
Control 2 EC	0.101%	15:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19D		
Control 3 EC	0.101%	15:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDUJPR2 - 1104.u.

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

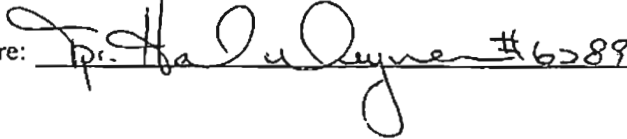Signature:  #6289

Badge No.: 6289

Date: 07/26/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00665	Calib. Date: 02/09/2010
Certification File No.:	00666	Calib. No.: 00008
Linearity File No.:	00667	Cert. Date: 02/09/2010
Solution File No.:	00731	Cert. No.: 00007
Sequential File No.:	00731	Lin. Date: 02/09/2010
		Lin. No.: 00007
		Soln. Date: 07/04/2010
		Soln. No.: 00078
		File Date: 07/04/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0311
Control Solution %: 0.100%		Expires: 02/02/2011
Solution Control Lot: 09B063		Bottle No.: 0962

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:59D		
Control 1 EC	0.101%	08:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	08:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:01D		
Control 2 EC	0.099%	08:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		
Control 3 EC	0.100%	08:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	08:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

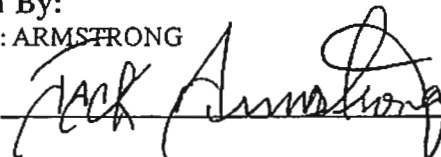

#93

Badge No.: 93

Date: 07/04/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00665	Calib. Date:	02/09/2010
Certification File No.:	00666	Cert. Date:	02/09/2010
Linearity File No.:	00667	Lin. Date:	02/09/2010
Solution File No.:	00723	Soln. Date:	06/16/2010
Sequential File No.:	00723	File Date:	06/16/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	0954

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:34D		
Control 1 EC	0.102%	13:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:36D		
Control 2 EC	0.100%	13:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:37D		
Control 3 EC	0.100%	13:38D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDJSP2-110 *H.W.*

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature: *H. Weyman #6289*

Badge No.: 6289

Date: 06/16/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00665	Calib. Date: 02/09/2010
Certification File No.:	00666	Calib. No.: 00008
Linearity File No.:	00667	Cert. Date: 02/09/2010
Solution File No.:	00716	Cert. No.: 00007
Sequential File No.:	00716	Lin. Date: 02/09/2010
		Lin. No.: 00007
		Soln. Date: 05/24/2010
		Soln. No.: 00076
		File Date: 05/24/2010

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUN S3-0310
Control Solution %:	0.100%		Expires: 02/02/2011
Solution Control Lot:	09B063		Bottle No.: 0967

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:28D		
Control 1 EC	0.102%	12:29D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:29D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29D		
Control 2 EC	0.101%	12:30D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:30D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:31D		
Control 3 EC	0.101%	12:31D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	12:31D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____

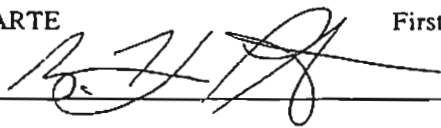

Badge No.: 31

Date: 05/24/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00665 **Calib. Date:** 02/09/2010 **Calib. No.:** 00008
Certification File No.: 00666 **Cert. Date:** 02/09/2010 **Cert. No.:** 00007
Linearity File No.: 00667 **Lin. Date:** 02/09/2010 **Lin. No.:** 00007
Solution File No.: 00688 **Soln. Date:** 03/28/2010 **Soln. No.:** 00074
Sequential File No.: 00688 **File Date:** 03/28/2010

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0310
Control Solution %: 0.100% **Expires:** 02/02/2011
Solution Control Lot: 09B063 **Bottle No.:** 0970

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:14S		
Control 1 EC	0.101%	07:15S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	07:15S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:15S		
Control 2 EC	0.099%	07:16S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:16S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:17S		
Control 3 EC	0.099%	07:17S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	07:17S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

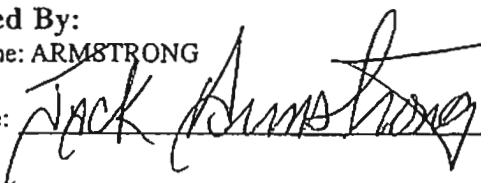

Badge No.: 93

Date: 03/28/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00665	Calib. Date:	02/09/2010
Certification File No.:	00666	Cert. Date:	02/09/2010
Linearity File No.:	00667	Lin. Date:	02/09/2010
Solution File No.:	00678	Soln. Date:	03/08/2010
Sequential File No.:	00678	File Date:	03/08/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	0968

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:20S		
Control 1 EC	0.100%	15:20S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:20S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:21S		
Control 2 EC	0.099%	15:22S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:22S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:23S		
Control 3 EC	0.100%	15:23S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:23S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:24S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____

B. Lacarte 2231

Badge No.: 31

Date: 03/08/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00665	Calib. Date:	02/09/2010
Certification File No.:	00666	Cert. No.:	00007
Linearity File No.:	00667	Lin. Date:	02/09/2010
Solution File No.:	00668	Soln. No.:	00072
Sequential File No.:	00668	File Date:	02/09/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	0964

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:01S		
Control 1 EC	0.101%	14:01S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:01S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:02S		
Control 2 EC	0.100%	14:03S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	14:03S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:03S		
Control 3 EC	0.100%	14:04S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:04S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDWJPZ - 109 H.W.C.

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

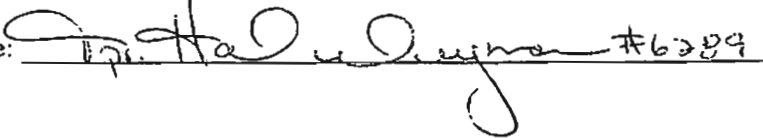Signature:  #6289

Badge No.: 6289

Date: 02/09/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00599	Calib. Date: 08/10/2009
Certification File No.:	00600	Calib. No.: 00007
Linearity File No.:	00601	Cert. Date: 08/10/2009
Solution File No.:	00664	Cert. No.: 00006
Sequential File No.:	00664	Lin. Date: 08/10/2009
		Lin. No.: 00006
		Soln. Date: 02/05/2010
		Soln. No.: 00071
		File Date: 02/05/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0963

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:36S		
Control 1 EC	0.099%	13:37S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:37S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:38S		
Control 2 EC	0.097%	13:38S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:38S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:39S		
Control 3 EC	0.099%	13:40S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:40S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 02/05/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00007
Calibration File No.:	00599	Cert. Date:	08/10/2009
Certification File No.:	00600	Lin. Date:	08/10/2009
Linearity File No.:	00601	Soln. Date:	01/12/2010
Solution File No.:	00654	File Date:	01/12/2010
Sequential File No.:	00654		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0310
Control Solution %:	0.100%			Expires:	02/02/2011
Solution Control Lot:	09B063			Bottle No.:	0969

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:53S		
Control 1 EC	0.100%	08:53S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:53S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:54S		
Control 2 EC	0.097%	08:55S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:55S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56S		
Control 3 EC	0.098%	08:56S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:56S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 01/12/2010