

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	01016	Calib. Date: 11/28/2011
Certification File No.:	01017	Calib. No.: 00014
Linearity File No.:	01018	Cert. Date: 11/28/2011
Solution File No.:	01024	Cert. No.: 00011
Sequential File No.:	01024	Lin. Date: 11/28/2011
		Lin. No.: 00011
		Soln. Date: 12/17/2011
		Soln. No.: 00109
		File Date: 12/17/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1025

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:31S		
Control 1 EC	0.101%	02:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:33S		
Control 2 EC	0.099%	02:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:34S		
Control 3 EC	0.099%	02:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

OC Armstrong #93

Badge No.: 93

Date: 12/17/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00925 Calib. Date: 06/27/2011 Calib. No.: 00013
Certification File No.: 00926 Cert. Date: 06/27/2011 Cert. No.: 00010
Linearity File No.: 00927 Lin. Date: 06/27/2011 Lin. No.: 00010
Solution File No.: 01012 Soln. Date: 11/26/2011 Soln. No.: 00107
Sequential File No.: 01012 File Date: 11/26/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0311
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1022

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:44S		
Control 1 EC	0.096%	07:45S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	07:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:45S		
Control 2 EC	0.095%	07:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	07:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:47S		
Control 3 EC	0.095%	07:47S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	07:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: REINHOLT

First Name: THOMAS

MI: R

Signature: _____



Badge No.: 2276

Date: 11/26/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00925 Calib. Date: 06/27/2011 Calib. No.: 00013
Certification File No.: 00926 Cert. Date: 06/27/2011 Cert. No.: 00010
Linearity File No.: 00927 Lin. Date: 06/27/2011 Lin. No.: 00010
Solution File No.: 01003 Soln. Date: 11/12/2011 Soln. No.: 00105
Sequential File No.: 01003 File Date: 11/12/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0311
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1018

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:47S		
Control 1 EC	0.098%	12:48S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	12:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:49S		
Control 2 EC	0.097%	12:49S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	12:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:50S		
Control 3 EC	0.097%	12:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	12:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: REINHOLT

First Name: THOMAS

MI: R

Signature: _____



Badge No.: 2276

Date: 11/12/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00925 Calib. Date: 06/27/2011 Calib. No.: 00013
Certification File No.: 00926 Cert. Date: 06/27/2011 Cert. No.: 00010
Linearity File No.: 00927 Lin. Date: 06/27/2011 Lin. No.: 00010
Solution File No.: 00998 Soln. Date: 11/03/2011 Soln. No.: 00104
Sequential File No.: 00998 File Date: 11/03/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0311
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1019

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:19S		
Control 1 EC	0.100%	13:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20S		
Control 2 EC	0.099%	13:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21S		
Control 3 EC	0.098%	13:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 11/03/2011

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00925	Calib. Date:	06/27/2011
Certification File No.:	00926	Cert. Date:	06/27/2011
Linearity File No.:	00927	Lin. Date:	06/27/2011
Solution File No.:	00986	Soln. Date:	10/09/2011
Sequential File No.:	00986	File Date:	10/09/2011

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0311
Control Solution %:	0.100%			Expires:	03/10/2012
Solution Control Lot:	10C077			Bottle No.:	1020

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:50D		
Control 1 EC	0.099%	09:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52D		
Control 2 EC	0.098%	09:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53D		
Control 3 EC	0.098%	09:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

OFC. Armstrong #93

Badge No.: 93

Date: 10/09/2011

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00925	Calib. Date: 06/27/2011
Certification File No.:	00926	Calib. No.: 00013
Linearity File No.:	00927	Cert. Date: 06/27/2011
Solution File No.:	00975	Cert. No.: 00010
Sequential File No.:	00975	Lin. Date: 06/27/2011
		Lin. No.: 00010
		Soln. Date: 09/23/2011
		Soln. No.: 00102
		File Date: 09/23/2011

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0311
Control Solution %:	0.100%			Expires:	03/10/2012
Solution Control Lot:	10C077			Bottle No.:	1015

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:38D		
Control 1 EC	0.099%	10:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40D		
Control 2 EC	0.098%	10:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41D		
Control 3 EC	0.098%	10:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____

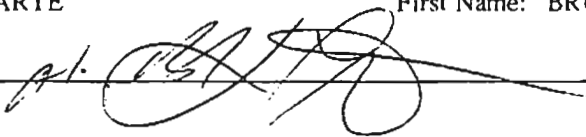

Badge No.: 31

Date: 09/23/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00925 Calib. Date: 06/27/2011 Calib. No.: 00013
Certification File No.: 00926 Cert. Date: 06/27/2011 Cert. No.: 00010
Linearity File No.: 00927 Lin. Date: 06/27/2011 Lin. No.: 00010
Solution File No.: 00963 Soln. Date: 09/03/2011 Soln. No.: 00101
Sequential File No.: 00963 File Date: 09/03/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0311
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1014

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:09D		
Control 1 EC	0.099%	12:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:11D		
Control 2 EC	0.098%	12:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:12D		
Control 3 EC	0.099%	12:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 09/03/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00925	Calib. Date:	06/27/2011
Certification File No.:	00926	Cert. Date:	06/27/2011
Linearity File No.:	00927	Lin. Date:	06/27/2011
Solution File No.:	00950	Soln. Date:	08/09/2011
Sequential File No.:	00950	File Date:	08/09/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1013

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:59D		
Control 1 EC	0.099%	07:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00D		
Control 2 EC	0.099%	08:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:01D		
Control 3 EC	0.098%	08:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: OPC. Jack Armstrong #93

Badge No.: 93

Date: 08/09/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00925	Calib. Date:	06/27/2011
Certification File No.:	00926	Cert. No.:	00013
Linearity File No.:	00927	Lin. Date:	06/27/2011
Solution File No.:	00941	Lin. No.:	00010
Sequential File No.:	00941	Soln. Date:	07/20/2011
		Soln. No.:	00099
		File Date:	07/20/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1011

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:13D		
Control 1 EC	0.099%	09:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14D		
Control 2 EC	0.099%	09:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15D		
Control 3 EC	0.099%	09:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____




Badge No.: 31

Date: 07/20/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00838 Calib. Date: 01/11/2011 Calib. No.: 00012
Certification File No.: 00839 Cert. Date: 01/11/2011 Cert. No.: 00009
Linearity File No.: 00840 Lin. Date: 01/11/2011 Lin. No.: 00009
Solution File No.: 00917 Soln. Date: 06/13/2011 Soln. No.: 00097
Sequential File No.: 00917 File Date: 06/13/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0310
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1006

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:07D		
Control 1 EC	0.099%	09:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:09D		
Control 2 EC	0.099%	09:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:10D		
Control 3 EC	0.099%	09:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____

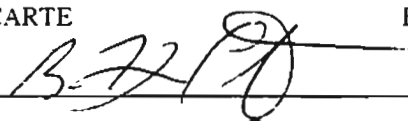

Badge No.: 31

Date: 06/13/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00838 Calib. Date: 01/11/2011 Calib. No.: 00012
Certification File No.: 00839 Cert. Date: 01/11/2011 Cert. No.: 00009
Linearity File No.: 00840 Lin. Date: 01/11/2011 Lin. No.: 00009
Solution File No.: 00908 Soln. Date: 05/27/2011 Soln. No.: 00096
Sequential File No.: 00908 File Date: 05/27/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0310
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1008

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:43D		
Control 1 EC	0.099%	11:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:44D		
Control 2 EC	0.099%	11:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:46D		
Control 3 EC	0.099%	11:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 05/27/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00838	Calib. Date:	01/11/2011
Certification File No.:	00839	Cert. Date:	01/11/2011
Linearity File No.:	00840	Lin. Date:	01/11/2011
Solution File No.:	00898	Soln. Date:	05/06/2011
Sequential File No.:	00898	File Date:	05/06/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1007

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:26D		
Control 1 EC	0.099%	20:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:27D		
Control 2 EC	0.099%	20:28D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:28D		
Control 3 EC	0.099%	20:29D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

J.F. Armstrong #93

Badge No.: 93

Date: 05/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00012
Calibration File No.:	00838	Cert. Date:	01/11/2011
Certification File No.:	00839	Lin. Date:	01/11/2011
Linearity File No.:	00840	Soln. Date:	04/17/2011
Solution File No.:	00888	File Date:	04/17/2011
Sequential File No.:	00888		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	1010

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:38D		
Control 1 EC	0.098%	11:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:39D		
Control 2 EC	0.098%	11:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:41D		
Control 3 EC	0.099%	11:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: REINHOLT

First Name: THOMAS

MI: R

Signature: _____



Badge No.: 2276

Date: 04/17/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00838 Calib. Date: 01/11/2011 Calib. No.: 00012
Certification File No.: 00839 Cert. Date: 01/11/2011 Cert. No.: 00009
Linearity File No.: 00840 Lin. Date: 01/11/2011 Lin. No.: 00009
Solution File No.: 00874 Soln. Date: 03/22/2011 Soln. No.: 00093
Sequential File No.: 00874 File Date: 03/22/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0310
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1009

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:54S		
Control 1 EC	0.100%	13:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:56S		
Control 2 EC	0.100%	13:56S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:57S		
Control 3 EC	0.100%	13:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 03/22/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00838	Calib. Date: 01/11/2011
Certification File No.:	00839	Calib. No.: 00012
Linearity File No.:	00840	Cert. Date: 01/11/2011
Solution File No.:	00867	Cert. No.: 00009
Sequential File No.:	00867	Lin. Date: 01/11/2011
		Lin. No.: 00009
		Soln. Date: 02/27/2011
		Soln. No.: 00092
		File Date: 02/27/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1004

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:26S		
Control 1 EC	0.099%	09:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27S		
Control 2 EC	0.098%	09:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28S		
Control 3 EC	0.098%	09:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

Jack J. Armstrong #93

Badge No.: 93

Date: 02/27/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00838 Calib. Date: 01/11/2011 Calib. No.: 00012
Certification File No.: 00839 Cert. Date: 01/11/2011 Cert. No.: 00009
Linearity File No.: 00840 Lin. Date: 01/11/2011 Lin. No.: 00009
Solution File No.: 00849 Soln. Date: 02/08/2011 Soln. No.: 00091
Sequential File No.: 00849 File Date: 02/08/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0310
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1003

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:34S		
Control 1 EC	0.100%	09:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:35S		
Control 2 EC	0.100%	09:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:36S		
Control 3 EC	0.100%	09:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 02/08/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00838	Calib. Date: 01/11/2011
Certification File No.:	00839	Calib. No.: 00012
Linearity File No.:	00840	Cert. Date: 01/11/2011
Solution File No.:	00841	Cert. No.: 00009
Sequential File No.:	00841	Lin. Date: 01/11/2011
		Lin. No.: 00009
		Soln. Date: 01/11/2011
		Soln. No.: 00090
		File Date: 01/11/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1002

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:34S		
Control 1 EC	0.100%	12:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35S		
Control 2 EC	0.100%	12:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:36S		
Control 3 EC	0.100%	12:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDWJPZ-1094 ul.

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

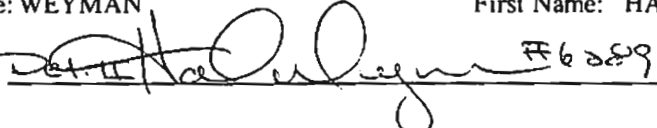Signature: 

#6289

Badge No.: 6289

Date: 01/11/2011



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 3/24/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10C077


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1198 to 0.1202 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 10, 2012

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 6th day of April, 2010.


 Notary

Linda L. Danovitch
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable

