

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARDC-0066  
**Location:** EVESHAM TOWNSHIP P.D.  
**Calibration File No.:** 00152 **Calib. Date:** 10/07/2013 **Calib. No.:** 00009  
**Certification File No.:** 00153 **Cert. Date:** 10/07/2013 **Cert. No.:** 00005  
**Linearity File No.:** 00154 **Lin. Date:** 10/07/2013 **Lin. No.:** 00004  
**Solution File No.:** 00168 **Soln. Date:** 11/27/2013 **Soln. No.:** 00030  
**Sequential File No.:** 00168 **File Date:** 11/27/2013

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDDC-0001  
**Control Solution %:** 0.100% **Expires:** 03/02/2014  
**Solution Control Lot:** 12C100 **Bottle No.:** 1083

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:30S		
Control 1 EC	0.102%	11:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31S		
Control 2 EC	0.100%	11:32S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:32S		
Control 3 EC	0.100%	11:33S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:34S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: RITTER

First Name: RONALD

MI: C

Signature: \_\_\_\_\_

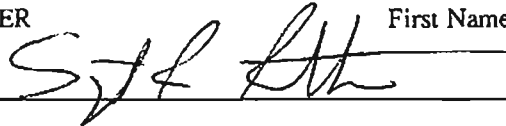

Badge No.: 63

Date: 11/27/2013







State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

JEFFREY S. CHIESA  
 Attorney General

KIM GUADAGNO  
 Lt. Governor

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 3/21/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12C100

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 2, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Monica L. Trapontin  
 Forensic Scientist III  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 23rd day of March, 2012.

Notary

MARY ELIZABETH MCLAUGHLIN  
 NOTARY PUBLIC OF NEW JERSEY  
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable



# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARDC-0066  
**Location:** EVESHAM TOWNSHIP P.D.  
**Calibration File No.:** 00087 **Calib. Date:** 04/29/2013 **Calib. No.:** 00008  
**Certification File No.:** 00088 **Cert. Date:** 04/29/2013 **Cert. No.:** 00004  
**Linearity File No.:** 00089 **Lin. Date:** 04/29/2013 **Lin. No.:** 00003  
**Solution File No.:** 00149 **Soln. Date:** 10/01/2013 **Soln. No.:** 00027  
**Sequential File No.:** 00149 **File Date:** 10/01/2013

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0311  
**Control Solution %:** 0.100% **Expires:** 03/02/2014  
**Solution Control Lot:** 12C100 **Bottle No.:** 1089

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:04D		
Control 1 EC	0.100%	17:05D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:06D		
Control 2 EC	0.099%	17:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07D		
Control 3 EC	0.098%	17:08D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: RITTER

First Name: RONALD

MI: C

Signature: \_\_\_\_\_

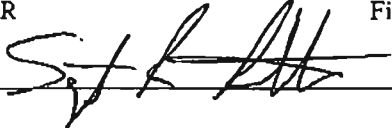

Badge No.: 63

Date: 10/01/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00008
Calibration File No.:	00087	Calib. Date:	04/29/2013
Certification File No.:	00088	Cert. Date:	04/29/2013
Linearity File No.:	00089	Lin. Date:	04/29/2013
Solution File No.:	00141	Soln. Date:	09/03/2013
Sequential File No.:	00141	File Date:	09/03/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0311
Control Solution %:	0.100%			Expires:	03/02/2014
Solution Control Lot:	12C100			Bottle No.:	1079

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:04D		
Control 1 EC	0.100%	12:05D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:06D		
Control 2 EC	0.098%	12:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	12:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07D		
Control 3 EC	0.098%	12:08D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: RITTER

First Name: RONALD

MI: C

Signature: \_\_\_\_\_



Badge No.: 63

Date: 09/03/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00087	Calib. Date:	04/29/2013
Certification File No.:	00088	Cert. Date:	04/29/2013
Linearity File No.:	00089	Lin. Date:	04/29/2013
Solution File No.:	00131	Soln. Date:	08/04/2013
Sequential File No.:	00131	File Date:	08/04/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0311
Control Solution %:	0.100%			Expires:	03/02/2014
Solution Control Lot:	12C100			Bottle No.:	1077

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:12D		
Control 1 EC	0.098%	09:12D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	09:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13D		
Control 2 EC	0.097%	09:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14D		
Control 3 EC	0.097%	09:15D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: DOUGHERTY

First Name: ANDREW

MI: B

Signature:

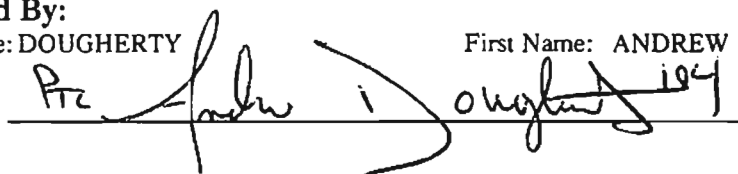

Badge No.: 104

Date: 08/04/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00087	Calib. Date: 04/29/2013
Certification File No.:	00088	Calib. No.: 00008
Linearity File No.:	00089	Cert. Date: 04/29/2013
Solution File No.:	00121	Cert. No.: 00004
Sequential File No.:	00121	Lin. Date: 04/29/2013
		Lin. No.: 00003
		Soln. Date: 07/09/2013
		Soln. No.: 00024
		File Date: 07/09/2013

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUN S3-0311
Control Solution %:	0.100%		Expires: 03/02/2014
Solution Control Lot:	12C100		Bottle No.: 1088

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:14D		
Control 1 EC	0.103%	11:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		
Control 2 EC	0.101%	11:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		
Control 3 EC	0.101%	11:17D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: *Ritter*

First Name: RONALD

MI: C

Signature: \_\_\_\_\_

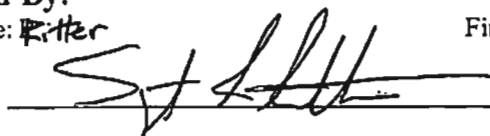

Badge No.: 63

Date: 07/09/2013



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00087	Calib. Date:	04/29/2013
Certification File No.:	00088	Cert. Date:	04/29/2013
Linearity File No.:	00089	Lin. Date:	04/29/2013
Solution File No.:	00113	Soln. Date:	06/10/2013
Sequential File No.:	00113	File Date:	06/10/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	12C100	Expires:	03/02/2014
		Bottle No.:	1081

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:23D		
Control 1 EC	0.100%	06:24D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	06:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:24D		
Control 2 EC	0.098%	06:25D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:26D		
Control 3 EC	0.098%	06:26D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:27D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: \_\_\_\_\_

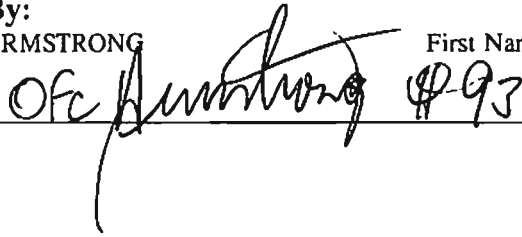

Badge No.: 93

Date: 06/10/2013

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARDC-0066  
**Location:** EVESHAM TOWNSHIP P.D.  
**Calibration File No.:** 00087 **Calib. Date:** 04/29/2013 **Calib. No.:** 00008  
**Certification File No.:** 00088 **Cert. Date:** 04/29/2013 **Cert. No.:** 00004  
**Linearity File No.:** 00089 **Lin. Date:** 04/29/2013 **Lin. No.:** 00003  
**Solution File No.:** 00110 **Soln. Date:** 06/07/2013 **Soln. No.:** 00022  
**Sequential File No.:** 00110 **File Date:** 06/07/2013

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0311  
**Control Solution %:** 0.100% **Expires:** 03/02/2014  
**Solution Control Lot:** 12C100 **Bottle No.:** 1096

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:05D		
Control 1 EC	0.096%	11:06D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	11:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:07D		
Control 2 EC	0.096%	11:08D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	11:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		
Control 3 EC	0.095%	11:09D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	11:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: DOUGHERTY

First Name: ANDREW

MI: B

Signature: Andrew Dougherty

Badge No.: 104

Date: 06/07/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
<b>Location:</b>	EVESHAM TOWNSHIP P.D.		
<b>Calibration File No.:</b>	00087	<b>Calib. Date:</b>	04/29/2013
<b>Certification File No.:</b>	00088	<b>Cert. Date:</b>	04/29/2013
<b>Linearity File No.:</b>	00089	<b>Lin. Date:</b>	04/29/2013
<b>Solution File No.:</b>	00103	<b>Soln. Date:</b>	05/24/2013
<b>Sequential File No.:</b>	00103	<b>File Date:</b>	05/24/2013
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUN S3-0311
<b>Solution Control Lot:</b>	12C100	<b>Expires:</b>	03/02/2014
		<b>Bottle No.:</b>	1080

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:33D		
Control 1 EC	0.098%	23:34D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:34D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:35D		
Control 2 EC	0.098%	23:35D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:36D		
Control 3 EC	0.098%	23:37D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: Jack Armstrong #93

Badge No.: 93

Date: 05/24/2013

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARDC-0066  
**Location:** EVESHAM TOWNSHIP P.D.  
**Calibration File No.:** 00087 **Calib. Date:** 04/29/2013 **Calib. No.:** 00008  
**Certification File No.:** 00088 **Cert. Date:** 04/29/2013 **Cert. No.:** 00004  
**Linearity File No.:** 00089 **Lin. Date:** 04/29/2013 **Lin. No.:** 00003  
**Solution File No.:** 00096 **Soln. Date:** 05/13/2013 **Soln. No.:** 00020  
**Sequential File No.:** 00096 **File Date:** 05/13/2013

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0311  
**Control Solution %:** 0.100% **Expires:** 03/02/2014  
**Solution Control Lot:** 12C100 **Bottle No.:** 1086

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:44D		
Control 1 EC	0.100%	12:45D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:46D		
Control 2 EC	0.099%	12:46D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:47D		
Control 3 EC	0.099%	12:48D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: RITTER

First Name: RONALD

MI: C

Signature: \_\_\_\_\_

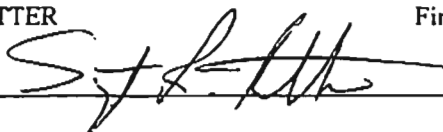

Badge No.: 63

Date: 05/13/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00007
Calibration File No.:	00042	Cert. Date:	11/14/2012
Certification File No.:	00043	Lin. Date:	11/14/2012
Linearity File No.:	00044	Soln. Date:	04/22/2013
Solution File No.:	00086	File Date:	04/22/2013
Sequential File No.:	00086		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0311
Control Solution %:	0.100%			Expires:	09/13/2014
Solution Control Lot:	121107			Bottle No.:	0986

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:24D		
Control 1 EC	-.---%	13:24D	N/A	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	13:24D	N/A	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: RITTER

First Name: RONALD

MI: C

Signature: \_\_\_\_\_

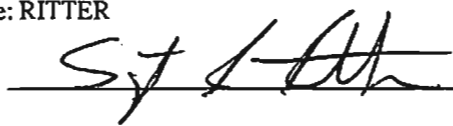

Badge No.: 63

Date: 04/22/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00042	Calib. Date:	11/14/2012
Certification File No.:	00043	Cert. Date:	11/14/2012
Linearity File No.:	00044	Lin. Date:	11/14/2012
Solution File No.:	00085	Soln. Date:	04/20/2013
Sequential File No.:	00085	File Date:	04/20/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	121107	Expires:	09/13/2014
		Bottle No.:	0983

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:11D		
Control 1 EC	-.---%	19:12D	N/A	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	19:12D	N/A	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: DEGREGORIO

First Name: MICHAEL

MI: J

Signature: \_\_\_\_\_



Badge No.: 117

Date: 04/20/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00042	Calib. Date:	11/14/2012
Certification File No.:	00043	Cert. Date:	11/14/2012
Linearity File No.:	00044	Lin. Date:	11/14/2012
Solution File No.:	00084	Soln. Date:	04/20/2013
Sequential File No.:	00084	File Date:	04/20/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0311
Solution Control Lot:	121107	Expires:	09/13/2014
		Bottle No.:	0988

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:00D		
Control 1 EC	-.---%	19:01D	N/A	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	19:01D	N/A	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: DEGREGORIO

First Name: MICHAEL

MI: J

Signature: \_\_\_\_\_



Badge No.: 117

Date: 04/20/2013