

ALCOTEST CHECKLIST

Municipality: FLORENCE TWP Alcotest Ser.#: ARTN - 0053

County: BURLINGTON Date of Calibration: 12-19-2019

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDUM 53-0222
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWT 12-293
- 4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 191959 016
- 5. **NIST - Traceable Digital Thermometer Readings.**
- 6.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator]
Ser. #: DDXK 12-396
- 7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>18240</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>18250</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>18220</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>18260</u>
- 8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety

<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>18260</u>
--	-----------------	--------------
- 8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

<input type="checkbox"/>	A.	0.04% used in Calibration/Linearity Testing.	<u>DDWE 53-0206</u>
<input type="checkbox"/>	B.	0.08% used in Calibration/Linearity Testing.	<u>DDWF 53-0218</u>
<input type="checkbox"/>	C.	0.10% used in Calibration/Linearity Testing. [Same as CU34 unit on instrument.]	
<input type="checkbox"/>	D.	0.16% used in Calibration/Linearity Testing.	<u>DDWI 53-0334</u>
- 9.
 - A. New Standard Solution Report following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 19240

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48884 and 59 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

1-10-17

SERIAL NUMBER:

ARTN-0053

Dräger Safety Diagnostics, Inc.

BC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

BDUM 53-0222

Certification Date:

Technician:

Re-Certification Due Date:

10-16-19

BS/JL

10-16-20

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDWJ P2-293

10-16-19

10-16-20

Probe Value:

104

Draeger, Inc.

BS/JL



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177835

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 191959016 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	20 Apr 2019	1000424560
Thermistor Module	A27129	10 Jan 2020	1000436202
Temperature Calibration Bath	A73332		
Temperature Probe	3039	08 May 2019	6-B7F4L-20-1
Temperature Calibration Bath	A79341		
Temperature Probe	5394	29 Jan 2020	B9124038
Temperature Calibration Bath	B16388		
Temperature Probe	5267	28 Jan 2020	B9124036

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 13 Feb 2019 Cal Due Date: 13 Feb 2021
 Test Conditions: 38.85%RH 24.21°C 1023mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	0.000	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.000	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.000	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.001	100.004	Y	99.951	100.051	0.0087	>4:1

This certificate indicates traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max=As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Justice
Aaron Justice, Technical Manager

Note

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RVA.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177835

Traceable® Certificate of Calibration for Digital Thermometer

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.D1
Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

TR. 1 DAVID M. NAPOLITANO
Name

7237
Badge No.

Location:

FLORENCE TOWNSHIP P.D.
Agency


ARTN-0053
Alcotest Serial No.

Equipment:

191 959 016
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDWE 53-0206	0840 S	0942 S	34.0 °C
0.08%	DDWF 53-0218	0840 S	0943 S	34.0 °C
0.10%	DDUM 53-0222	0840 S	0943 S	34.0 °C
0.16%	DDWJ 53-0334	0840 S	0944 S	34.0 °C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.


Coordinator's Signature

12.19.19
Date

Alcotest 7110 Calibration Record

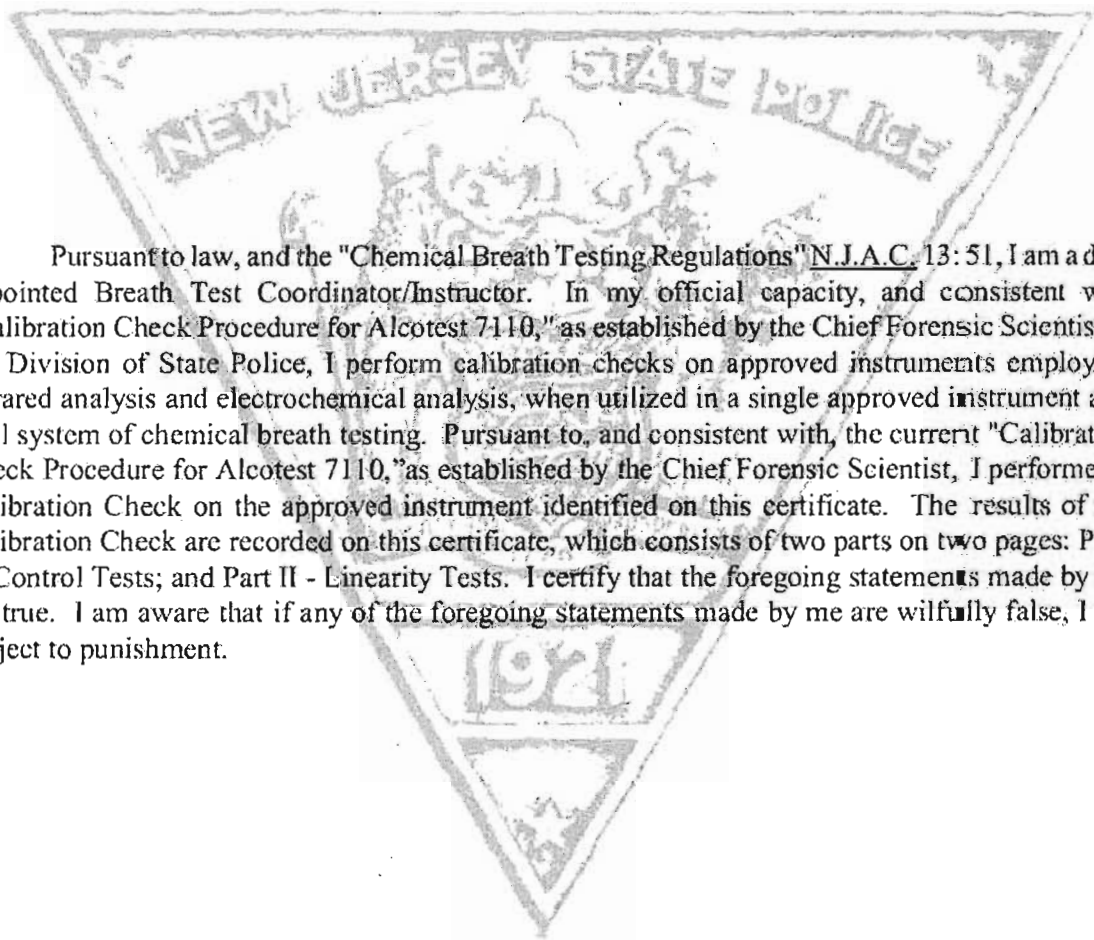
Equipment Alcotest-7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01068 Calib. Date: 12/19/2019 Calib. No.: 00040
Certification File No.: 01038 Cert. Date: 07/09/2019 Cert. No.: 00031
Linearity File No.: 01039 Lin. Date: 07/09/2019 Lin. No.: 00031
Solution File No.: 01064 Soln. Date: 12/04/2019 Soln. No.: 00239
Sequential File No.: 01068 File Date: 12/19/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 07/23/2020
Solution Control Lot: 18220 Bottle No.: 0582

Coordinator

Last Name: NAPOLITANO First Name: DAVID MI: M.
Signature: *David Napolitano* 7237 Badge No.: 7237
Date: 12/19/2019

*Black Key Temperature Probe Serial.....# DDXK P2-396 (DN)
*Digital NIST Temperature Measuring System Serial.....# 191 959 016 (DN)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13: 51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01068 Calib. Date: 12/19/2019 Calib. No.: 00040
Certification File No.: 01069 Cert. Date: 12/19/2019 Cert. No.: 00032
Linearity File No.: 01039 Lin. Date: 07/09/2019 Lin. No.: 00031
Solution File No.: 01064 Soln. Date: 12/04/2019 Soln. No.: 00239
Sequential File No.: 01069 File Date: 12/19/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 07/23/2020
Solution Control Lot: 18220 Bottle No.: 0582

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:50S		
Control 1 EC	0.100%	09:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		
Control 2 EC	0.098%	09:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53S		
Control 3 EC	0.097%	09:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54S		

All tests within acceptable tolerance.

Coordinator

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature: *David M. Napolitano* 7237

Badge No.: 7237

Date: 12/19/2019

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment

Alcotest 7110 MKIII-C
Location: FLORENCE TOWNSHIP P.D. Serial No.: ARTN-0053
Calibration File No.: 01068 Calib. Date: 12/19/2019 Calib. No.: 00040
Certification File No.: 01069 Cert. Date: 12/19/2019 Cert. No.: 00032
Linearity File No.: 01070 Lin. Date: 12/19/2019 Lin. No.: 00032
Solution File No.: 01064 Soln. Date: 12/04/2019 Soln. No.: 00239
Sequential File No.: 01070 File Date: 12/19/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0206
Control Solution %: 0.040% Expires: 07/31/2020
Solution Control Lot: 18240 Bottle No.: 0542

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0218
Control Solution %: 0.080% Expires: 08/06/2020
Solution Control Lot: 18250 Bottle No.: 0304

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0334
Control Solution %: 0.160% Expires: 08/21/2020
Solution Control Lot: 18260 Bottle No.: 0370

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:05S		
Control 1 EC	0.041%	10:06S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	10:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08S		
Control 2 EC	0.038%	10:08S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.039%	10:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:10S		
Control 3 EC	0.081%	10:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	10:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:12S		
Control 4 EC	0.080%	10:13S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	10:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14S		
Control 5 EC	0.160%	10:15S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.160%	10:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17S		
Control 6 EC	0.156%	10:17S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.159%	10:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:19S		


All tests within acceptable tolerance.

Coordinator

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature: 

Badge No.: 7237

Date: 12/19/2019

DEPARTMENT OF
Law and Public Safety
 This is to certify that

David M. Napolitano

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1964 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 9th DAY OF October

TWO THOUSAND AND Eighteen

[Signature]
 COLONEL
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2538 (Rev. 01/15)

DEPARTMENT OF
Law and Public Safety
 This is to certify that

David M. Napolitano
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1964 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 7th DAY OF October

TWO THOUSAND AND Ten

[Signature]
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 6/20/12	CAPE MAY P.A.	Adam Stankis
2. 11/6/14	CCPA	Adam Stankis
3. 6/23/16	CCPA	Adam Stankis
4. 1/16/18	LAKE HURLEY	Adam Stankis
5.		
6.		
7.		
8.		
9.		

S.P. 2538 (Rev. 03/10)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/28/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0486 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 31, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29th day of August, 2018.

Mary E. McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/30/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0976 to 0.0987 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 06, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 4th day of September, 2018.
Mary E. McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency
New Jersey is an Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 07/31/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1210 to 0.1233 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of August, 2018.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/13/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1938 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of September 2018.

Mary E. McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDWES3-0206

Certification Date:

7-19-19

Technician:

BS

Re-Certification Due Date:

7-19-20

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDWFS3-0218

Certification Date:

7-19-19

Technician:

BS

Re-Certification Due Date:

7-19-20

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDW153-0334

Certification Date:

7-19-19

Technician:

BS

Re-Certification Due Date:

7-19-20

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2-396

Certification Date:

7-18-19

Next Certification Due:

7-18-20

Probe Value:

10.4

Draeger, Inc.

BS

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01068	Calib. Date:	12/19/2019
Certification File No.:	01069	Cert. No.:	00040
Linearity File No.:	01070	Cert. Date:	12/19/2019
Solution File No.:	01071	Lin. Date:	12/19/2019
Sequential File No.:	01071	Lin. No.:	00032
		Soln. Date:	12/19/2019
		Soln. No.:	00240
		File Date:	12/19/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	19240	Expires:	09/09/2021
		Bottle No.:	0566

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:25S		
Control 1 EC	0.100%	11:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:26S		
Control 2 EC	0.099%	11:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:28S		
Control 3 EC	0.096%	11:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:29S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJ P2-293 (2)

Changed By:

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature:  7237

Badge No.: 7237

Date: 12/19/2019



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/19/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1209 to 0.1240 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 09, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 26 day of September, 2019.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

