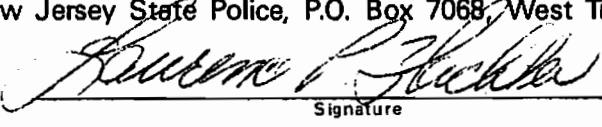
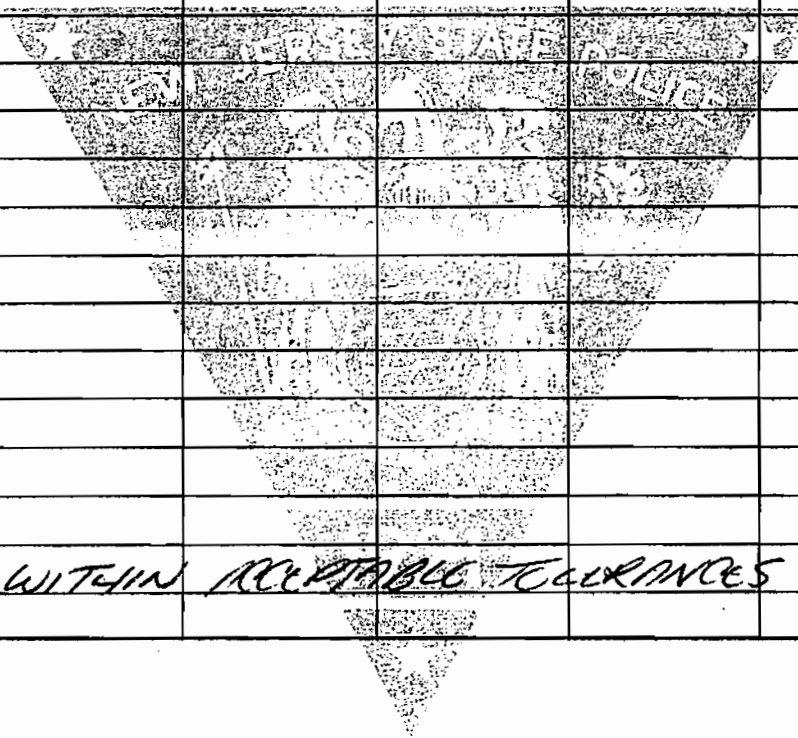
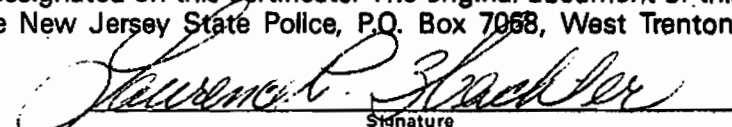


STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE				Periodic Inspection	<input checked="" type="checkbox"/>	Number	104-01
				Other Inspection	<input type="checkbox"/>	Date	10-19-01
Instrument	Serial Number		Department		County		
BREATHALYZER 900	8909014-002		FLORENCE TWP		BURLINGTON		
05 Cylinder Output	00300 Ampoule Control Number	05 Optical System	05 Balance Lost Motion	05 Instrument Temperature	101070 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results	
INSTRUMENT LOCATION: N/A							
Background Check			Effect	No Effect	Remarks		
N/A							
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE							
RADIO TRANSMISSION TESTING							
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS		
*6 TESTS WITHIN ACCEPTABLE TOLERANCES							
REMARKS: NONE							
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.							
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>							
OCTOBER 19, 2001 Date				 Signature			
				LAWRENCE P. WANCHTER 4603 Name and Badge Number (Print)			
LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE							

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE					Periodic Inspection <input type="checkbox"/>	Number <i>103-01</i>
					Other Inspection <input checked="" type="checkbox"/>	Date <i>080901</i>
Instrument <i>BREATHALYZER 900</i>		Serial Number <i>8909014-002</i>		Department <i>FLORENCE TWP</i>		County <i>BURLINGTON</i>
Cylinder Output <i>OK</i>	Ampoule Control Number <i>00300</i>	Optical System <i>OK</i>	Balance Lost Motion <i>OK</i>	Instrument Temperature <i>OK</i>	Sim. # <i>01070</i> .10	Instrument Test Percentage Results <i>*SEE BELOW</i>
INSTRUMENT LOCATION: <i>N/A</i>						
Background Check <i>N/A</i>			Effect	No Effect	Remarks	
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE						
RADIO TRANSMISSION TESTING						
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS	
<i>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</i>						
REMARKS: <i>(COMPLAINT INSTRUMENT NOT MAINTAINING PROPER TEMPERATURE RANGE. COMPLAINT IOWENED UNDESIGNED REPAIR) THERMOSTAT. THEN WAS ABLE TO (CONDUCT SIX (6) SIMULATOR TESTS WITHIN ACCEPTABLE TOLERANCES. THE EXISTENCE OF THIS MALFUNCTION WOULD MAKE ADHERANCE TO CHECK LIST IMPOSSIBLE.</i>						
The above instrument has been <input checked="" type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.						
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>						
<i>August 9, 2001</i> Date			<i>Lawrence P. Wright</i> Signature			
			<i>THE LAWRENCE P. WRIGHT 4663</i> Name and Badge Number (Print)			
LEGEND:						
N/E -- NO EFFECT		N/A -- NOT APPLICABLE				

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE				Periodic Inspection <input checked="" type="checkbox"/>	Number 102-01
				Other Inspection <input type="checkbox"/>	Date 07-11-01
Instrument BREATHANALYZER 900	Serial Number 8909014-002	Department FLORENCE TWPSP	County BURLINGTON		
Cylinder Output OK	Ampoule Control Number 00100 00300	Optical System OK	Balance Lost Motion OK	Instrument Temperature OK	Simulator Solution Percentage KT#00150 .10
					Instrument Test Percentage Results *SEE BELOW
INSTRUMENT LOCATION: N/A					
Background Check N/A		Effect	No Effect	Remarks	
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE					
RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
					
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					
REMARKS: NONE					
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.					
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>					
JULY 11, 2001 Date			 Signature		
			WACHTER LAWRENCE P WACHTER 4063 Name and Badge Number (Print)		
LEGEND:					
N/E - NO EFFECT		N/A - NOT APPLICABLE			

**STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE**

Periodic Inspection <input checked="checked" type="checkbox"/>	Number 101-01
Other Inspection <input type="checkbox"/>	Date 05-14-01

Instrument BREATHALYZER 900	Serial Number 899014-002	Department FLORENCE TWP	County BURLINGTON
--------------------------------	-----------------------------	----------------------------	----------------------

OK Cylinder Output	00100 00300 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	101.#00150 .10 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
-----------------------	--	----------------------	---------------------------	------------------------------	--	--

INSTRUMENT LOCATION: N/A

Background Check N/A	Effect	No Effect	Remarks
-------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS

* 6 TESTS WITHIN ACCEPTABLE TOLERANCES

REMARKS:
NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

May 14, 2001 Date


 Signature
LAWRENCE P. WACHTER 4663
 Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number 100-01
Other Inspection Date 02-23-01

Instrument BREATHALYZER 900 Serial Number 8909014-002 Department FLORENCE TWP County BURLINGTON

<u>OK</u> Cylinder Output	<u>00100</u> <u>00300</u> Ampoule Control Number	<u>OK</u> Optical System	<u>OK</u> Balance Lost Motion	<u>OK</u> Instrument Temperature	<u>N/A #00150</u> <u>.10</u> Simulator Solution Percentage	<u>*SEE BELOW</u> Instrument Test Percentage Results
------------------------------	--	-----------------------------	----------------------------------	-------------------------------------	--	---

INSTRUMENT LOCATION: N/A

Background Check <u>N/A</u>	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<u>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</u>					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

FEBRUARY 23, 2001
Date

Signature
THOMAS L. WACHTER 4663
Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

**STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE**

Periodic Inspection <input checked="" type="checkbox"/>	Number 79.01
Other Inspection <input type="checkbox"/>	Date 01-12-01

Instrument BREATHALYZER 900	Serial Number 8909014-002	Department FLORENCE TWP
Cylinder Output <i>OK</i>	Ampoule Control Number 00100 00300	Optical System <i>OK</i>
Balance Lost Motion <i>OK</i>	Instrument Temperature <i>OK</i>	Simulator Solution Percentage 100% ISO .10
Instrument Test Percentage Results *FSCC 2006W		County BURKINGTON

INSTRUMENT LOCATION: *N/A*

Background Check <i>N/A</i>	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE


RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<i>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</i>					

REMARKS: *NONE*

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

JANUARY 12, 2001
Date


Signature
T. LAWRENCE P. WRIGHT #603
Name and Badge Number (Print)

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE	Periodic Inspection <input checked="" type="checkbox"/>	Number 98-00
	Other Inspection <input type="checkbox"/>	Date 11-13-00

Instrument BREATHANALYZER 900	Serial Number 8909014-002	Department FLORENCE TWPSP	County BURLINGTON
----------------------------------	------------------------------	------------------------------	----------------------

Cylinder Output OK	Ampoule Control Number 00100 00998	Optical System OK	Balance Lost Motion OK	Instrument Temperature OK	Simulator Solution Percentage 157.00150 110	Instrument Test Percentage Results *SEE BELOW
-----------------------	--	----------------------	---------------------------	------------------------------	---	--

INSTRUMENT LOCATION: N/A

Background Check N/A	Effect	No Effect	Remarks
-------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: NONE

The above Instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

Signature: *Laurence P. Wachter*
 Name and Badge Number (Print): **TPA I LAURENCE P. WACHTER #663**

Date: November 13, 2000

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number **97-00**
Other Inspection Date **9-14-00**

Instrument **ALCANTERALYZER 900** Serial Number **8909014-002** Department **FLORENCE TOWNSHIP** County **BURLINGTON**

OK Cylinder Output	OK Ampoule Control Number 00998 9310701801	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	OK Simulator Solution Percentage 67.149810 .10	*-SEE BELOW Instrument Test Percentage Results
-----------------------	--	----------------------	---------------------------	------------------------------	--	---

INSTRUMENT LOCATION: **N/A**

Background Check **N/A** Effect No Effect Remarks

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING						
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS	
<i>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</i>						

REMARKS: **NONE**

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 1068, West Trenton, New Jersey 08628-0068."

September 14, 2000 Date

Lauren P. ... Signature
LAUREN P. ... 1663 Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number 96-00
 Other Inspection Date 6-13-00

Instrument BREATHALYZER 900 Serial Number 8107014-002 Department FLORENCE TWP. County BURLINGTON

OK Cylinder Output	00998 9310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	10.10 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
-----------------------	---	----------------------	---------------------------	------------------------------	--	--

INSTRUMENT LOCATION: N/A

Background Check	Effect	No Effect	Remarks
N/A			

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING


OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7088, West Trenton, New Jersey 08628-0068."

JUNE 13, 2000
Date


 Signature
 LAWRENCE P. WICHTER 4663
 Name and Badge Number (Print)

LEGEND: N/E — NO EFFECT N/A — NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE	Periodic Inspection <input checked="" type="checkbox"/>	Number 9400
	Other Inspection <input type="checkbox"/>	Date 1-10-00

Instrument BREATHALYZER 900	Serial Number 8909014-002	Department FLORENCE TWP	County BURLINGTON
OK	9310701501	OK	OK
OK	OK	OK	OK
Cylinder Output	Ampoule Control Number	Optical System	Balance Lost Motion
		Instrument Temperature	Simulator Solution Percentage
		18.799001	.10
			*SEE BELOW

INSTRUMENT LOCATION: N/A			
Background Check	Effect	No Effect	Remarks
N/A			

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

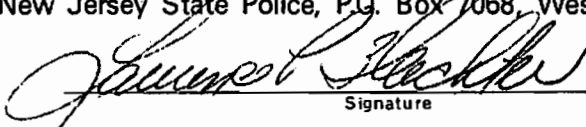
RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 1068, West Trenton, New Jersey 08628-0068."

JANUARY 10, 2000
Date


Signature
VINCENT P. HUNTER #663
Name and Badge Number (Print)

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE					Periodic Inspection <input checked="" type="checkbox"/>	Number 93-99
					Other Inspection <input type="checkbox"/>	Date 11-24-99
Instrument BREATHANALYZER 900	Serial Number 8909014-002	Department FLORENCE TOWNSHIP		County BURLINGTON		
OK Cylinder Output	9310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	101.4051 / 110 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
INSTRUMENT LOCATION: N/A						
Background Check		Effect	No Effect	Remarks		

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: **NONE**

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

Lawrence P. Wichter
 Signature

TP-I LAWRENCE P. WICHTER 4683
 Name and Badge Number (Print)

NOVEMBER 24, 1999
 Date

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number 97-99
Other Inspection Date 7.30.99

Instrument BREATHALYZER 900 Serial Number 890904-002 Department FLORENCE Twp 2 County BERKUNTON

OK Cylinder Output	9310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	LT # 99081 110 Simulator Solution Percentage	*SEE PCOW Instrument Test Percentage Results
-----------------------	--------------------------------------	----------------------	---------------------------	------------------------------	--	--

INSTRUMENT LOCATION: N/A

Background Check N/A
Effect No Effect
Remarks

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
*6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

JULY 30, 1999
Date

James P. ...
Signature
TRO. ILMURACK P. ... 4603
Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number **83-99**
 Other Inspection Date **3-1-99**

Instrument **BREATHALYZER 900** Serial Number **8909014-002** Department **FLORENCE TWP** County **BURLINGTON**

OK Cylinder Output	4310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	107.798180 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
------------------------------	---	-----------------------------	----------------------------------	-------------------------------------	--	---

INSTRUMENT LOCATION: **N/A**

Background Check	Effect	No Effect	Remarks
N/A			

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
*6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: **NONE**

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

March 1, 1999
 Date

[Signature]
 Signature
TRE LAURICER P. 1663
 Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection

Number 87-98

Other Inspection

Date 12-10-98

Instrument <u>ALCANTHALYZER 700</u>		Serial Number <u>89091014-002</u>		Department <u>FLORENCE TOWNSHIP</u>		County <u>BURLINGTON</u>	
<u>OK</u> Cylinder Output	<u>9310701501</u> Ampoule Control Number	<u>OK</u> Optical System	<u>OK</u> Balance Lost Motion	<u>OK</u> Instrument Temperature	<u>NOT # 70180 .10</u> Simulator Solution Percentage	<u>*SEE BELOW</u> Instrument Test Percentage Results	
INSTRUMENT LOCATION: <u>N/A</u>							
Background Check <u>N/A</u>		Effect	No Effect	Remarks			

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<u>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</u>					

REMARKS: (COMPLAINANT INSTRUMENT NOT HEATING TO PROPER TEMPERATURE RANGE. (COMPLAINANT FEELING REPAIRED THERMOSTAT THAN (CONDUCTED SIX(6) SIMULATOR TESTS WITHIN) ACCEPTABLE TOLERANCES THE EXISTENCE OF THIS MALFUNCTION WOULD MAKE ADHERENCE TO CHECK-LIST IMPOSSIBLE)

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

DECEMBER 10, 1998
Date

[Signature]
Signature
PROF. LAWRENCE P. WRIGHT 463
Name and Badge Number (Print)

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

STATE OF NEW JERSEY
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection

Number

86-98

Other Inspection

Date

10-7-98

Instrument: **BREATHALYZER 900** Serial Number: **8909014-002** Department: **FLORENCE TWP** County: **BURLINGTON**

OK Cylinder Output	9310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	101. #9090 .10 Simulator Solution Percentage	*SEE BLOW Instrument Test Percentage Results
-----------------------	--------------------------------------	----------------------	---------------------------	------------------------------	--	--

INSTRUMENT LOCATION: **N/A**

Background Check	Effect	No Effect	Remarks
N/A			

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: **NONE**

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

October 7, 1998
Date

Thomas P. L... 4653
Signature
THOMAS P. L... 4653
Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE

BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number 87-98
Other Inspection Date 6-30-98

Instrument BREATHALYZER 900 Serial Number 8909014-002 Department FLORENCE TOWNSHIP County BURLINGTON

<u>OK</u> Cylinder Output	<u>9310701501</u> Ampoule Control Number	<u>OK</u> Optical System	<u>OK</u> Balance Lost Motion	<u>OK</u> Instrument Temperature	<u>10. #92090</u> <u>.10</u> Simulator Solution Percentage	<u>*57.1</u> <u>57.10</u> Instrument Test Percentage Results
------------------------------	---	-----------------------------	----------------------------------	-------------------------------------	--	--

INSTRUMENT LOCATION: N/A
Background Check N/A Effect No Effect Remarks

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING


OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<u>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</u>					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

JUNE 30, 1998
Date


Signature
WILLIAM P. ARCHER 4883
Name and Badge Number (Print)

LEGEND: N/E -- NO EFFECT N/A -- NOT APPLICABLE

**STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE**

Periodic Inspection Number **83-98**
 Other Inspection Date **5-5-98**

Instrument: **BREATHALYZER 900** Serial Number: **8909014002** Department: **FLORENCE TWP** County: **BURLINGTON**

Cylinder Output: **OK** Ampoule Control Number: **9310701501**
 Optical System: **OK** Balance Lost Motion: **OK** Instrument Temperature: **OK**
 Simulator Solution Percentage: **107. # 98090 110** Instrument Test Percentage Results: ***SEE BELOW**

INSTRUMENT LOCATION: **N/A**

Background Check: **N/A** Effect: No Effect: Remarks:

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					


REMARKS: **NONE**

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 1068, West Trenton, New Jersey 08628-0068."

MAY 5, 1998 Date
[Signature] Signature
TRICIA LAURENCE PURWITER 4663 Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE				Periodic Inspection <input checked="" type="checkbox"/>	Number 82-98
				Other Inspection <input type="checkbox"/>	Date 3-24-98
Instrument BREATHALYZER 900		Serial Number 8909014-002	Department FLORENCE TWPSP		County BURLINGTON
Cylinder Output OK	Ampoule Control Number 9310701501	Optical System OK	Balance Lost Motion OK	Instrument Temperature OK	Simulator Solution Percentage 10T # 9090 .10
Instrument Test Percentage Results *SEE BELOW					
INSTRUMENT LOCATION: N/A					
Background Check N/A		Effect	No Effect	Remarks	
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE					
RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
*6 TESTS WITHIN ACCEPTABLE TOLERANCES					
REMARKS: NONE					
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.					
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>					
MARCH 24, 1998 Date		 Signature			
		TP-1 LAURENCE P. WACHTER #683 Name and Badge Number (Print)			
LEGEND:					
N/E — NO EFFECT		N/A — NOT APPLICABLE			

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE	Periodic Inspection <input checked="checked" type="checkbox"/>	Number 81-98
	Other Inspection <input type="checkbox"/>	Date 1-23-98

Instrument BREATHALYZER 900	Serial Number 8909014-002	Department FLORENCE TOWNSHIP
		County BURLINGTON

OK	9310701501	OK	OK	OK	OK	KT. #97060 .10	*SEE BELOW
Cylinder Output	Ampoule Control Number	Optical System	Balance Lost Motion	Instrument Temperature	Simulator Solution Percentage		Instrument Test Percentage Results

INSTRUMENT LOCATION: N/A			
Background Check N/A	Effect	No Effect	Remarks


ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."


 Signature

TP. LAURENCE P. WACHTER 4663
 Name and Badge Number (Print)

JANUARY 23, 1998
 Date

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

**STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE**

Periodic Inspection <input checked="" type="checkbox"/>	Number 80-97
Other Inspection <input type="checkbox"/>	Date 12-16-97

Instrument BREATHALYZER 900	Serial Number 8909014-002	Department FLORENCE TWSP	County BURLINGTON
---------------------------------------	-------------------------------------	------------------------------------	-----------------------------

OK Cylinder Output	9310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	107.#97060 .10 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
-----------------------	--------------------------------------	----------------------	---------------------------	------------------------------	--	--

INSTRUMENT LOCATION: **N/A**

Background Check N/A	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: **NONE**


The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

December 16, 1997
Date

[Signature]
Signature
TATI LAURANCE P. WALTER #683
Name and Badge Number (Print)

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE		Periodic Inspection <input checked="" type="checkbox"/>	Number 79-97		
		Other Inspection <input type="checkbox"/>	Date 11-6-97		
Instrument BREATHALYZER 900	Serial Number 8909014-008	Department FLORENCE TWP	County BURLINGTON		
OK Cylinder Output	9310701502 9310701501 Ampoules Control Number	OK Optical System	OK Balance Lost Motion		
OK Instrument Temperature	101. #97060 .10 Simulator Solution Percentage	OK Instrument Test Percentage Results	*SEE BELOW		
INSTRUMENT LOCATION: N/A					
Background Check		Effect	No Effect		
N/A			Remarks		
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE					
RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					
REMARKS: NONE					
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.					
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>					
NOVEMBER 6, 1997 Date			 Signature SP1 LAURENCE P. WACHTER 4603 Name and Badge Number (Print)		
LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE					

STATE OF NEW JERSEY
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection <input type="checkbox"/>	Number 78-97
Other Inspection <input checked="" type="checkbox"/>	Date 9-29-97

Instrument <i>BREATHALYZER 900</i>	Serial Number <i>8909014-002</i>	Department <i>FLORENCE TOWNSHIP</i>	County <i>BURLINGTON</i>
OK Cylinder Output	<i>9310701502</i> <i>9310701501</i> Ampoule Control Number	OK Optical System	OK Balance Lost Motion
		OK Instrument Temperature	<i>LOT. #97080</i> <i>110</i> Simulator Solution Percentage
			<i>*5% K</i> <i>BELOW</i> Instrument Test Percentage Results

INSTRUMENT LOCATION: *N/A*

Background Check <i>N/A</i>	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<i>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</i>					

REMARKS: *COMPLAINT OF INSTRUMENT NOT HEATING TO PROPER TEMPERATURE RANGE. COMPLAINT FOUNDED. REPLACED THERMOSTAT. CONDUCTED 6 SIMULATOR TESTS WITHIN ACCEPTABLE TOLERANCES. THE EXISTENCE OF THIS MALFUNCTION WOULD MAKE ADHERENCE TO CHECK-LIST IMPOSSIBLE.*

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

September 29, 1997
Date

Lawrence P. Wauter
Signature
L.P. LAURENCE P. WAUTER #653
Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection <input checked="" type="checkbox"/>	Number 77-97
Other Inspection <input type="checkbox"/>	Date 9-3-97

Instrument BREATHALYZER 900	Serial Number 8909014-002	Department FLORENCE TWP	County BURLINGTON
---------------------------------------	-------------------------------------	-----------------------------------	-----------------------------

OK Cylinder Output	9310701502 9310701501 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	101. #96250 .10 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
-----------------------	--	----------------------	---------------------------	------------------------------	---	--

INSTRUMENT LOCATION: **N/A**

Background Check N/A	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					

REMARKS: **NONE**

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7088, West Trenton, New Jersey 08628-0068."

SEPTEMBER 3, 1997
Date

Laurence P. Wachter
Signature
TPAI LAURENCE P. WACHTER 4653
Name and Badge Number (Print)

LEGEND: N/E — NO EFFECT N/A — NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection	<input checked="" type="checkbox"/>	Number	<u>75-97</u>
Other Inspection	<input type="checkbox"/>	Date	<u>6-19-97</u>

Instrument	<u>BRELATHEANALYZER 900</u>	Serial Number	<u>8909014-002</u>	Department	<u>FLORENCE TWPSP</u>	County	<u>BURLINGTON</u>
Cylinder Output	<u>OK</u>	Ampoule Control Number	<u>9310701502</u>	Optical System	<u>OK</u>	Balance Lost Motion	<u>OK</u>
				Instrument Temperature	<u>OK</u>	Simulator Solution Percentage	<u>10T. #96250 *52% .10 BELOW</u>
INSTRUMENT LOCATION: <u>N/A</u>							
Background Check		Effect	No Effect	Remarks			
<u>N/A</u>							

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<u>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</u>					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.


"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 1068, West Trenton, New Jersey 08628-0068."

JUNE 19, 1997
Date

Lawrence P. Anichter
Signature
LPT-I LAURENCE P. ANICHTER 4603
Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE					Periodic Inspection <input type="checkbox"/>	Number <u>73-97</u>
					Other Inspection <input checked="" type="checkbox"/>	Date <u>3-31-97</u>
Instrument <u>BREATHALYZER 900</u>	Serial Number <u>8909014-002</u>	Department <u>FLORENCE TWP</u>		County <u>BURLINGTON</u>		
OK Cylinder Output	<u>931070502</u> Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	<u>1ST #96250</u> <u>.10</u> Simulator Solution Percentage	<u>*SEE BELOW</u> Instrument Test Percentage Results
INSTRUMENT LOCATION: <u>N/A</u>						
Background Check <u>N/A</u>	Effect	No Effect	Remarks			
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE						
RADIO TRANSMISSION TESTING						
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS	
<u>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</u>						
REMARKS: <u>COMPLAINT OF IMPROPER READINGS. COMPLAINT UNFOUNDED UNDETECTED CONDUCTED MULTIPLE SIMULATOR TESTS WITH READINGS OBTAINED WITHIN ACCEPTABLE TOLERANCES. UNABLE TO DUPLICATE COMPLAINT.</u>						
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.						
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>						
<u>MARCH 31, 1997</u> Date		<u>Lawrence P. Hatcher</u> Signature				
		<u>TRT LAWRENCE P. WINTER 465</u> Name and Badge Number (Print)				
LEGEND:						
N/E - NO EFFECT			N/A - NOT APPLICABLE			

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE					Periodic Inspection <input checked="" type="checkbox"/>	Number 72-97
					Other Inspection <input type="checkbox"/>	Date 2-26-97
Instrument BREATHALYZER 900		Serial Number 8909019-002		Department FLORENCE TOWNSHIP		County BURLINGTON
OK Cylinder Output	9310701502 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	101.96250 .10 Simulator Solution Percentage	*SEE BELOW Instrument Test Percentage Results
INSTRUMENT LOCATION: N/A						
Background Check N/A			Effect	No Effect	Remarks	
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE						
RADIO TRANSMISSION TESTING						
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS	
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES						
REMARKS: NONE						
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.						
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>						
FEBRUARY 26, 1997 Date				 Signature		
				TR. J. LAURENCE P. WACHTER 4663 Name and Badge Number (Print)		
LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE						

STATE OF NEW JERSEY
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number 71-97
 Other Inspection Date 1-17-97

Instrument BREATHALYZER 900 Serial Number 890901A-002 Department FLORENCE TWP County BURLINGTON

<u>OK</u> Cylinder Output	<u>9310701502</u> Ampoule Control Number	<u>OK</u> Optical System	<u>OK</u> Balance Lost Motion	<u>OK</u> Instrument Temperature	<u>LOT. #96080 .10</u> Simulator Solution Percentage	<u>*SEE BELOW</u> Instrument Test Percentage Results
------------------------------	---	-----------------------------	----------------------------------	-------------------------------------	---	---

INSTRUMENT LOCATION: N/A

Background Check N/A Effect No Effect Remarks

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
<u>* 6 TESTS WITHIN ACCEPTABLE TOLERANCES</u>					

REMARKS: NONE


The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

JANUARY 17, 1997
 Date

Laurence P. Wachter
 Signature
TRAIL LAURENCE P. WACHTER 4063
 Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE				Periodic Inspection <input checked="" type="checkbox"/>	Number 70-96
				Other Inspection <input type="checkbox"/>	Date 12-6-96
Instrument BREATH-ANALYZER 900		Serial Number 8909014-002		Department FLORENCE TWP 12	
County BURLINGTON					
OK Cylinder Output	9310701502 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	KT.#76080 .10 Simulator Solution Percentage
*SEE BELOW Instrument Test Percentage Results					
INSTRUMENT LOCATION: N/A					
Background Check N/A		Effect	No Effect	Remarks	
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE					
RADIO TRANSMISSION TESTING					
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCES					
REMARKS: NONE					
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.					
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>					
DECEMBER 6, 1996 Date			 Signature 4663		
			LAURENCE P. WINTER Name and Badge Number (Print)		
LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE					

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection <input checked="checked" type="checkbox"/>	Number <i>6796</i>
Other Inspection <input checked="checked" type="checkbox"/>	Date <i>08-19-96</i>

Instrument <i>BREATHALYZER 900</i>	Serial Number <i>8909014002</i>	Department <i>FLORHAM TWP</i>	County <i>BERGEN</i>
---------------------------------------	------------------------------------	----------------------------------	-------------------------

Cylinder Output <i>O.K.</i>	Ampoule Control Number <i>9310701503</i>	Optical System <i>O.K.</i>	Balance Lost Motion <i>O.K.</i>	Instrument Temperature <i>O.K.</i>	Simulator Solution Percentage <i>LOT # 96080 .10</i>	Instrument Test Percentage Results <i>* SEE BELOW</i>
--------------------------------	---	-------------------------------	------------------------------------	---------------------------------------	---	--

INSTRUMENT LOCATION: *N/A*

Background Check <i>N/A</i>	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS

* *6 TESTS WITHIN ACCEPTABLE TOLERANCE*

REMARKS: *INSPECTION REVEALED VERY LOW CYLINDER OUTPUT. FURTHER INSPECTION REVEALED A CRACKED INLET HOSE. SAME REPLACED THE EXISTENCE OF THIS MALFUNCTION WOULD PRODUCE LOW TEST RESULTS.*

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

AUGUST 19, 1996
Date

Craig S. Potter
Signature
771 C.S. POTTER - 4096
Name and Badge Number (Print)

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

**STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE**

Periodic Inspection <input checked="" type="checkbox"/>	Number <i>6696</i>
Other Inspection <input type="checkbox"/>	Date <i>07/19/96</i>

Instrument <i>RADIATION 900</i>	Serial Number <i>8909014-002</i>	Department <i>FLORENCE TWP</i>	County <i>Burlington</i>
------------------------------------	-------------------------------------	-----------------------------------	-----------------------------

Cylinder Output <i>OK</i>	Ampoule Control Number <i>9710701503</i>	Optical System <i>OK</i>	Balance Lost Motion <i>OK</i>	Instrument Temperature <i>OK</i>	Simulator Solution Percentage <i>LOT-96080 10</i>	Instrument Test Percentage Results <i>* 5.7 18.00</i>
------------------------------	---	-----------------------------	----------------------------------	-------------------------------------	--	--

INSTRUMENT LOCATION: *N/A*

Background Check <i>N/A</i>	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS

* 6 TESTS WITHIN ACCEPTABLE TOLERANCE

REMARKS: *none*

The above instrument has been repaired and inspected and found to be in satisfactory working condition.


"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

July 19, 1996
Date

[Signature]
Signature

771101001
Name and Badge Number (Print)

LEGEND: N/E – NO EFFECT N/A – NOT APPLICABLE

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE					Periodic Inspection <input checked="" type="checkbox"/>	Number 6596
					Other Inspection <input checked="" type="checkbox"/>	Date 05/31/96
Instrument <i>BILATERALYZER 900</i>		Serial Number <i>8909014-002</i>		Department <i>FLORHAM TWP</i>		County <i>BURLINGAME</i>
<i>OK</i> Cylinder Output	<i>9310701502</i> Ampoule Control Number	<i>OK</i> Optical System	<i>OK</i> Balance Lost Motion	<i>OK</i> Instrument Temperature	<i>LOT#95402 .10</i> Simulator Solution Percentage	<i>5.5 18.200</i> Instrument Test Percentage Results
INSTRUMENT LOCATION: <i>N/A</i>						
Background Check <i>N/A</i>		Effect	No Effect	Remarks		
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE						
RADIO TRANSMISSION TESTING						
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS	
<i>* 6 TESTS WITHIN ACCEPTABLE TOLERANCE</i>						
REMARKS: <i>COMPLAINT TEMPERATURE NOT COMING UP. INSPECTION REVEALED JUNCTION PLUG DISCONNECTED. NO POWER WAS BEING SUPPLIED JUNCTION PLUG RECONNECTED. THE EXISTENCE OF THIS MALFUNCTION WOULD MAKE ADHERENCE TO THE CHECK-OFF LIST IMPOSSIBLE.</i>						
The above instrument has been <input checked="" type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.						
<p>"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."</p>						
<i>MAY 31 1996</i> Date				 Signature		
				<i>THOMAS C. SMITH 2016</i> Name and Badge Number (Print)		
LEGEND:						
N/E — NO EFFECT			N/A — NOT APPLICABLE			

STATE OF NEW JERSEY DEPARTMENT OF LAW AND PUBLIC SAFETY DIVISION OF STATE POLICE BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE						Periodic Inspection <input checked="" type="checkbox"/>	Number <i>6496</i>
						Other Inspection <input type="checkbox"/>	Date <i>0430-96</i>
Instrument <i>BREATHALYZER 900</i>		Serial Number <i>8909014-002</i>		Department <i>FLORENCE TWP</i>		County <i>Burlington</i>	
<i>OK</i> Cylinder Output	<i>00892</i> <i>9310701502</i> Ampoule Control Number	<i>O.K.</i> Optical System	<i>O.K.</i> Balance Lost Motion	<i>O.K.</i> Instrument Temperature	<i>LOT# 95402</i> <i>10</i> Simulator Solution Percentage	<i>*5% BLOW</i> Instrument Test Percentage Results	
INSTRUMENT LOCATION: <i>N/A</i>							
Background Check <i>N/A</i>			Effect	No Effect	Remarks		
<input checked="" type="checkbox"/> ABOVE INSTRUMENT IS NOT RFI SENSITIVE							
RADIO TRANSMISSION TESTING							
OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS		
<i>* 6 TESTS WITHIN ACCEPTABLE TOLERANCE.</i>							
REMARKS: <i>NONE</i>							
The above instrument has been <input type="checkbox"/> repaired and <input checked="" type="checkbox"/> inspected and found to be in satisfactory working condition.							
<p> "I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068." </p>							
<i>APRIL 30, 1996</i> Date				<i>Lucy S. Potte</i> Signature			
				<i>APRIL 30, 1996 44096</i> Name and Badge Number (Print)			
LEGEND:							
N/E — NO EFFECT			N/A — NOT APPLICABLE				

**STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE**

Periodic Inspection <input checked="" type="checkbox"/>	Number <i>6396</i>
Other Inspection <input type="checkbox"/>	Date <i>03-13-96</i>

Instrument <i>BREATHALYZER 900</i>	Serial Number <i>8909014-002</i>	Department <i>FLORHAM TWP</i>	County <i>BURLINGTON</i>
---------------------------------------	-------------------------------------	----------------------------------	-----------------------------

<i>O.K.</i> Cylinder Output	<i>00892</i> Ampoule Control Number	<i>O.K.</i> Optical System	<i>O.K.</i> Balance Lost Motion	<i>O.K.</i> Instrument Temperature	<i>LOT# 95402</i> <i>.10</i> Simulator Solution Percentage	<i>* 5% BLOW</i> Instrument Test Percentage Results
--------------------------------	--	-------------------------------	------------------------------------	---------------------------------------	--	--

INSTRUMENT LOCATION: *N/A*

Background Check <i>N/A</i>	Effect	No Effect	Remarks
--------------------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS

** 6 TESTS WITHIN ACCEPTABLE TOLERANCE.*

REMARKS:
NOTE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

MARCH 13, 1996
Date

Greg S. Potter
Signature
TP2 ICS Potter - 4096
Name and Badge Number (Print)

LEGEND: N/E - NO EFFECT N/A - NOT APPLICABLE

STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENT INSPECTION CERTIFICATE

Periodic Inspection Number 62-96

Other Inspection Date 2-20-96

Instrument BREATHALYZER 90L Serial Number 8909014-002 Department FLORENCE TWP County BURLINGTON

OK Cylinder Output	00892 Ampoule Control Number	OK Optical System	OK Balance Lost Motion	OK Instrument Temperature	100% F 95.286 Simulator Solution Percentage	* SE 82.14 Instrument Test Percentage Results
-----------------------	---------------------------------	----------------------	---------------------------	------------------------------	--	---

INSTRUMENT LOCATION: NA

Background Check NA	Effect	No Effect	Remarks
---------------------	--------	-----------	---------

ABOVE INSTRUMENT IS NOT RFI SENSITIVE

RADIO TRANSMISSION TESTING

OPERATING FREQUENCY	CHANNEL DESIGNATION	BASE STATION	MOBILE (Distance)	PORTABLE (Distance)	REMARKS
* 6 TESTS WITHIN ACCEPTABLE TOLERANCE					

REMARKS: NONE

The above instrument has been repaired and inspected and found to be in satisfactory working condition.

"I am a Breath Test Coordinator Instructor, empowered by the Attorney General of the State of New Jersey, pursuant to the provisions of P. L. 1966 c. 142 S3 as amended (C. 39:4-50.3) and rules and regulations adopted thereunder, to perform inspection and maintenance of approved instruments for performing chemical analysis of a person's breath. I hereby affirm that I have inspected the approved instrument designated on this certificate. I further attest that this document contains a true, accurate and complete record of the inspection and maintenance performed herein, including random sample testing of ampoules used in the operation of this approved instrument as is evidenced by the ampoules control number (s) designated on this certificate. The original document of this inspection is on file at Division Headquarters of the New Jersey State Police, P.O. Box 7068, West Trenton, New Jersey 08628-0068."

FEBRUARY 20, 1996
Date

Kevin M. Johnson
Signature
PA II KEVIN M JOHNSON # 400
Name and Badge Number (Print)

LEGEND:

N/E — NO EFFECT

N/A — NOT APPLICABLE