

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00704 **Calib. Date:** 06/12/2014 **Calib. No.:** 00024
Certification File No.: 00705 **Cert. Date:** 06/12/2014 **Cert. No.:** 00017
Linearity File No.: 00706 **Lin. Date:** 06/12/2014 **Lin. No.:** 00017
Solution File No.: 00738 **Soln. Date:** 10/10/2014 **Soln. No.:** 00157
Sequential File No.: 00738 **File Date:** 10/10/2014

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 04/29/2016
Solution Control Lot: 14D129 **Bottle No.:** 0496

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:49D		
Control 1 EC	0.100%	18:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:50D		
Control 2 EC	0.099%	18:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:51D		
Control 3 EC	0.099%	18:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI

First Name: MAURO

M1: J

Signature: 

Badge No.: 4025

Date: 10/10/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00704	Calib. Date: 06/12/2014
Certification File No.:	00705	Calib. No.: 00024
Linearity File No.:	00706	Cert. Date: 06/12/2014
Solution File No.:	00729	Cert. No.: 00017
Sequential File No.:	00729	Lin. Date: 06/12/2014
		Lin. No.: 00017
		Soln. Date: 09/05/2014
		Soln. No.: 00156
		File Date: 09/05/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1097

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:28D		
Control 1 EC	0.098%	08:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	08:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:30D		
Control 2 EC	0.097%	08:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:31D		
Control 3 EC	0.098%	08:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: _____



Badge No.: 4029

Date: 09/05/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00704	Calib. Date:	06/12/2014
Certification File No.:	00705	Cert. Date:	06/12/2014
Linearity File No.:	00706	Lin. Date:	06/12/2014
Solution File No.:	00722	Soln. Date:	08/19/2014
Sequential File No.:	00722	File Date:	08/19/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	12K108	Expires:	11/05/2014
		Bottle No.:	1096

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:59D		
Control 1 EC	0.096%	09:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	09:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:01D		
Control 2 EC	0.097%	09:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:02D		
Control 3 EC	0.096%	09:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: _____

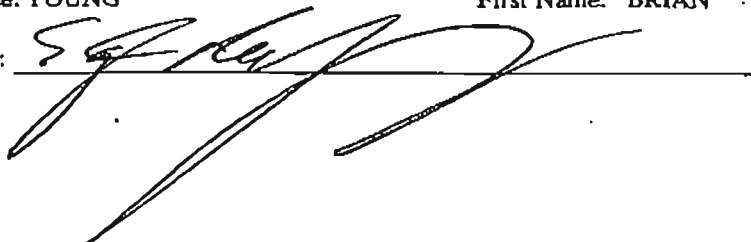

Badge No.: 4034

Date: 08/19/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00704	Calib. Date: 06/12/2014
Certification File No.:	00705	Cert. No.: 00024
Linearity File No.:	00706	Cert. No.: 00017
Solution File No.:	00717	Lin. Date: 06/12/2014
Sequential File No.:	00717	Lin. No.: 00017
		Soln. No.: 00154
		Soln. Date: 07/19/2014
		File Date: 07/19/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1091

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:53D		
Control 1 EC	0.099%	16:53D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	16:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:54D		
Control 2 EC	0.097%	16:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:55D		
Control 3 EC	0.097%	16:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	16:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____



Badge No.: 4026

Date: 07/19/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C		Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		Calib. No.: 00024
Calibration File No.:	00704	Calib. Date: 06/12/2014	Cert. No.: 00017
Certification File No.:	00705	Cert. Date: 06/12/2014	Lin. No.: 00017
Linearity File No.:	00706	Lin. Date: 06/12/2014	Soln. No.: 00153
Solution File No.:	00711	Soln. Date: 06/22/2014	
Sequential File No.:	00711	File Date: 06/22/2014	

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUM S3-0222
Control Solution %:	0.100%		Expires: 11/05/2014
Solution Control Lot:	12K108		Bottle No.: 1087

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:30D		
Control 1 EC	0.098%	07:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:31D		
Control 2 EC	0.096%	07:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	07:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:32D		
Control 3 EC	0.097%	07:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____



Badge No.: 4025

Date: 06/22/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00655	Calib. Date:	12/17/2013
Certification File No.:	00656	Cert. No.:	00023
Linearity File No.:	00657	Cert. Date:	12/17/2013
Solution File No.:	00699	Lin. No.:	00016
Sequential File No.:	00699	Soln. Date:	05/25/2014
		Soln. No.:	00151
		File Date:	05/25/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	12K108	Expires:	11/05/2014
		Bottle No.:	1086

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:37D		
Control 1 EC	0.097%	04:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	04:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:38D		
Control 2 EC	0.097%	04:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	04:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:39D		
Control 3 EC	0.097%	04:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	04:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:41D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

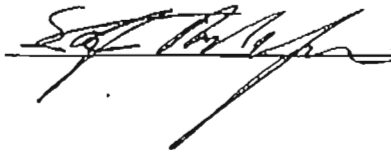Signature: 

Badge No.: 4034

Date: 05/25/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00023
Calibration File No.:	00655	Cert. Date:	12/17/2013
Certification File No.:	00656	Lin. Date:	12/17/2013
Linearity File No.:	00657	Soln. Date:	03/22/2014
Solution File No.:	00692	File Date:	03/22/2014
Sequential File No.:	00692		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	12K108	Expires:	11/05/2014
		Bottle No.:	1081

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:54S		
Control 1 EC	0.098%	01:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:56S		
Control 2 EC	0.096%	01:56S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:57S		
Control 3 EC	0.096%	01:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: _____



Badge No.: 4034

Date: 03/22/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00655	Calib. Date:	12/17/2013
Certification File No.:	00656	Cert. Date:	12/17/2013
Linearity File No.:	00657	Lin. Date:	12/17/2013
Solution File No.:	00686	Soln. Date:	02/25/2014
Sequential File No.:	00686	File Date:	02/25/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%		
Solution Control Lot:	12K108	Serial No.:	DDUM S3-0225
		Expires:	11/05/2014
		Bottle No.:	1099

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:47S		
Control 1 EC	0.099%	14:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:48S		
Control 2 EC	0.097%	14:49S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:50S		
Control 3 EC	0.097%	14:50S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	14:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____

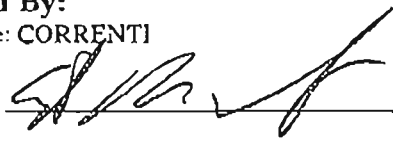

Badge No.: 4025

Date: 02/25/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00023
Calibration File No.:	00655	Cert. Date:	12/17/2013
Certification File No.:	00656	Calib. No.:	00016
Linearity File No.:	00657	Cert. No.:	00016
Solution File No.:	00681	Lin. No.:	00016
Sequential File No.:	00681	Soln. No.:	00147
		File Date:	02/11/2014

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%	Expires:	11/05/2014	Bottle No.:	1082
Solution Control Lot:	12K108				

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:08S		
Control 1 EC	0.099%	22:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	22:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:09S		
Control 2 EC	0.098%	22:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	22:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:11S		
Control 3 EC	0.098%	22:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____



Badge No.: 4025

Date: 02/11/2014