

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00027
Calibration File No.:	00818	Cert. Date:	10/13/2015
Certification File No.:	00819	Lin. Date:	10/13/2015
Linearity File No.:	00820	Soln. Date:	12/09/2015
Solution File No.:	00830	File Date:	12/09/2015
Sequential File No.:	00830		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM.S3-0225
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	0489

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:00S		
Control 1 EC	0.101%	03:00S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.103%	03:00S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:01S		
Control 2 EC	0.101%	03:02S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.103%	03:02S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:02S		
Control 3 EC	0.101%	03:03S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	03:03S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCULLY


First Name: DANIEL

MI: S

Signature: 

Badge No.: 4065

Date: 12/09/2015

Signature: 

Badge No.: 4065

Date: 12/09/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00818	Calib. Date:	10/13/2015
Certification File No.:	00819	Cert. Date:	10/13/2015
Linearity File No.:	00820	Lin. Date:	10/13/2015
Solution File No.:	00829	Soln. Date:	12/09/2015
Sequential File No.:	00829	File Date:	12/09/2015

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	04/29/2016
Solution Control Lot:	14D129			Bottle No.:	0484

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:22S		
Control 1 EC	-.---%	01:22S	23.0°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	01:22S	23.0°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCULLY

First Name: DANIEL

MI: S


Signature: _____



Badge No.: 4065

Date: 12/09/2015

Signature: _____



Badge No.: 4065

Date: 12/09/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00818	Calib. Date:	10/13/2015
Certification File No.:	00819	Cert. No.:	00027
Linearity File No.:	00820	Cert. Date:	10/13/2015
Solution File No.:	00823	Lin. No.:	00020
Sequential File No.:	00823	Soln. Date:	11/13/2015
		Soln. No.:	00173
		File Date:	11/13/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	0487

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:17S		
Control 1 EC	0.101%	00:18S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	00:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:19S		
Control 2 EC	0.100%	00:19S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	00:19S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:20S		
Control 3 EC	0.100%	00:21S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	00:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____



Badge No.: 4041


Date: 11/13/2015

Signature: _____



Date: 11/13/2015

Signature: _____



Date: 11/13/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00780	Calib. No.: 00026
Certification File No.:	00781	Cert. No.: 00019
Linearity File No.:	00782	Lin. No.: 00019
Solution File No.:	00806	Soln. No.: 00170
Sequential File No.:	00806	File Date: 08/20/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	14D129	Expires: 04/29/2016
		Bottle No.: 0488

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:48D		
Control 1 EC	0.099%	00:48D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:48D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:49D		
Control 2 EC	0.099%	00:50D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:50D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:50D		
Control 3 EC	0.099%	00:51D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	00:51D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J


Signature: _____

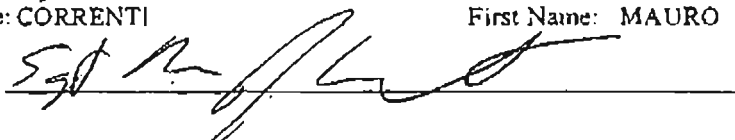

Badge No.: 4025

Date: 08/20/2015


Signature: _____

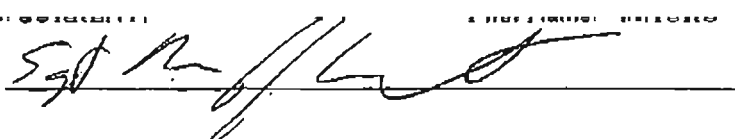

Badge No.: 4025

Date: 08/20/2015

Signature: _____

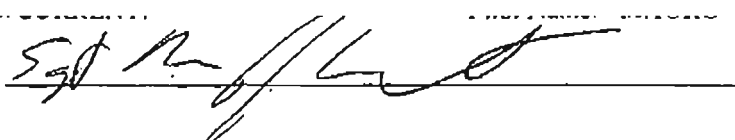

Badge No.: 4025

Date: 08/20/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00780	Calib. Date: 04/21/2015
Certification File No.:	00781	Calib. No.: 00026
Linearity File No.:	00782	Cert. Date: 04/21/2015
Solution File No.:	00801	Cert. No.: 00019
Sequential File No.:	00801	Lin. Date: 04/21/2015
		Lin. No.: 00019
		Soln. Date: 07/23/2015
		Soln. No.: 00169
		File Date: 07/23/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	14D129	Expires: 04/29/2016
		Bottle No.: 0477

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:28D		
Control 1 EC	0.101%	02:29D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	02:29D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:30D		
Control 2 EC	0.100%	02:30D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:30D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:31D		
Control 3 EC	0.100%	02:32D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:32D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____



Badge No.: 4041

Date: 07/23/2015

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Solution File No.:	00801	Soln. Date: 07/23/2015
Sequential File No.:	00801	Soln. No.: 00169
		File Date: 07/23/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	14D129	Expires: 04/29/2016
		Bottle No.: 0477

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:28D		

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00780	Calib. Date:	04/21/2015
Certification File No.:	00781	Cert. Date:	04/21/2015
Linearity File No.:	00782	Lin. Date:	04/21/2015
Solution File No.:	00796	Soln. Date:	06/21/2015
Sequential File No.:	00796	File Date:	06/21/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	0478

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:27D		
Control 1 EC	0.099%	23:28D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:28D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:29D		
Control 2 EC	0.099%	23:29D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:29D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:30D		
Control 3 EC	0.098%	23:31D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:31D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:31D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI


First Name: MAURO

MI: J

Signature: 


Badge No.: 4025

Date: 06/21/2015

Signature: 

Badge No.: 4025

Date: 06/21/2015

Signature: 

Badge No.: 4025

Date: 06/21/2015

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00749	Calib. Date: 12/08/2014
Certification File No.:	00750	Cert. No.: 00025
Linearity File No.:	00751	Cert. Date: 12/08/2014
Solution File No.:	00778	Lin. No.: 00018
Sequential File No.:	00778	Soln. No.: 00165
		File Date: 03/29/2015

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUM S3-0222
Control Solution %:	0.100%		Expires: 04/29/2016
Solution Control Lot:	14D129		Bottle No.: 0498

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:01S		
Control 1 EC	0.100%	15:01S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:02S		
Control 2 EC	0.098%	15:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:04S		
Control 3 EC	0.099%	15:04S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SHAFER

First Name: JASON

MI: A


Signature: _____

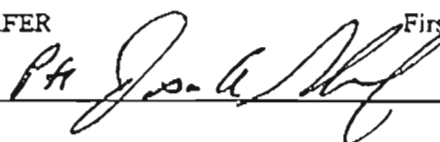

Badge No.: 4045

Date: 03/29/2015


Signature: _____



Badge No.: 4045

Date: 03/29/2015

Signature: _____



Badge No.: 4045

Date: 03/29/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00025
Calibration File No.:	00749	Cert. Date:	12/08/2014
Certification File No.:	00750	Lin. Date:	12/08/2014
Linearity File No.:	00751	Soln. Date:	02/28/2015
Solution File No.:	00768	File Date:	02/28/2015
Sequential File No.:	00768		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	0497

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:05S		
Control 1 EC	0.100%	04:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:07S		
Control 2 EC	0.098%	04:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:08S		
Control 3 EC	0.099%	04:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:10S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: 

Badge No.: 4034

Date: 02/28/2015

Solution File No.:	00768	Soln. Date:	02/28/2015	Soln. No.:	00763
Sequential File No.:	00768	File Date:	02/28/2015		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0222
Control Solution %:	0.100%			Expires:	04/29/2016
Solution Control Lot:	14D129			Bottle No.:	0497

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:05S		
Control 1 EC	0.100%	04:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:06S	34.0°C	*** TEST PASSED ***

Calibrating Unit New Standard Solution Report

Equipment	Alcores 7110 MKII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00749	Calib. Date: 12/08/2014
Certification File No.:	00750	Cert. Date: 12/08/2014
Linearity File No.:	00751	Lin. Date: 12/08/2014
Solution File No.:	00761	Soln. Date: 02/03/2015
Sequential File No.:	00761	File Date: 02/03/2015

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUM S3-0222
Control Solution %:	0.100%		Expires: 04/29/2016
Solution Control Lot:	14D129		Bottle No.: 0483

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:09S		
Control 1 EC	0.100%	02:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	02:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:10S		
Control 2 EC	0.100%	02:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	02:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:12S		
Control 3 EC	0.100%	02:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	02:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcores 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GREENBERG

First Name: JONATHAN

MI: M


Signature:

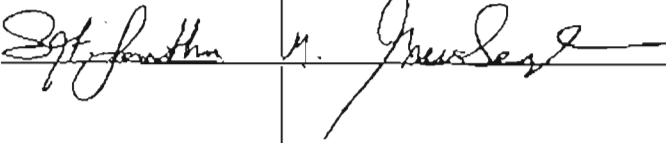

Badge No.: 4031

Date: 02/03/2015

Signature:

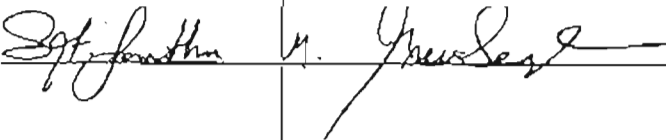

Badge No.: 4031

Date: 02/03/2015

Solution File No.: 00761
Sequential File No.: 00761

Soln. Date: 02/03/2015
File Date: 02/03/2015

Soln. No.: 00162

Calibrating Unit: **WET**
Control Solution %: 0.100%

Model No.: CU-34

Serial No.: DDUM S3-0222
Expires: 04/29/2016