

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00561	Calib. Date: 08/22/2012
Certification File No.:	00562	Calib. No.: 00020
Linearity File No.:	00563	Cert. Date: 08/22/2012
Solution File No.:	00587	Cert. No.: 00013
Sequential File No.:	00587	Lin. Date: 08/22/2012
		Lin. No.: 00013
		Soln. Date: 11/28/2012
		Soln. No.: 00130
		File Date: 11/28/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	11A085	Expires: 01/20/2013
		Boule No.: 0666

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:09S		
Control 1 EC	0.102%	04:10S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:10S		
Control 2 EC	0.101%	04:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	04:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:12S		
Control 3 EC	0.101%	04:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 11/28/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00561	Calib. Date: 08/22/2012
Certification File No.:	00562	Calib. No.: 00020
Linearity File No.:	00563	Cert. Date: 08/22/2012
Solution File No.:	00584	Cert. No.: 00013
Sequential File No.:	00584	Lin. Date: 08/22/2012
		Lin. No.: 00013
		Soln. Date: 10/22/2012
		Soln. No.: 00129
		File Date: 10/22/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0663

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:20D		
Control 1 EC	0.102%	21:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	21:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:21D		
Control 2 EC	0.101%	21:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	21:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:22D		
Control 3 EC	0.101%	21:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 10/22/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00561	Calib. Date:	08/22/2012
Certification File No.:	00562	Cert. Date:	08/22/2012
Linearity File No.:	00563	Lin. Date:	08/22/2012
Solution File No.:	00577	Soln. Date:	09/21/2012
Sequential File No.:	00577	File Date:	09/21/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	11A085	Expires:	01/20/2013
		Bottle No.:	0668

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:24D		
Control 1 EC	0.100%	17:25D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:26D		
Control 2 EC	0.100%	17:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:27D		
Control 3 EC	0.099%	17:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:28D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

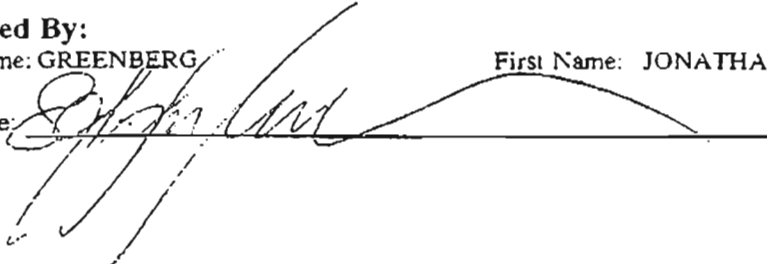Signature: 

Badge No.: 4031

Date: 09/21/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.		
<b>Calibration File No.:</b>	00529	<b>Calib. Date:</b>	02/23/2012
<b>Certification File No.:</b>	00530	<b>Cert. No.:</b>	00019
<b>Linearity File No.:</b>	00531	<b>Cert. Date:</b>	02/23/2012
<b>Solution File No.:</b>	00558	<b>Lin. No.:</b>	00012
<b>Sequential File No.:</b>	00558	<b>Soln. Date:</b>	08/03/2012
		<b>Soln. No.:</b>	00125
		<b>File Date:</b>	08/03/2012
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0225
<b>Solution Control Lot:</b>	11A085	<b>Expires:</b>	01/20/2013
		<b>Bottle No.:</b>	0667

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:35D		
Control 1 EC	0.099%	03:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:36D		
Control 2 EC	0.099%	03:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:37D		
Control 3 EC	0.099%	03:38D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 08/03/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00019
Calibration File No.:	00529	Cert. Date:	02/23/2012
Certification File No.:	00530	Lin. Date:	02/23/2012
Linearity File No.:	00531	Soln. Date:	07/04/2012
Solution File No.:	00552	File Date:	07/04/2012
Sequential File No.:	00552		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	01/20/2013
Solution Control Lot:	11A085			Bottle No.:	6520

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:11D		
Control 1 EC	0.100%	12:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:12D		
Control 2 EC	0.099%	12:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:14D		
Control 3 EC	0.099%	12:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature:

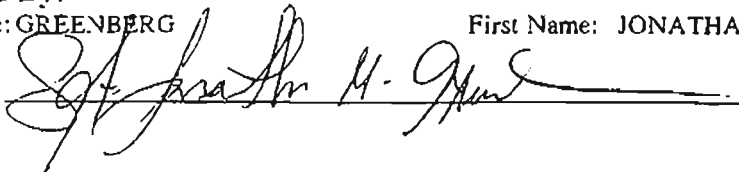

Badge No.: 4031

Date: 07/04/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00529	Calib. Date: 02/23/2012
Certification File No.:	00530	Calib. No.: 00019
Linearity File No.:	00531	Cert. Date: 02/23/2012
Solution File No.:	00545	Cert. No.: 00012
Sequential File No.:	00545	Lin. Date: 02/23/2012
		Lin. No.: 00012
		Soln. Date: 06/01/2012
		Soln. No.: 00123
		File Date: 06/01/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0658

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:06D		
Control 1 EC	0.098%	01:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	01:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:07D		
Control 2 EC	0.097%	01:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:09D		
Control 3 EC	0.098%	01:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	01:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: PANARO

First Name: BRIAN

MI: K

Signature: *Brian K. Panaro*

Badge No.: 4032

Date: 06/01/2012

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00529 **Callb. Date:** 02/23/2012 **Calib. No.:** 00019  
**Certification File No.:** 00530 **Cert. Date:** 02/23/2012 **Cert. No.:** 00012  
**Linearity File No.:** 00531 **Lin. Date:** 02/23/2012 **Lin. No.:** 00012  
**Solution File No.:** 00539 **Soln. Date:** 04/26/2012 **Soln. No.:** 00122  
**Sequential File No.:** 00539 **File Date:** 04/26/2012

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 01/20/2013  
**Solution Control Lot:** 11A085 **Bottle No.:** 0674

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:12D		
Control 1 EC	0.101%	17:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:13D		
Control 2 EC	0.100%	17:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:15D		
Control 3 EC	0.099%	17:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_

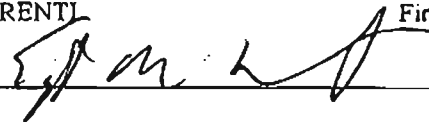

Badge No.: 4025

Date: 04/26/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00529	Calib. Date: 02/23/2012
Certification File No.:	00530	Calib. No.: 00019
Linearity File No.:	00531	Cert. Date: 02/23/2012
Solution File No.:	00537	Cert. No.: 00012
Sequential File No.:	00537	Lin. Date: 02/23/2012
		Lin. No.: 00012
		Soln. Date: 03/23/2012
		Soln. No.: 00121
		File Date: 03/23/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0670

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:15S		
Control 1 EC	0.099%	20:16S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:17S		
Control 2 EC	0.099%	20:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:18S		
Control 3 EC	0.099%	20:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:19S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: 

Badge No.: 4031

Date: 03/23/2012



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00018
Calibration File No.:	00489	Cert. Date:	09/16/2011
Certification File No.:	00490	Lin. Date:	09/16/2011
Linearity File No.:	00491	Soln. Date:	01/30/2012
Solution File No.:	00525	File Date:	01/30/2012
Sequential File No.:	00525		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	01/20/2013
Solution Control Lot:	11A085			Bottle No.:	0669

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:50S		
Control 1 EC	0.100%	03:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:51S		
Control 2 EC	0.099%	03:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:52S		
Control 3 EC	0.099%	03:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: PANARO

First Name: BRIAN

MI: K

Signature: *Brian L Panaro*

Badge No.: 4032

Date: 01/30/2012

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00489	Calib. Date: 09/16/2011
Certification File No.:	00490	Cert. No.: 00018
Linearity File No.:	00491	Cert. Date: 09/16/2011
Solution File No.:	00519	Lin. No.: 00011
Sequential File No.:	00519	Lin. Date: 09/16/2011
		Soln. No.: 00118
		Soln. Date: 12/30/2011
		File Date: 12/30/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 6650

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:55S		
Control 1 EC	0.099%	09:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57S		
Control 2 EC	0.100%	09:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:58S		
Control 3 EC	0.099%	09:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: \_\_\_\_\_



Badge No.: 4031

Date: 12/30/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00489	Calib. Date: 09/16/2011
Certification File No.:	00490	Calib. No.: 00018
Linearity File No.:	00491	Cert. Date: 09/16/2011
Solution File No.:	00509	Cert. No.: 00011
Sequential File No.:	00509	Lin. Date: 09/16/2011
		Lin. No.: 00011
		Soln. Date: 11/29/2011
		Soln. No.: 00117
		File Date: 11/29/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0664

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:24S		
Control 1 EC	0.100%	09:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25S		
Control 2 EC	0.099%	09:26S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27S		
Control 3 EC	0.099%	09:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	09:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_

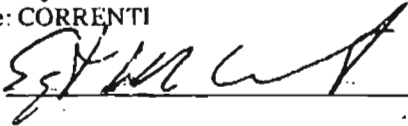

Badge No.: 4025

Date: 11/29/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C		Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00489	Calib. Date: 09/16/2011	Calib. No.: 00018
Certification File No.:	00490	Cert. Date: 09/16/2011	Cert. No.: 00011
Linearity File No.:	00491	Lin. Date: 09/16/2011	Lin. No.: 00011
Solution File No.:	00501	Soln. Date: 11/01/2011	Soln. No.: 00116
Sequential File No.:	00501	File Date: 11/01/2011	

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	01/20/2013
Solution Control Lot:	11A085			Bottle No.:	6600

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:01S		
Control 1 EC	0.101%	16:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:03S		
Control 2 EC	0.100%	16:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:04S		
Control 3 EC	0.100%	16:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature:

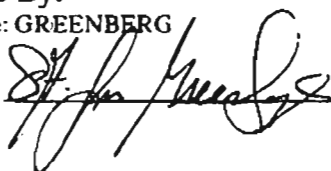

Badge No.: 4031

Date: 11/01/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00489	Calib. No.: 00018
Certification File No.:	00490	Cert. No.: 00011
Linearity File No.:	00491	Lin. No.: 00011
Solution File No.:	00497	Soln. No.: 00115
Sequential File No.:	00497	File Date: 10/05/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0655

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:10D		
Control 1 EC	0.101%	07:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:11D		
Control 2 EC	0.100%	07:12D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:12D		
Control 3 EC	0.100%	07:13D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	07:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: \_\_\_\_\_

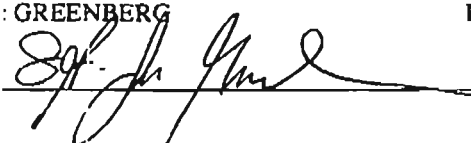

Badge No.: 4031

Date: 10/05/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00458	Calib. Date: 03/28/2011
Certification File No.:	00459	Calib. No.: 00017
Linearity File No.:	00460	Cert. Date: 03/28/2011
Solution File No.:	00486	Cert. No.: 00010
Sequential File No.:	00486	Lin. Date: 03/28/2011
		Lin. No.: 00010
		Soln. Date: 09/09/2011
		Soln. No.: 00112
		File Date: 09/09/2011
<b>Calibrating Unit:</b>	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0654

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:33D		
Control 1 EC	0.099%	20:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:35D		
Control 2 EC	0.099%	20:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:36D		
Control 3 EC	0.099%	20:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature:

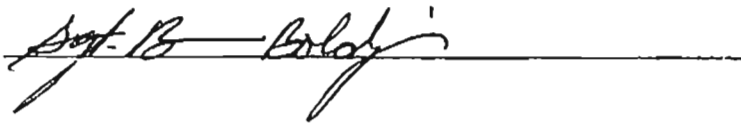

Badge No.: 4028

Date: 09/09/2011

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00458 **Calib. Date:** 03/28/2011 **Calib. No.:** 00017  
**Certification File No.:** 00459 **Cert. Date:** 03/28/2011 **Cert. No.:** 00010  
**Linearity File No.:** 00460 **Lin. Date:** 03/28/2011 **Lin. No.:** 00010  
**Solution File No.:** 00484 **Soln. Date:** 08/10/2011 **Soln. No.:** 00111  
**Sequential File No.:** 00484 **File Date:** 08/10/2011

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222  
**Control Solution %:** 0.100% **Expires:** 01/20/2013  
**Solution Control Lot:** 11A085 **Bottle No.:** 6530

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:24D		
Control 1 EC	0.100%	04:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:25D		
Control 2 EC	0.100%	04:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:26D		
Control 3 EC	0.100%	04:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: 

Badge No.: 4031

Date: 08/10/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.		
<b>Calibration File No.:</b>	00458	<b>Calib. Date:</b>	03/28/2011
<b>Certification File No.:</b>	00459	<b>Cert. No.:</b>	00017
<b>Linearity File No.:</b>	00460	<b>Cert. Date:</b>	03/28/2011
<b>Solution File No.:</b>	00480	<b>Lin. No.:</b>	00010
<b>Sequential File No.:</b>	00480	<b>Soln. Date:</b>	07/15/2011
		<b>Soln. No.:</b>	00110
		<b>File Date:</b>	07/15/2011
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0222
<b>Solution Control Lot:</b>	10F079	<b>Expires:</b>	06/10/2012
		<b>Bottle No.:</b>	1082

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:54D		
Control 1 EC	0.098%	06:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank:	0.000%	06:56D		
Control 2 EC	0.098%	06:56D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank:	0.000%	06:57D		
Control 3 EC	0.098%	06:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	06:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:58D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 07/15/2011



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00017
Calibration File No.:	00458	Cert. Date:	03/28/2011
Certification File No.:	00459	Lin. Date:	03/28/2011
Linearity File No.:	00460	Soln. Date:	06/25/2011
Solution File No.:	00477	File Date:	06/25/2011
Sequential File No.:	00477		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	10F079	Expires:	06/10/2012
		Bottle No.:	1087

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:20D		
Control 1 EC	0.099%	09:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		
Control 2 EC	0.099%	09:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		
Control 3 EC	0.099%	09:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: \_\_\_\_\_

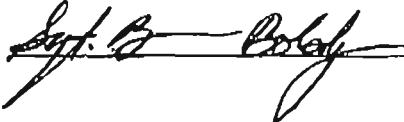

Badge No.: 4028

Date: 06/25/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.	<b>Calib. No.:</b>	00017
<b>Calibration File No.:</b>	00458	<b>Calib. Date:</b>	03/28/2011
<b>Certification File No.:</b>	00459	<b>Cert. Date:</b>	03/28/2011
<b>Linearity File No.:</b>	00460	<b>Lin. Date:</b>	03/28/2011
<b>Solution File No.:</b>	00472	<b>Soln. Date:</b>	05/29/2011
<b>Sequential File No.:</b>	00472	<b>File Date:</b>	05/29/2011
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0222
<b>Solution Control Lot:</b>	10F079	<b>Expires:</b>	06/10/2012
		<b>Bottle No.:</b>	1081

Function	Result	Time	Temperature	Comment(s)
	%RAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank:	0.000%	03:38D		
Control 1 EC	0.098%	03:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	03:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank:	0.000%	03:39D		
Control 2 EC	0.097%	03:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank:	0.000%	03:40D		
Control 3 EC	0.098%	03:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

M1: A

Signature: \_\_\_\_\_

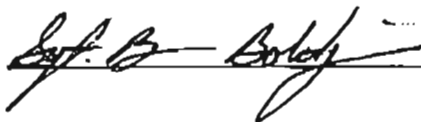

Badge No.: 4028

Date: 05/29/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00017
Calibration File No.:	00458	Cert. Date:	03/28/2011
Certification File No.:	00459	Lin. Date:	03/28/2011
Linearity File No.:	00460	Soln. Date:	04/28/2011
Solution File No.:	00467	File Date:	04/28/2011
Sequential File No.:	00467		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	10F079	Expires:	06/10/2012
		Bottle No.:	1083

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:07D		
Control 1 EC	0.099%	07:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:08D		
Control 2 EC	0.098%	07:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:09D		
Control 3 EC	0.099%	07:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:10D		

All tests within acceptable tolerance.

On this date I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 04/28/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00458	Calib. Date:	03/28/2011
Certification File No.:	00459	Cert. Date:	03/28/2011
Linearity File No.:	00460	Lin. Date:	03/28/2011
Solution File No.:	00461	Soln. Date:	03/28/2011
Sequential File No.:	00461	File Date:	03/28/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	10F079	Expires:	06/10/2012
		Bottle No.:	1093

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:25S	15:25D	
Control 1 EC	0.099%	14:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:26S		
Control 2 EC	0.099%	14:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:27S		
Control 3 EC	0.099%	14:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:29S	15:29D	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-293<sub>010</sub>

**Changed By:**

Last Name: DELLANOCE

First Name: JOSEPH

M1: S

Signature: \_\_\_\_\_

*Tr. II* *J. Dellanoce* #6027

Badge No.: 6027

Date: 03/28/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.		
<b>Calibration File No.:</b>	00427	<b>Calib. Date:</b>	01/05/2011
<b>Certification File No.:</b>	00428	<b>Cert. No.:</b>	00010
<b>Linearity File No.:</b>	00429	<b>Cert. Date:</b>	01/05/2011
<b>Solution File No.:</b>	00446	<b>Lin. No.:</b>	00009
<b>Sequential File No.:</b>	00446	<b>Lin. Date:</b>	01/05/2011
		<b>Soln. No.:</b>	00102
		<b>Soln. Date:</b>	03/05/2011
		<b>File Date:</b>	03/05/2011
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0222
<b>Solution Control Lot:</b>	10F079	<b>Expires:</b>	06/10/2012
		<b>Bottle No.:</b>	1088

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:27S		
Control 1 EC	0.098%	09:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29S		
Control 2 EC	0.096%	09:29S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		
Control 3 EC	0.097%	09:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: \_\_\_\_\_

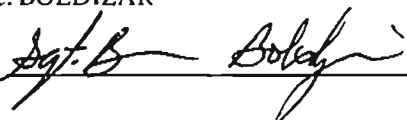

Badge No.: 4028

Date: 03/05/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00427	Calib. Date: 01/05/2011
Certification File No.:	00428	Calib. No.: 00010
Linearity File No.:	00429	Cert. Date: 01/05/2011
Solution File No.:	00441	Cert. No.: 00009
Sequential File No.:	00441	Lin. Date: 01/05/2011
		Lin. No.: 00009
		Soln. Date: 02/26/2011
		Soln. No.: 00101
		File Date: 02/26/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	10F079	Expires: 06/10/2012
		Bottle No.: 1086

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:40S		
Control 1 EC	0.097%	04:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	04:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:42S		
Control 2 EC	0.096%	04:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	04:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:43S		
Control 3 EC	0.097%	04:44S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	04:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:45S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: \_\_\_\_\_

Badge No.: 4029

Date: 02/26/2011

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00427 Calib. Date: 01/05/2011 Calib. No.: 00010  
Certification File No.: 00428 Cert. Date: 01/05/2011 Cert. No.: 00009  
Linearity File No.: 00429 Lin. Date: 01/05/2011 Lin. No.: 00009  
Solution File No.: 00438 Soln. Date: 02/11/2011 Soln. No.: 00100  
Sequential File No.: 00438 File Date: 02/11/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 06/10/2012  
Solution Control Lot: 10F079 Bottle No.: 1092

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:13S		
Control 1 EC	0.099%	08:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:15S		
Control 2 EC	0.097%	08:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:16S		
Control 3 EC	0.098%	08:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 02/11/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00427	Calib. Date: 01/05/2011
Certification File No.:	00428	Calib. No.: 00010
Linearity File No.:	00429	Cert. Date: 01/05/2011
Solution File No.:	00437	Cert. No.: 00009
Sequential File No.:	00437	Lin. Date: 01/05/2011
		Lin. No.: 00009
		Soln. Date: 02/10/2011
		Soln. No.: 00099
		File Date: 02/10/2011
<b>Calibrating Unit:</b>	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	10F079	Expires: 06/10/2012
		Bottle No.: 1091

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:02S		
Control 1 EC	0.099%	11:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04S		
Control 2 EC	0.096%	11:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05S		
Control 3 EC	0.099%	11:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:07S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GOLDEN

First Name: DOMENIQUE

MI: L

Signature: 

Badge No.: 4023

Date: 02/10/2011



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00009
Calibration File No.:	00392	Calib. Date:	07/06/2010
Certification File No.:	00393	Cert. Date:	07/06/2010
Linearity File No.:	00394	Lin. Date:	07/06/2010
Solution File No.:	00424	Soln. Date:	12/22/2010
Sequential File No.:	00424	File Date:	12/22/2010
Calibrating Unit:	WFT	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	10F079	Expires:	06/10/2012
		Bottle No.:	1077

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:04S		
Control 1 EC	0.103%	12:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	12:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:06S		
Control 2 EC	0.100%	12:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		
Control 3 EC	0.102%	12:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	12:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

*TEMPERATURE PROBE SERIAL NUMBER: DDWTP2-293<sub>3</sub>*

**Changed By:**

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: *Joseph Dellanoce #6027*

Badge No.: 6027

Date: 12/22/2010



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

NDUMS3-0222

Certification Date

11-17-10

Technician

MM

Re-Certification Due Date

11-17-11

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWTP2-293

Certification date:

11-17-10

Next Certification due:

11-17-11

Probe Value

105

Draeger Safety Diagnostics, Inc.  
Technical Service Department

MM

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00392 **Calib. Date:** 07/06/2010 **Calib. No.:** 00009  
**Certification File No.:** 00393 **Cert. Date:** 07/06/2010 **Cert. No.:** 00008  
**Linearity File No.:** 00394 **Lin. Date:** 07/06/2010 **Lin. No.:** 00008  
**Solution File No.:** 00423 **Soln. Date:** 12/17/2010 **Soln. No.:** 00095  
**Sequential File No.:** 00423 **File Date:** 12/17/2010

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 06/10/2012  
**Solution Control Lot:** 10F079 **Bottle No.:** 1089

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:43S		
Control 1 EC	0.103%	05:43S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	05:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:44S		
Control 2 EC	0.100%	05:45S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:46S		
Control 3 EC	0.101%	05:46S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:47S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 12/17/2010

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00392	Calib. Date: 07/06/2010
Certification File No.:	00393	Cert. No.: 00009
Linearity File No.:	00394	Lin. Date: 07/06/2010
Solution File No.:	00415	Lin. No.: 00008
Sequential File No.:	00415	Soln. Date: 11/02/2010
		Soln. No.: 00093
		File Date: 11/02/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	10F079	Expires: 06/10/2012
		Bottle No.: 1096

Function	Result	Time	Temperature	Comment(s) or Error(s)
	%BAC	HH:MM	Simulator (°C)	
Ambient Air Blank	0.000%	08:42S		
Control 1 EC	0.103%	08:43S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	08:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:43S		
Control 2 EC	0.101%	08:44S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:45S		
Control 3 EC	0.100%	08:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 11/02/2010

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00392	Calib. No.: 00009
Certification File No.:	00393	Cert. No.: 00008
Linearity File No.:	00394	Lin. No.: 00008
Solution File No.:	00413	Soln. No.: 00092
Sequential File No.:	00413	File Date: 10/06/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 1101

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:04D		
Control 1 EC	0.101%	05:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	05:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:05D		
Control 2 EC	0.101%	05:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:06D		
Control 3 EC	0.101%	05:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: \_\_\_\_\_



Badge No.: 4028

Date: 10/06/2010

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00009
Calibration File No.:	00392	Cert. Date:	07/06/2010
Certification File No.:	00393	Lin. Date:	07/06/2010
Linearity File No.:	00394	Soln. Date:	09/18/2010
Solution File No.:	00411	File Date:	09/18/2010
Sequential File No.:	00411		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1107

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:34D		
Control 1 EC	0.101%	07:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:35D		
Control 2 EC	0.100%	07:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:37D		
Control 3 EC	0.100%	07:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	07:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: \_\_\_\_\_



Badge No.: 4031

Date: 09/18/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00009
Calibration File No.:	00392	Cert. Date:	07/06/2010
Certification File No.:	00393	Lin. Date:	07/06/2010
Linearity File No.:	00394	Soln. Date:	09/06/2010
Solution File No.:	00409	File Date:	09/06/2010
Sequential File No.:	00409		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	02/02/2011
Solution Control Lot:	09B063			Bottle No.:	1102

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:34D		
Control 1 EC	0.100%	20:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:35D		
Control 2 EC	0.099%	20:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:36D		
Control 3 EC	0.099%	20:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: \_\_\_\_\_



Badge No.: 4028

Date: 09/06/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00009
Calibration File No.:	00392	Cert. Date:	07/06/2010
Certification File No.:	00393	Lin. Date:	07/06/2010
Linearity File No.:	00394	Soln. Date:	08/16/2010
Solution File No.:	00402	File Date:	08/16/2010
Sequential File No.:	00402		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1106

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:43D		
Control 1 EC	0.102%	02:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	02:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:45D		
Control 2 EC	0.100%	02:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:46D		
Control 3 EC	0.100%	02:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	02:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 08/16/2010



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00392	Calib. Date: 07/06/2010
Certification File No.:	00393	Calib. No.: 00009
Linearity File No.:	00394	Cert. Date: 07/06/2010
Solution File No.:	00399	Cert. No.: 00008
Sequential File No.:	00399	Lin. Date: 07/06/2010
		Lin. No.: 00008
		Soln. Date: 07/28/2010
		Soln. No.: 00088
		File Date: 07/28/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUM S3-0225
Control Solution %: 0.100%		Expires: 02/02/2011
Solution Control Lot: 09B063		Bottle No.: 1112

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:20D		
Control 1 EC	0.102%	06:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:21D		
Control 2 EC	0.100%	06:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:22D		
Control 3 EC	0.100%	06:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Det. Ben Palombi II*

Badge No.: 4019

Date: 07/28/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00392	Calib. Date: 07/06/2010
Certification File No.:	00393	Calib. No.: 00009
Linearity File No.:	00394	Cert. Date: 07/06/2010
Solution File No.:	00395	Cert. No.: 00008
Sequential File No.:	00395	Lin. Date: 07/06/2010
		Lin. No.: 00008
		Soln. Date: 07/06/2010
		Soln. No.: 00087
		File Date: 07/06/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 1122

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:35D		
Control 1 EC	0.100%	13:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:37D		
Control 2 EC	0.100%	13:37D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:38D		
Control 3 EC	0.100%	13:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:39D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWTP2-144<sub>250</sub>

**Changed By:**

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: \_\_\_\_\_

T.D. II [Signature] # 6027

Badge No.: 6027

Date: 07/06/2010

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00356 Calib. Date: 01/07/2010 Calib. No.: 00008  
Certification File No.: 00357 Cert. Date: 01/07/2010 Cert. No.: 00007  
Linearity File No.: 00358 Lin. Date: 01/07/2010 Lin. No.: 00007  
Solution File No.: 00386 Soln. Date: 05/21/2010 Soln. No.: 00085  
Sequential File No.: 00386 File Date: 05/21/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 02/02/2011  
Solution Control Lot: 09B063 Bottle No.: 1119

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:03D		
Control 1 EC	0.100%	17:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:05D		
Control 2 EC	0.098%	17:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:06D		
Control 3 EC	0.099%	17:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_

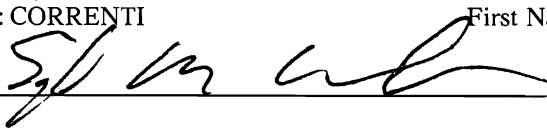

Badge No.: 4025

Date: 05/21/2010

# Calibrating Unit New Standard Solution Report


<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00356	Calib. Date: 01/07/2010
Certification File No.:	00357	Calib. No.: 00008
Linearity File No.:	00358	Cert. Date: 01/07/2010
Solution File No.:	00381	Cert. No.: 00007
Sequential File No.:	00381	Lin. Date: 01/07/2010
		Lin. No.: 00007
		Soln. Date: 04/24/2010
		Soln. No.: 00084
		File Date: 04/24/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 1103

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:26D		
Control 1 EC	0.100%	21:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:27D		
Control 2 EC	0.099%	21:28D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:28D		
Control 3 EC	0.100%	21:29D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:30D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI	First Name: MAURO	MI: J
Signature: 		Badge No.: 4025
		Date: 04/24/2010

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00356 Calib. Date: 01/07/2010 Calib. No.: 00008  
Certification File No.: 00357 Cert. Date: 01/07/2010 Cert. No.: 00007  
Linearity File No.: 00358 Lin. Date: 01/07/2010 Lin. No.: 00007  
Solution File No.: 00378 Soln. Date: 03/25/2010 Soln. No.: 00083  
Sequential File No.: 00378 File Date: 03/25/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 02/02/2011  
Solution Control Lot: 09B063 Bottle No.: 1111

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:03S		
Control 1 EC	0.101%	14:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:04S		
Control 2 EC	0.099%	14:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:06S		
Control 3 EC	0.100%	14:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: \_\_\_\_\_



Badge No.: 4029

Date: 03/25/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00008
Calibration File No.:	00356	Cert. Date:	01/07/2010
Certification File No.:	00357	Lin. Date:	01/07/2010
Linearity File No.:	00358	Soln. Date:	03/24/2010
Solution File No.:	00377	File Date:	03/24/2010
Sequential File No.:	00377		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1116

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:49S		
Control 1 EC	-.---%	12:50S	20.5°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	12:50S	20.5°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: \_\_\_\_\_

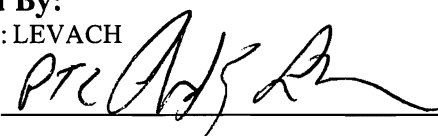

Badge No.: 4029

Date: 03/24/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00008
Calibration File No.:	00356	Cert. Date:	01/07/2010
Certification File No.:	00357	Lin. Date:	01/07/2010
Linearity File No.:	00358	Soln. Date:	03/23/2010
Solution File No.:	00376	File Date:	03/23/2010
Sequential File No.:	00376		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1116

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:34S		
Control 1 EC	-.---%	14:35S	19.3°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	14:35S	19.3°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: \_\_\_\_\_

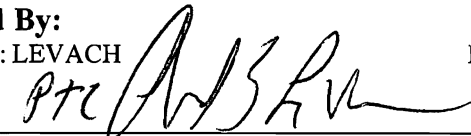

Badge No.: 4029

Date: 03/23/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00008
Calibration File No.:	00356	Cert. Date:	01/07/2010
Certification File No.:	00357	Lin. Date:	01/07/2010
Linearity File No.:	00358	Soln. Date:	03/23/2010
Solution File No.:	00375	File Date:	03/23/2010
Sequential File No.:	00375		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1116

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:33S		
Control 1 EC	-.---%	13:34S	19.0°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	13:34S	19.0°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: \_\_\_\_\_



Badge No.: 4029

Date: 03/23/2010



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00356	Calib. Date: 01/07/2010
Certification File No.:	00357	Calib. No.: 00008
Linearity File No.:	00358	Cert. Date: 01/07/2010
Solution File No.:	00371	Cert. No.: 00007
Sequential File No.:	00371	Lin. Date: 01/07/2010
		Lin. No.: 00007
		Soln. Date: 03/02/2010
		Soln. No.: 00079
		File Date: 03/02/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 1123

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:55S		
Control 1 EC	0.101%	07:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:56S		
Control 2 EC	0.099%	07:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:58S		
Control 3 EC	0.099%	07:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: \_\_\_\_\_

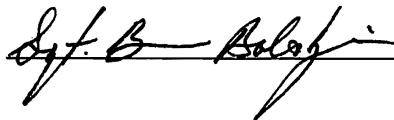

Badge No.: 4028

Date: 03/02/2010

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00356 Calib. Date: 01/07/2010 Calib. No.: 00008  
Certification File No.: 00357 Cert. Date: 01/07/2010 Cert. No.: 00007  
Linearity File No.: 00358 Lin. Date: 01/07/2010 Lin. No.: 00007  
Solution File No.: 00367 Soln. Date: 02/01/2010 Soln. No.: 00078  
Sequential File No.: 00367 File Date: 02/01/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 02/02/2011  
Solution Control Lot: 09B063 Bottle No.: 1113

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:00S		
Control 1 EC	0.099%	10:01S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:01S		
Control 2 EC	0.097%	10:02S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03S		
Control 3 EC	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 02/01/2010

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00356	Calib. Date: 01/07/2010
Certification File No.:	00357	Calib. No.: 00008
Linearity File No.:	00358	Cert. Date: 01/07/2010
Solution File No.:	00359	Cert. No.: 00007
Sequential File No.:	00359	Lin. Date: 01/07/2010
		Lin. No.: 00007
		Soln. Date: 01/07/2010
		Soln. No.: 00077
		File Date: 01/07/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 1117

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:26S		
Control 1 EC	0.103%	12:27S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:28S		
Control 2 EC	0.101%	12:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29S		
Control 3 EC	0.101%	12:30S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:31S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

*Temperature Probe Serial Number: DDWJP2-29335*

**Changed By:**

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *TP: I J Sullivan #5103*

Badge No.: 5103

Date: 01/07/2010

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00327 Calib. Date: 07/13/2009 Calib. No.: 00007  
Certification File No.: 00328 Cert. Date: 07/13/2009 Cert. No.: 00006  
Linearity File No.: 00329 Lin. Date: 07/13/2009 Lin. No.: 00006  
Solution File No.: 00354 Soln. Date: 12/11/2009 Soln. No.: 00076  
Sequential File No.: 00354 File Date: 12/11/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 02/02/2011  
Solution Control Lot: 09B063 Bottle No.: 1110

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:46S		
Control 1 EC	0.101%	07:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:47S		
Control 2 EC	0.099%	07:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:48S		
Control 3 EC	0.099%	07:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	07:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Ken Palombi III*

Badge No.: 4019

Date: 12/11/2009

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00327 Calib. Date: 07/13/2009 Calib. No.: 00007  
Certification File No.: 00328 Cert. Date: 07/13/2009 Cert. No.: 00006  
Linearity File No.: 00329 Lin. Date: 07/13/2009 Lin. No.: 00006  
Solution File No.: 00349 Soln. Date: 11/26/2009 Soln. No.: 00075  
Sequential File No.: 00349 File Date: 11/26/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 02/02/2011  
Solution Control Lot: 09B063 Bottle No.: 1120

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:40S		
Control 1 EC	0.100%	07:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:41S		
Control 2 EC	0.099%	07:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:42S		
Control 3 EC	0.099%	07:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:44S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 11/26/2009

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00327	Calib. Date:	07/13/2009
Certification File No.:	00328	Cert. No.:	00007
Linearity File No.:	00329	Cert. Date:	07/13/2009
Solution File No.:	00347	Lin. No.:	00006
Sequential File No.:	00347	Lin. Date:	07/13/2009
		Soln. No.:	00074
		Soln. Date:	10/30/2009
		File Date:	10/30/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1109

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:49S		
Control 1 EC	0.100%	07:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:51S		
Control 2 EC	0.099%	07:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	07:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:52S		
Control 3 EC	0.100%	07:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 10/30/2009

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 00327 Calib. Date: 07/13/2009 Calib. No.: 00007  
Certification File No.: 00328 Cert. Date: 07/13/2009 Cert. No.: 00006  
Linearity File No.: 00329 Lin. Date: 07/13/2009 Lin. No.: 00006  
Solution File No.: 00345 Soln. Date: 10/03/2009 Soln. No.: 00073  
Sequential File No.: 00345 File Date: 10/03/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 02/02/2011  
Solution Control Lot: 09B063 Bottle No.: 1114

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:57D		
Control 1 EC	0.100%	08:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59D		
Control 2 EC	0.100%	08:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:00D		
Control 3 EC	0.100%	09:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:01D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

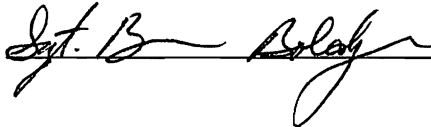Signature: 

Badge No.: 4028

Date: 10/03/2009

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00327	Calib. Date: 07/13/2009
Certification File No.:	00328	Cert. No.: 00007
Linearity File No.:	00329	Cert. Date: 07/13/2009
Solution File No.:	00343	Lin. No.: 00006
Sequential File No.:	00343	Lin. Date: 07/13/2009
		Soln. No.: 00072
		Soln. Date: 09/08/2009
		File Date: 09/08/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 1118

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:43D		
Control 1 EC	0.101%	11:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:44D		
Control 2 EC	0.100%	11:44D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	11:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:45D		
Control 3 EC	0.100%	11:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:46D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: \_\_\_\_\_

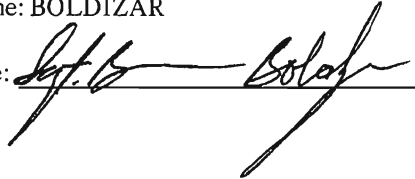

Badge No.: 4028

Date: 09/08/2009



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.	<b>Calib. No.:</b>	00007
<b>Calibration File No.:</b>	00327	<b>Calib. Date:</b>	07/13/2009
<b>Certification File No.:</b>	00328	<b>Cert. Date:</b>	07/13/2009
<b>Linearity File No.:</b>	00329	<b>Lin. Date:</b>	07/13/2009
<b>Solution File No.:</b>	00339	<b>Soln. Date:</b>	08/17/2009
<b>Sequential File No.:</b>	00339	<b>File Date:</b>	08/17/2009
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0222
<b>Solution Control Lot:</b>	09B063	<b>Expires:</b>	02/02/2011
		<b>Bottle No.:</b>	1124

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:33D		
Control 1 EC	0.098%	15:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:34D		
Control 2 EC	0.097%	15:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:36D		
Control 3 EC	0.097%	15:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

*TEMPERATURE PROBE SERIAL NUMBER: DDUM S3-293 FM*

**Changed By:**

Last Name: MASSENBERG

First Name: FERNANDEZ

MI: -

Signature: *[Handwritten Signature]* 5823

Badge No.: 5623

Date: 08/17/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00007
Calibration File No.:	00327	Calib. Date:	07/13/2009
Certification File No.:	00328	Cert. Date:	07/13/2009
Linearity File No.:	00329	Lin. Date:	07/13/2009
Solution File No.:	00338	Soln. Date:	08/11/2009
Sequential File No.:	00338	File Date:	08/11/2009
Calibrating Unit:	WLT	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1121

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:07D		
Control 1 EC	0.101%	08:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 2 EC	0.099%	08:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09D		
Control 3 EC	0.098%	08:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

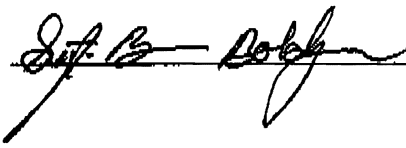Signature: 

Badge No.: 4028

Date: 08/11/2009

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00007
Calibration File No.:	00327	Cert. Date:	07/13/2009
Certification File No.:	00328	Lin. Date:	07/13/2009
Linearity File No.:	00329	Soln. Date:	07/13/2009
Solution File No.:	00330	File Date:	07/13/2009
Sequential File No.:	00330		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	1125

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:02D		
Control 1 EC	0.101%	14:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:03D		
Control 2 EC	0.100%	14:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:04D		
Control 3 EC	0.100%	14:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWSP2-144 FM

**Changed By:**

Last Name: MASSENBERG

First Name: FERNANDEZ

MI: -

Signature: \_\_\_\_\_

*[Handwritten Signature]*

Badge No.: 5623

Date: 07/13/2009



State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

JON S. CORZINE  
Governor

ANNE MILGRAM  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 2/27/2009

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 09B063

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1199 to 0.1205 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 2, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 5 day of March, 2009.

Notary  
JOHN R. LEAVER  
NOTARY PUBLIC STATE OF NEW JERSEY  
MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00291	Calib. Date: 01/23/2009
Certification File No.:	00292	Calib. No.: 00006
Linearity File No.:	00293	Cert. Date: 01/23/2009
Solution File No.:	00326	Cert. No.: 00005
Sequential File No.:	00326	Lin. Date: 01/23/2009
		Lin. No.: 00005
		Soln. Date: 07/13/2009
		Soln. No.: 00068
		File Date: 07/13/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 0282

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:10D		
Control 1 EC	0.100%	02:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:12D		
Control 2 EC	0.099%	02:12D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	02:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:13D		
Control 3 EC	0.099%	02:13D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 07/13/2009

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00291 **Calib. Date:** 01/23/2009 **Calib. No.:** 00006  
**Certification File No.:** 00292 **Cert. Date:** 01/23/2009 **Cert. No.:** 00005  
**Linearity File No.:** 00293 **Lin. Date:** 01/23/2009 **Lin. No.:** 00005  
**Solution File No.:** 00323 **Soln. Date:** 06/16/2009 **Soln. No.:** 00067  
**Sequential File No.:** 00323 **File Date:** 06/16/2009

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 01/09/2010  
**Solution Control Lot:** 08A049 **Bottle No.:** 0285

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:30D		
Control 1 EC	0.100%	11:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31D		
Control 2 EC	0.099%	11:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33D		
Control 3 EC	0.100%	11:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: PTC Charles Levach

Badge No.: 4029

Date: 06/16/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00291	Calib. Date: 01/23/2009
Certification File No.:	00292	Calib. No.: 00006
Linearity File No.:	00293	Cert. Date: 01/23/2009
Solution File No.:	00320	Cert. No.: 00005
Sequential File No.:	00320	Lin. Date: 01/23/2009
		Lin. No.: 00005
		Soln. Date: 05/23/2009
		Soln. No.: 00066
		File Date: 05/23/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 0283

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:13D		
Control 1 EC	0.100%	19:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:14D		
Control 2 EC	0.098%	19:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:15D		
Control 3 EC	0.099%	19:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	19:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:17D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: 

Badge No.: 4019

Date: 05/23/2009

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00291 **Calib. Date:** 01/23/2009 **Calib. No.:** 00006  
**Certification File No.:** 00292 **Cert. Date:** 01/23/2009 **Cert. No.:** 00005  
**Linearity File No.:** 00293 **Lin. Date:** 01/23/2009 **Lin. No.:** 00005  
**Solution File No.:** 00319 **Soln. Date:** 05/23/2009 **Soln. No.:** 00065  
**Sequential File No.:** 00319 **File Date:** 05/23/2009

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 01/09/2010  
**Solution Control Lot:** 08A049 **Bottle No.:** 0281

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:31D		
Control 1 EC	0.101%	14:32D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.113%	14:32D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	14:33D		
Control 2 EC	0.099%	14:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:34D		
Control 3 EC	0.099%	14:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:35D		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

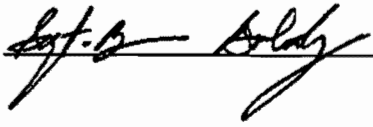Signature: 

Badge No.: 4028

Date: 05/23/2009



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.	
<b>Calibration File No.:</b>	00291	<b>Calib. Date:</b> 01/23/2009
<b>Certification File No.:</b>	00292	<b>Calib. No.:</b> 00006
<b>Linearity File No.:</b>	00293	<b>Cert. Date:</b> 01/23/2009
<b>Solution File No.:</b>	00318	<b>Cert. No.:</b> 00005
<b>Sequential File No.:</b>	00318	<b>Lin. Date:</b> 01/23/2009
		<b>Lin. No.:</b> 00005
		<b>Soln. Date:</b> 05/23/2009
		<b>Soln. No.:</b> 00064
		<b>File Date:</b> 05/23/2009
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b> CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b> DDUM S3-0225
<b>Solution Control Lot:</b>	08A049	<b>Expires:</b> 01/09/2010
		<b>Bottle No.:</b> 0281

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:59D		
Control 1 EC	0.101%	08:00D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.107%	08:00D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:01D		
Control 2 EC	0.100%	08:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		
Control 3 EC	0.099%	08:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:03D		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 05/23/2009

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00291 **Calib. Date:** 01/23/2009 **Calib. No.:** 00006  
**Certification File No.:** 00292 **Cert. Date:** 01/23/2009 **Cert. No.:** 00005  
**Linearity File No.:** 00293 **Lin. Date:** 01/23/2009 **Lin. No.:** 00005  
**Solution File No.:** 00314 **Soln. Date:** 04/25/2009 **Soln. No.:** 00063  
**Sequential File No.:** 00314 **File Date:** 04/25/2009

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 01/09/2010  
**Solution Control Lot:** 08A049 **Bottle No.:** 0284

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:18D		
Control 1 EC	0.098%	11:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		
Control 2 EC	0.097%	11:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20D		
Control 3 EC	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: 

Badge No.: 4016

Date: 04/25/2009

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00291 **Calib. Date:** 01/23/2009 **Calib. No.:** 00006  
**Certification File No.:** 00292 **Cert. Date:** 01/23/2009 **Cert. No.:** 00005  
**Linearity File No.:** 00293 **Lin. Date:** 01/23/2009 **Lin. No.:** 00005  
**Solution File No.:** 00310 **Soln. Date:** 03/28/2009 **Soln. No.:** 00062  
**Sequential File No.:** 00310 **File Date:** 03/28/2009

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 01/09/2010  
**Solution Control Lot:** 08A049 **Bottle No.:** 0280

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:22S		
Control 1 EC	0.101%	23:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:23S		
Control 2 EC	0.099%	23:24S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:25S		
Control 3 EC	0.099%	23:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:26S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: 

Badge No.: 4016

Date: 03/28/2009

# Calibrating Unit


## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00291	Calib. Date: 01/23/2009
Certification File No.:	00292	Calib. No.: 00006
Linearity File No.:	00293	Cert. Date: 01/23/2009
Solution File No.:	00307	Cert. No.: 00005
Sequential File No.:	00307	Lin. Date: 01/23/2009
		Lin. No.: 00005
		Soln. Date: 03/13/2009
		Soln. No.: 00061
		File Date: 03/13/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 0277

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:34S		
Control 1 EC	0.099%	08:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:36S		
Control 2 EC	0.098%	08:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:37S		
Control 3 EC	0.099%	08:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:39S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**  
 Last Name: LEVACH First Name: CHARLES MI: -  
 Signature:  Badge No.: 4029  
Date: 03/13/2009

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.	<b>Calib. No.:</b>	00006
<b>Calibration File No.:</b>	00291	<b>Cert. Date:</b>	01/23/2009
<b>Certification File No.:</b>	00292	<b>Lin. Date:</b>	01/23/2009
<b>Linearity File No.:</b>	00293	<b>Soln. Date:</b>	02/18/2009
<b>Solution File No.:</b>	00298	<b>File Date:</b>	02/18/2009
<b>Sequential File No.:</b>	00298		
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0225
<b>Solution Control Lot:</b>	08A049	<b>Expires:</b>	01/09/2010
		<b>Bottle No.:</b>	0276

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:41S		
Control 1 EC	0.100%	02:42S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	02:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:43S		
Control 2 EC	0.098%	02:43S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	02:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:44S		
Control 3 EC	0.100%	02:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_

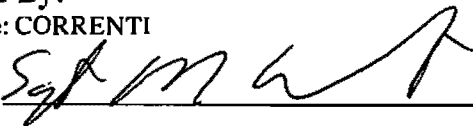

Badge No.: 4025

Date: 02/18/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
<b>Location:</b>	FLORENCE TOWNSHIP P.D.		
<b>Calibration File No.:</b>	00291	<b>Calib. Date:</b>	01/23/2009
<b>Certification File No.:</b>	00292	<b>Cert. No.:</b>	00006
<b>Linearity File No.:</b>	00293	<b>Cert. Date:</b>	01/23/2009
<b>Solution File No.:</b>	00294	<b>Lin. No.:</b>	00005
<b>Sequential File No.:</b>	00294	<b>Soln. Date:</b>	01/23/2009
		<b>Soln. No.:</b>	00059
		<b>File Date:</b>	01/23/2009
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDUM S3-0225
<b>Solution Control Lot:</b>	08A049	<b>Expires:</b>	01/09/2010
		<b>Bottle No.:</b>	0287

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:57S		
Control 1 EC	0.102%	16:57S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:58S		
Control 2 EC	0.099%	16:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00S		
Control 3 EC	0.100%	17:00S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:01S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

*TEMPERATURE PROBE SERIAL NUMBER: DDWJPR-144 FM*

**Changed By:**

Last Name: MASSENBERG

First Name: FERNANDEZ

MI: -

Signature: *[Handwritten Signature]*

*[Handwritten Signature]* 5623

Badge No.: 5623

Date: 01/23/2009

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00251 **Calib. Date:** 07/29/2008 **Calib. No.:** 00005  
**Certification File No.:** 00252 **Cert. Date:** 07/29/2008 **Cert. No.:** 00004  
**Linearity File No.:** 00253 **Lin. Date:** 07/29/2008 **Lin. No.:** 00004  
**Solution File No.:** 00289 **Soln. Date:** 01/16/2009 **Soln. No.:** 00058  
**Sequential File No.:** 00289 **File Date:** 01/16/2009

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 01/09/2010  
**Solution Control Lot:** 08A049 **Bottle No.:** 0288

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:46S		
Control 1 EC	0.101%	08:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47S		
Control 2 EC	0.099%	08:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49S		
Control 3 EC	0.099%	08:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 01/16/2009