

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00251 **Calib. Date:** 07/29/2008 **Calib. No.:** 00005
Certification File No.: 00252 **Cert. Date:** 07/29/2008 **Cert. No.:** 00004
Linearity File No.: 00253 **Lin. Date:** 07/29/2008 **Lin. No.:** 00004
Solution File No.: 00284 **Soln. Date:** 12/22/2008 **Soln. No.:** 00057
Sequential File No.: 00284 **File Date:** 12/22/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 01/09/2010
Solution Control Lot: 08A049 **Bottle No.:** 0279

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:03S		
Control 1 EC	0.101%	15:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:05S		
Control 2 EC	0.099%	15:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:06S		
Control 3 EC	0.099%	15:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 12/22/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00251	Calib. Date: 07/29/2008
Certification File No.:	00252	Calib. No.: 00005
Linearity File No.:	00253	Cert. Date: 07/29/2008
Solution File No.:	00282	Cert. No.: 00004
Sequential File No.:	00282	Lin. Date: 07/29/2008
		Lin. No.: 00004
		Soln. Date: 12/02/2008
		Soln. No.: 00056
		File Date: 12/02/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 0278

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:44S		
Control 1 EC	0.100%	09:44S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45S		
Control 2 EC	0.099%	09:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47S		
Control 3 EC	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: _____

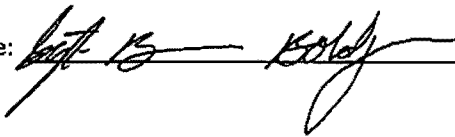

Badge No.: 4028

Date: 12/02/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00251	Calib. Date: 07/29/2008
Certification File No.:	00252	Calib. No.: 00005
Linearity File No.:	00253	Cert. Date: 07/29/2008
Solution File No.:	00276	Cert. No.: 00004
Sequential File No.:	00276	Lin. Date: 07/29/2008
		Lin. No.: 00004
		Soln. Date: 11/07/2008
		Soln. No.: 00055
		File Date: 11/07/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 0294

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:02S		
Control 1 EC	0.100%	10:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03S		
Control 2 EC	0.098%	10:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05S		
Control 3 EC	0.098%	10:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-144 re

Changed By:

Last Name: CROSS	First Name: WILLIAM	MI: M
Signature: <u>TPR. I WILLIAM CROSS #5342</u>	Badge No.: 5342	Date: 11/07/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00251	Calib. Date:	07/29/2008
Certification File No.:	00252	Cert. No.:	00005
Linearity File No.:	00253	Cert. Date:	07/29/2008
Solution File No.:	00273	Lin. No.:	00004
Sequential File No.:	00273	Lin. Date:	07/29/2008
		Soln. Date:	10/30/2008
		Soln. No.:	00054
		File Date:	10/30/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	08A049	Expires:	01/09/2010
		Bottle No.:	0297

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:00S		
Control 1 EC	0.100%	01:00S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:01S		
Control 2 EC	0.099%	01:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:02S		
Control 3 EC	0.099%	01:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:03S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

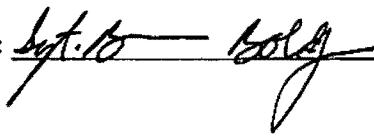Signature:  _____

Badge No.: 4028

Date: 10/30/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00251 **Calib. Date:** 07/29/2008 **Calib. No.:** 00005
Certification File No.: 00252 **Cert. Date:** 07/29/2008 **Cert. No.:** 00004
Linearity File No.: 00253 **Lin. Date:** 07/29/2008 **Lin. No.:** 00004
Solution File No.: 00266 **Soln. Date:** 09/29/2008 **Soln. No.:** 00053
Sequential File No.: 00266 **File Date:** 09/29/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 01/09/2010
Solution Control Lot: 08A049 **Bottle No.:** 0298

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:19D		
Control 1 EC	0.101%	11:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21D		
Control 2 EC	0.099%	11:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		
Control 3 EC	0.099%	11:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 09/29/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00251 **Calib. Date:** 07/29/2008 **Calib. No.:** 00005
Certification File No.: 00252 **Cert. Date:** 07/29/2008 **Cert. No.:** 00004
Linearity File No.: 00253 **Lin. Date:** 07/29/2008 **Lin. No.:** 00004
Solution File No.: 00264 **Soln. Date:** 09/05/2008 **Soln. No.:** 00052
Sequential File No.: 00264 **File Date:** 09/05/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 01/09/2010
Solution Control Lot: 08A049 **Bottle No.:** 0299

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:33D		
Control 1 EC	0.100%	02:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:35D		
Control 2 EC	0.098%	02:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:36D		
Control 3 EC	0.098%	02:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Det Ben Palombi III*

Badge No.: 4019

Date: 09/05/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00251 **Calib. Date:** 07/29/2008 **Calib. No.:** 00005
Certification File No.: 00252 **Cert. Date:** 07/29/2008 **Cert. No.:** 00004
Linearity File No.: 00253 **Lin. Date:** 07/29/2008 **Lin. No.:** 00004
Solution File No.: 00257 **Soln. Date:** 08/10/2008 **Soln. No.:** 00048
Sequential File No.: 00257 **File Date:** 08/10/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 01/09/2010
Solution Control Lot: 08A049 **Bottle No.:** 0289

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:59D		
Control 1 EC	0.100%	10:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00D		
Control 2 EC	0.099%	10:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		
Control 3 EC	0.099%	10:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: _____



Badge No.: 4028

Date: 08/10/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00251	Calib. Date:	07/29/2008
Certification File No.:	00252	Cert. Date:	07/29/2008
Linearity File No.:	00253	Lin. Date:	07/29/2008
Solution File No.:	00254	Soln. Date:	07/29/2008
Sequential File No.:	00254	File Date:	07/29/2008

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0222
Control Solution %:	0.100%			Expires:	01/09/2010
Solution Control Lot:	08A049			Bottle No.:	0291

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:11D		
Control 1 EC	0.101%	11:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:12D		
Control 2 EC	0.100%	11:12D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13D		
Control 3 EC	0.100%	11:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROOF SERIAL NUMBER: DDWJPa-293 we

Changed By:

Last Name: CROSS

First Name: WILLIAM

MI: M

Signature: _____

TPR. I WILLIAM CROSS #5342

Badge No.: 5342

Date: 07/29/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 Calib. Date: 10/16/2007 Calib. No.: 00004
Certification File No.: 00197 Cert. Date: 10/16/2007 Cert. No.: 00003
Linearity File No.: 00198 Lin. Date: 10/16/2007 Lin. No.: 00003
Solution File No.: 00248 Soln. Date: 07/19/2008 Soln. No.: 00046
Sequential File No.: 00248 File Date: 07/19/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 01/09/2010
Solution Control Lot: 08A049 Bottle No.: 0292

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:51D		
Control 1 EC	0.101%	11:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52D		
Control 2 EC	0.100%	11:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53D		
Control 3 EC	0.100%	11:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: _____

Sgt Benjamin Palombi

Badge No.: 4019

Date: 07/19/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00196	Calib. Date:	10/16/2007
Certification File No.:	00197	Calib. No.:	00004
Linearity File No.:	00198	Cert. Date:	10/16/2007
Solution File No.:	00242	Cert. No.:	00003
Sequential File No.:	00242	Lin. Date:	10/16/2007
		Lin. No.:	00003
		Soln. Date:	06/22/2008
		Soln. No.:	00045
		File Date:	06/22/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	08A049	Expires:	01/09/2010
		Bottle No.:	0300

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:04D		
Control 1 EC	0.102%	20:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:05D		
Control 2 EC	0.100%	20:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:06D		
Control 3 EC	0.100%	20:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature:

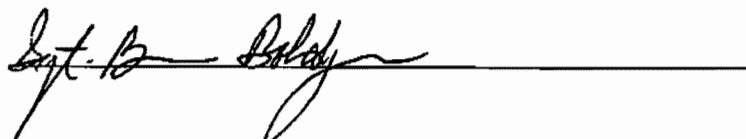

Badge No.: 4028

Date: 06/22/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00196	Calib. Date:	10/16/2007
Certification File No.:	00197	Cert. No.:	00004
Linearity File No.:	00198	Cert. Date:	10/16/2007
Solution File No.:	00236	Lin. Date:	10/16/2007
Sequential File No.:	00236	Lin. No.:	00003
		Soln. Date:	05/22/2008
		Soln. No.:	00044
		File Date:	05/22/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	08A049	Expires:	01/09/2010
		Bottle No.:	0293

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:59D		
Control 1 EC	0.101%	03:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:00D		
Control 2 EC	0.100%	04:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:01D		
Control 3 EC	0.100%	04:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: _____



Badge No.: 4029

Date: 05/22/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 **Calib. Date:** 10/16/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/16/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/16/2007 **Lin. No.:** 00003
Solution File No.: 00231 **Soln. Date:** 05/03/2008 **Soln. No.:** 00043
Sequential File No.: 00231 **File Date:** 05/03/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 01/09/2010
Solution Control Lot: 08A049 **Bottle No.:** 0295

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:03D		
Control 1 EC	0.103%	17:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	17:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:04D		
Control 2 EC	0.101%	17:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:06D		
Control 3 EC	0.101%	17:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	17:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 05/03/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 **Calib. Date:** 10/16/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/16/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/16/2007 **Lin. No.:** 00003
Solution File No.: 00226 **Soln. Date:** 04/06/2008 **Soln. No.:** 00042
Sequential File No.: 00226 **File Date:** 04/06/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 01/09/2010
Solution Control Lot: 08A049 **Bottle No.:** 0286

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:34D		
Control 1 EC	0.101%	16:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:35D		
Control 2 EC	0.100%	16:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:36D		
Control 3 EC	0.099%	16:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: _____



Badge No.: 4029

Date: 04/06/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00004
Calibration File No.:	00196	Cert. Date:	10/16/2007
Certification File No.:	00197	Lin. Date:	10/16/2007
Linearity File No.:	00198	Soln. Date:	03/18/2008
Solution File No.:	00221	File Date:	03/18/2008
Sequential File No.:	00221		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	06E033	Expires:	05/08/2008
		Bottle No.:	0622

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:53S		
Control 1 EC	0.101%	09:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	09:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55S		
Control 2 EC	0.100%	09:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56S		
Control 3 EC	0.100%	09:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Benjamin P. Lombi III*

Badge No.: 4019

Date: 03/18/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00196	Calib. Date: 10/16/2007
Certification File No.:	00197	Calib. No.: 00004
Linearity File No.:	00198	Cert. Date: 10/16/2007
Solution File No.:	00218	Cert. No.: 00003
Sequential File No.:	00218	Lin. Date: 10/16/2007
		Lin. No.: 00003
		Soln. Date: 02/20/2008
		Soln. No.: 00040
		File Date: 02/20/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	06E033	Expires: 05/08/2008
		Bottle No.: 0601

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:11S		
Control 1 EC	0.102%	17:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:12S		
Control 2 EC	0.100%	17:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:14S		
Control 3 EC	0.100%	17:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: _____

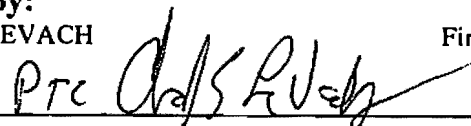

Badge No.: 4029

Date: 02/20/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 Calib. Date: 10/16/2007 Calib. No.: 00004
Certification File No.: 00197 Cert. Date: 10/16/2007 Cert. No.: 00003
Linearity File No.: 00198 Lin. Date: 10/16/2007 Lin. No.: 00003
Solution File No.: 00212 Soln. Date: 01/25/2008 Soln. No.: 00038
Sequential File No.: 00212 File Date: 01/25/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 05/08/2008
Solution Control Lot: 06E033 Bottle No.: 0617

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:44S		
Control 1 EC	0.102%	02:45S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	02:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:45S		
Control 2 EC	0.100%	02:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:47S		
Control 3 EC	0.101%	02:47S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	02:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 01/25/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 **Calib. Date:** 10/16/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/16/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/16/2007 **Lin. No.:** 00003
Solution File No.: 00211 **Soln. Date:** 12/30/2007 **Soln. No.:** 00037
Sequential File No.: 00211 **File Date:** 12/30/2007

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 05/08/2008
Solution Control Lot: 06E033 **Bottle No.:** 0625

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:50S		
Control 1 EC	0.100%	13:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51S		
Control 2 EC	0.099%	13:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:52S		
Control 3 EC	0.101%	13:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Det Benjamin Palombi III*

Badge No.: 4019

Date: 12/30/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 **Calib. Date:** 10/16/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/16/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/16/2007 **Lin. No.:** 00003
Solution File No.: 00206 **Soln. Date:** 12/03/2007 **Soln. No.:** 00036
Sequential File No.: 00206 **File Date:** 12/03/2007

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 05/08/2008
Solution Control Lot: 06E033 **Bottle No.:** 0621

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:19S		
Control 1 EC	0.101%	14:19S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:20S		
Control 2 EC	0.100%	14:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:21S		
Control 3 EC	0.101%	14:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-293 wne

Changed By:

Last Name: CROSS

First Name: WILLIAM

MI: M

Signature: TPR. I WILLIAM CROSS #5342

Badge No.: 5342

Date: 12/03/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00196 Calib. Date: 10/16/2007 Calib. No.: 00004
Certification File No.: 00197 Cert. Date: 10/16/2007 Cert. No.: 00003
Linearity File No.: 00198 Lin. Date: 10/16/2007 Lin. No.: 00003
Solution File No.: 00203 Soln. Date: 11/13/2007 Soln. No.: 00035
Sequential File No.: 00203 File Date: 11/13/2007

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 05/08/2008
Solution Control Lot: 06E033 Bottle No.: 0607

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:35S		
Control 1 EC	0.100%	08:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:36S		
Control 2 EC	0.099%	08:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:37S		
Control 3 EC	0.099%	08:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

Signature: 

Badge No.: 4028

Date: 11/13/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00004
Calibration File No.:	00196	Cert. Date:	10/16/2007
Certification File No.:	00197	Lin. Date:	10/16/2007
Linearity File No.:	00198	Soln. Date:	10/16/2007
Solution File No.:	00199	File Date:	10/16/2007
Sequential File No.:	00199		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	06E033	Expires:	05/08/2008
		Bottle No.:	0612

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:48D		
Control 1 EC	0.100%	10:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:49D		
Control 2 EC	0.099%	10:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:51D		
Control 3 EC	0.099%	10:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-144 WR

Changed By:

Last Name: CROSS	First Name: WILLIAM	MI: M
Signature: <u>TPR. I WILLIAM. Cross #5342</u>	Badge No.: 5342	Date: 10/16/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 Calib. Date: 10/17/2006 Calib. No.: 00003
Certification File No.: 00097 Cert. Date: 10/17/2006 Cert. No.: 00002
Linearity File No.: 00098 Lin. Date: 10/17/2006 Lin. No.: 00002
Solution File No.: 00195 Soln. Date: 10/12/2007 Soln. No.: 00033
Sequential File No.: 00195 File Date: 10/12/2007

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 05/08/2008
Solution Control Lot: 06E033 Bottle No.: 0623

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:38D		
Control 1 EC	0.098%	13:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:39D		
Control 2 EC	0.097%	13:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:40D		
Control 3 EC	0.098%	13:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	13:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: Sgt Benjamin Palombi III

Badge No.: 4019

Date: 10/12/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00096	Calib. Date:	10/17/2006
Certification File No.:	00097	Cert. Date:	10/17/2006
Linearity File No.:	00098	Lin. Date:	10/17/2006
Solution File No.:	00191	Soln. Date:	09/25/2007
Sequential File No.:	00191	File Date:	09/25/2007
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	06E033	Expires:	05/08/2008
		Bottle No.:	0613

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:36D		
Control 1 EC	0.100%	03:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:37D		
Control 2 EC	0.098%	03:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:38D		
Control 3 EC	0.098%	03:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:39D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 09/25/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00096	Calib. Date: 10/17/2006
Certification File No.:	00097	Calib. No.: 00003
Linearity File No.:	00098	Cert. Date: 10/17/2006
Solution File No.:	00185	Cert. No.: 00002
Sequential File No.:	00185	Lin. Date: 10/17/2006
		Lin. No.: 00002
		Soln. Date: 09/13/2007
		Soln. No.: 00031
		File Date: 09/13/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	06E033	Expires: 05/08/2008
		Bottle No.: 0603

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:44D		
Control 1 EC	0.098%	21:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:45D		
Control 2 EC	0.097%	21:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	21:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:46D		
Control 3 EC	0.098%	21:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Ben Palombi III*

Badge No.: 4019

Date: 09/13/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 **Calib. Date:** 10/17/2006 **Calib. No.:** 00003
Certification File No.: 00097 **Cert. Date:** 10/17/2006 **Cert. No.:** 00002
Linearity File No.: 00098 **Lin. Date:** 10/17/2006 **Lin. No.:** 00002
Solution File No.: 00182 **Soln. Date:** 08/15/2007 **Soln. No.:** 00030
Sequential File No.: 00182 **File Date:** 08/15/2007

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 05/08/2008
Solution Control Lot: 06E033 **Bottle No.:** 0618

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:49D		
Control 1 EC	0.098%	22:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:51D		
Control 2 EC	0.097%	22:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	22:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:52D		
Control 3 EC	0.097%	22:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	22:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: 

Badge No.: 4016

Date: 08/15/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00096	Calib. Date:	10/17/2006
Certification File No.:	00097	Cert. No.:	00003
Linearity File No.:	00098	Cert. Date:	10/17/2006
Solution File No.:	00178	Lin. Date:	10/17/2006
Sequential File No.:	00178	Lin. No.:	00002
		Soln. Date:	07/20/2007
		Soln. No.:	00029
		File Date:	07/20/2007
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	06E033	Expires:	05/08/2008
		Bottle No.:	0624

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:12D		
Control 1 EC	0.097%	02:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:13D		
Control 2 EC	0.097%	02:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:14D		
Control 3 EC	0.097%	02:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BUNCE

First Name: JOHN

MI: A

Signature: 

Badge No.: 4027

Date: 07/20/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 **Calib. Date:** 10/17/2006 **Calib. No.:** 00003
Certification File No.: 00097 **Cert. Date:** 10/17/2006 **Cert. No.:** 00002
Linearity File No.: 00098 **Lin. Date:** 10/17/2006 **Lin. No.:** 00002
Solution File No.: 00171 **Soln. Date:** 06/22/2007 **Soln. No.:** 00028
Sequential File No.: 00171 **File Date:** 06/22/2007

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 05/08/2008
Solution Control Lot: 06E033 **Bottle No.:** 0608

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:15D		
Control 1 EC	0.100%	04:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:16D		
Control 2 EC	0.098%	04:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:18D		
Control 3 EC	0.098%	04:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	04:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 06/22/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00096	Calib. Date: 10/17/2006
Certification File No.:	00097	Calib. No.: 00003
Linearity File No.:	00098	Cert. Date: 10/17/2006
Solution File No.:	00164	Cert. No.: 00002
Sequential File No.:	00164	Lin. Date: 10/17/2006
		Lin. No.: 00002
		Soln. Date: 05/27/2007
		Soln. No.: 00027
		File Date: 05/27/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	06E033	Expires: 05/08/2008
		Bottle No.: 0614

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:02D		
Control 1 EC	0.099%	20:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:04D		
Control 2 EC	0.098%	20:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	20:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:05D		
Control 3 EC	0.098%	20:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BUNCE

First Name: JOHN

MI: A

Signature: _____

Sgt J. A. R.

Badge No.: 4027

Date: 05/27/2007

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 Calib. Date: 10/17/2006 Calib. No.: 00003
Certification File No.: 00097 Cert. Date: 10/17/2006 Cert. No.: 00002
Linearity File No.: 00098 Lin. Date: 10/17/2006 Lin. No.: 00002
Solution File No.: 00155 Soln. Date: 04/30/2007 Soln. No.: 00026
Sequential File No.: 00155 File Date: 04/30/2007

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 05/08/2008
Solution Control Lot: 06E033 Bottle No.: 0609

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:29D		
Control 1 EC	0.098%	21:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:30D		
Control 2 EC	0.098%	21:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	21:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:31D		
Control 3 EC	0.098%	21:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: Sgt Ben Palombi III

Badge No.: 4019

Date: 04/30/2007

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 Calib. Date: 10/17/2006 Calib. No.: 00003
Certification File No.: 00097 Cert. Date: 10/17/2006 Cert. No.: 00002
Linearity File No.: 00098 Lin. Date: 10/17/2006 Lin. No.: 00002
Solution File No.: 00146 Soln. Date: 04/03/2007 Soln. No.: 00025
Sequential File No.: 00146 File Date: 04/03/2007

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 05/08/2008
Solution Control Lot: 06E033 Bottle No.: 0605

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:36D		
Control 1 EC	0.098%	01:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:37D		
Control 2 EC	0.096%	01:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:38D		
Control 3 EC	0.096%	01:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	01:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: _____

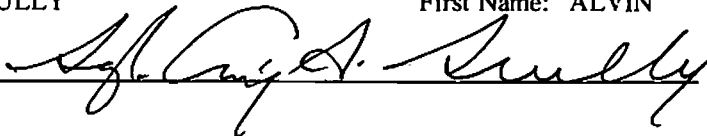

Badge No.: 4016

Date: 04/03/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 **Calib. Date:** 10/17/2006 **Calib. No.:** 00003
Certification File No.: 00097 **Cert. Date:** 10/17/2006 **Cert. No.:** 00002
Linearity File No.: 00098 **Lin. Date:** 10/17/2006 **Lin. No.:** 00002
Solution File No.: 00138 **Soln. Date:** 03/18/2007 **Soln. No.:** 00024
Sequential File No.: 00138 **File Date:** 03/18/2007

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 05/08/2008
Solution Control Lot: 06E033 **Bottle No.:** 0615

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:06S		
Control 1 EC	0.099%	12:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		
Control 2 EC	0.097%	12:08S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:09S		
Control 3 EC	0.097%	12:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Det Benjamin Palombi JT*

Badge No.: 4019

Date: 03/18/2007

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00096 **Calib. Date:** 10/17/2006 **Calib. No.:** 00003
Certification File No.: 00097 **Cert. Date:** 10/17/2006 **Cert. No.:** 00002
Linearity File No.: 00098 **Lin. Date:** 10/17/2006 **Lin. No.:** 00002
Solution File No.: 00135 **Soln. Date:** 02/19/2007 **Soln. No.:** 00023
Sequential File No.: 00135 **File Date:** 02/19/2007

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 05/08/2008
Solution Control Lot: 06E033 **Bottle No.:** 0610

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:30S		
Control 1 EC	0.100%	09:31S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		
Control 2 EC	0.099%	09:32S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33S		
Control 3 EC	0.099%	09:34S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Benjamin Palombi*

Badge No.: 4019

Date: 02/19/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00003
Calibration File No.:	00096	Calib. Date:	10/17/2006
Certification File No.:	00097	Cert. Date:	10/17/2006
Linearity File No.:	00098	Lin. Date:	10/17/2006
Solution File No.:	00128	Soln. Date:	01/22/2007
Sequential File No.:	00128	File Date:	01/22/2007
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	05F019	Expires:	06/03/2007
		Bottle No.:	0656

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:05S		
Control 1 EC	0.099%	10:06S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		
Control 2 EC	0.097%	10:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08S		
Control 3 EC	0.098%	10:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-144 WIR

Changed By:

Last Name: CROSS	First Name: WILLIAM	MI: M
Signature: <u><i>TPR. I WILLIAM CROSS #5342</i></u>	Badge No.: 5342	Date: 01/22/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00096	Calib. Date:	10/17/2006
Certification File No.:	00097	Cert. No.:	00003
Linearity File No.:	00098	Cert. Date:	10/17/2006
Solution File No.:	00121	Lin. No.:	00002
Sequential File No.:	00121	Lin. Date:	10/17/2006
		Soln. No.:	00021
		Soln. Date:	01/11/2007
		File Date:	01/11/2007
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	05F019	Expires:	06/03/2007
		Bottle No.:	0667

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:16S		
Control 1 EC	0.098%	20:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:18S		
Control 2 EC	0.097%	20:18S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	20:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:19S		
Control 3 EC	0.098%	20:19S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: _____

Sgt Ben Palombi III

Badge No.: 4019

Date: 01/11/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00096	Calib. Date: 10/17/2006
Certification File No.:	00097	Cert. No.: 00003
Linearity File No.:	00098	Cert. No.: 00002
Solution File No.:	00112	Lin. Date: 10/17/2006
Sequential File No.:	00112	Lin. No.: 00002
		Soln. Date: 12/13/2006
		Soln. No.: 00020
		File Date: 12/13/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0668

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:09S		
Control 1 EC	0.099%	04:10S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:10S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:10S		
Control 2 EC	0.099%	04:11S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:12S		
Control 3 EC	0.099%	04:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Det Ben Palombi III*

Badge No.: 4019

Date: 12/13/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00096	Calib. Date:	10/17/2006
Certification File No.:	00097	Cert. No.:	00003
Linearity File No.:	00098	Lin. No.:	00002
Solution File No.:	00099	Soln. No.:	00017
Sequential File No.:	00099	File Date:	10/17/2006
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	06E033	Expires:	05/08/2008
		Bottle No.:	0620

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:34D		
Control 1 EC	0.100%	11:35D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:36D		
Control 2 EC	0.099%	11:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:37D		
Control 3 EC	0.098%	11:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-293 WME

Changed By:

Last Name: CROSS

First Name: WILLIAM

MI: M

Signature: *TPR. I WILL M. Cross #5342*

Badge No.: 5342

Date: 10/17/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Calib. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00094	Cert. No.: 00001
Sequential File No.:	00094	Lin. Date: 10/21/2005
		Lin. No.: 00001
		Soln. Date: 09/25/2006
		Soln. No.: 00016
		File Date: 09/25/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0652

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:39D		
Control 1 EC	0.098%	21:40D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	21:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:40D		
Control 2 EC	0.097%	21:41D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	21:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:42D		
Control 3 EC	0.097%	21:42D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Benjamin Palombi III*

Badge No.: 4019

Date: 09/25/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00091 **Soln. Date:** 08/27/2006 **Soln. No.:** 00015
Sequential File No.: 00091 **File Date:** 08/27/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0834

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:59D		
Control 1 EC	0.096%	09:59D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00D		
Control 2 EC	0.097%	10:00D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:01D		
Control 3 EC	0.097%	10:02D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: Sgt Ben Palombi III

Badge No.: 4019

Date: 08/27/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Calib. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00082	Cert. No.: 00001
Sequential File No.:	00082	Lin. Date: 10/21/2005
		Lin. No.: 00001
		Soln. Date: 07/30/2006
		Soln. No.: 00014
		File Date: 07/30/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0669

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:30D		
Control 1 EC	0.098%	21:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:32D		
Control 2 EC	0.097%	21:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	21:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:33D		
Control 3 EC	0.098%	21:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Benjamin Palombi III*

Badge No.: 4019

Date: 07/30/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Cert. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00075	Lin. No.: 00001
Sequential File No.:	00075	Lin. Date: 10/21/2005
		Soln. No.: 00013
		Soln. Date: 07/01/2006
		File Date: 07/01/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0672

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:53D		
Control 1 EC	0.099%	04:53D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:54D		
Control 2 EC	0.098%	04:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:55D		
Control 3 EC	0.098%	04:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	04:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: _____

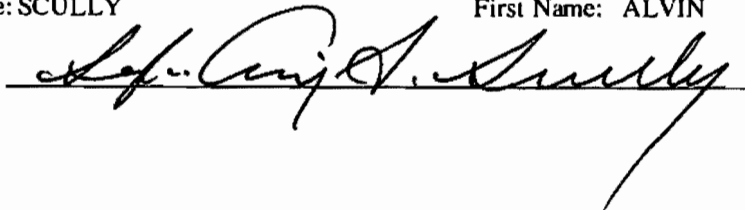

Badge No.: 4016

Date: 07/01/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Calib. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00070	Cert. No.: 00001
Sequential File No.:	00070	Lin. Date: 10/21/2005
		Lin. No.: 00001
		Soln. Date: 06/02/2006
		Soln. No.: 00012
		File Date: 06/02/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0651

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:18D		
Control 1 EC	0.097%	09:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19D		
Control 2 EC	0.097%	09:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		
Control 3 EC	0.097%	09:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: *Sgt Benjamin Palombi III*

Badge No.: 4019

Date: 06/02/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00062 **Soln. Date:** 05/12/2006 **Soln. No.:** 00011
Sequential File No.: 00062 **File Date:** 05/12/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0660

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:36D		
Control 1 EC	0.099%	20:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38D		
Control 2 EC	0.098%	20:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:39D		
Control 3 EC	0.098%	20:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature:

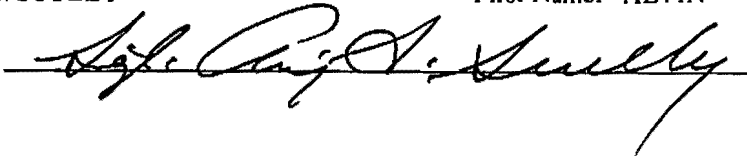

Badge No.: 4016

Date: 05/12/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00057 **Soln. Date:** 04/13/2006 **Soln. No.:** 00010
Sequential File No.: 00057 **File Date:** 04/13/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0665

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:34D		
Control 1 EC	0.099%	10:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35D		
Control 2 EC	0.097%	10:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:37D		
Control 3 EC	0.098%	10:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FAZEKAS

First Name: STEPHEN

MI: C

Signature: _____



Badge No.: 4021

Date: 04/13/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00051 **Soln. Date:** 03/25/2006 **Soln. No.:** 00009
Sequential File No.: 00051 **File Date:** 03/25/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0661

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:08S		
Control 1 EC	0.099%	07:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:09S		
Control 2 EC	0.099%	07:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:10S		
Control 3 EC	0.098%	07:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PALOMBI

First Name: BENJAMIN

MI: -

Signature: Sgt Benjamin Palombi III

Badge No.: 4019

Date: 03/25/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Calib. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00042	Cert. No.: 00001
Sequential File No.:	00042	Lin. Date: 10/21/2005
		Lin. No.: 00001
		Soln. Date: 02/23/2006
		Soln. No.: 00008
		File Date: 02/23/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0673

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:06S		
Control 1 EC	0.099%	16:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:07S		
Control 2 EC	0.098%	16:08S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:09S		
Control 3 EC	0.099%	16:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature:

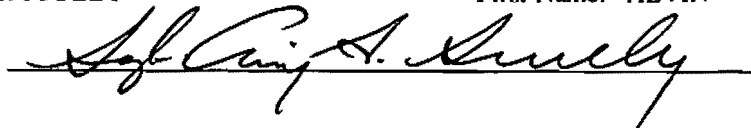

Badge No.: 4016

Date: 02/23/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Calib. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00036	Cert. No.: 00001
Sequential File No.:	00036	Lin. Date: 10/21/2005
		Lin. No.: 00001
		Soln. Date: 01/24/2006
		Soln. No.: 00007
		File Date: 01/24/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0670

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:24S		
Control 1 EC	0.099%	19:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:25S		
Control 2 EC	0.097%	19:26S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:27S		
Control 3 EC	0.097%	19:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:28S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: _____

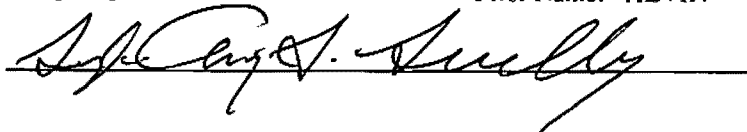

Badge No.: 4016

Date: 01/24/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00023 **Soln. Date:** 12/28/2005 **Soln. No.:** 00006
Sequential File No.: 00023 **File Date:** 12/28/2005

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0666

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:38S		
Control 1 EC	0.100%	12:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:40S		
Control 2 EC	0.099%	12:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41S		
Control 3 EC	0.099%	12:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:42S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BOLDIZAR

First Name: BRIAN

MI: A

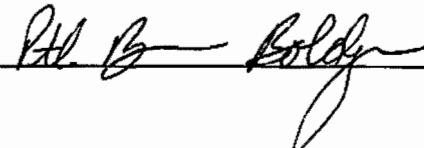Signature: 

Badge No.: 4028

Date: 12/28/2005

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00022 **Soln. Date:** 12/25/2005 **Soln. No.:** 00005
Sequential File No.: 00022 **File Date:** 12/25/2005

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0671

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:45S		
Control 1 EC	0.101%	12:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:47S		
Control 2 EC	0.099%	12:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:48S		
Control 3 EC	0.099%	12:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: _____

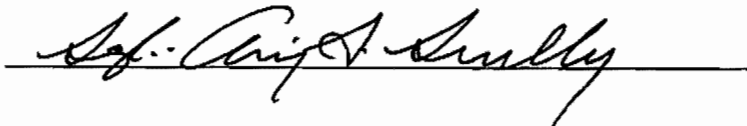

Badge No.: 4016

Date: 12/25/2005

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00002
Calibration File No.:	00009	Cert. Date:	10/21/2005
Certification File No.:	00010	Lin. Date:	10/21/2005
Linearity File No.:	00011	Soln. Date:	12/17/2005
Solution File No.:	00020	File Date:	12/17/2005
Sequential File No.:	00020		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	05F019	Expires:	06/03/2007
		Bottle No.:	0675

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:28S		
Control 1 EC	0.101%	09:29S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		
Control 2 EC	0.100%	09:30S	33.8°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:30S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		
Control 3 EC	0.099%	09:32S	33.8°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:32S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: _____

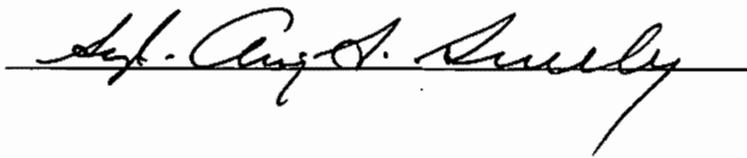

Badge No.: 4016

Date: 12/17/2005

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00009 **Calib. Date:** 10/21/2005 **Calib. No.:** 00002
Certification File No.: 00010 **Cert. Date:** 10/21/2005 **Cert. No.:** 00001
Linearity File No.: 00011 **Lin. Date:** 10/21/2005 **Lin. No.:** 00001
Solution File No.: 00016 **Soln. Date:** 11/18/2005 **Soln. No.:** 00003
Sequential File No.: 00016 **File Date:** 11/18/2005

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 06/03/2007
Solution Control Lot: 05F019 **Bottle No.:** 0674

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:39S		
Control 1 EC	0.098%	01:40S	33.8°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:40S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:40S		
Control 2 EC	0.098%	01:41S	33.8°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:41S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:41S		
Control 3 EC	0.098%	01:42S	33.8°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:42S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCULLY

First Name: ALVIN

MI: G

Signature: 

Badge No.: 4016

Date: 11/18/2005

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 10/21/2005
Certification File No.:	00010	Calib. No.: 00002
Linearity File No.:	00011	Cert. Date: 10/21/2005
Solution File No.:	00012	Cert. No.: 00001
Sequential File No.:	00012	Lin. Date: 10/21/2005
		Lin. No.: 00001
		Soln. Date: 10/21/2005
		Soln. No.: 00002
		File Date: 10/21/2005
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	05F019	Expires: 06/03/2007
		Bottle No.: 0664

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:18D		
Control 1 EC	0.100%	11:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		
Control 2 EC	0.099%	11:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20D		
Control 3 EC	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CROSS	First Name: WILLIAM	MI: M
Signature: <u>TPR. I WILLIAM M. CROSS #5342</u>	Badge No.: 5342	Date: 10/21/2005