

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01537	Calib. Date: 08/16/2016
Certification File No.:	01538	Calib. No.: 00027
Linearity File No.:	01539	Cert. Date: 08/16/2016
Solution File No.:	01562	Cert. No.: 00022
Sequential File No.:	01562	Lin. Date: 08/16/2016
		Lin. No.: 00022
		Soln. Date: 11/11/2016
		Soln. No.: 00192
		File Date: 11/11/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWH S3-0289
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0191

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:53S		
Control 1 EC	0.102%	23:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	23:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:54S		
Control 2 EC	0.101%	23:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	23:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:55S		
Control 3 EC	0.100%	23:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	23:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: _____



Badge No.: 1143

Date: 11/11/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01537	Calib. Date: 08/16/2016
Certification File No.:	01538	Calib. No.: 00027
Linearity File No.:	01539	Cert. Date: 08/16/2016
Solution File No.:	01557	Cert. No.: 00022
Sequential File No.:	01557	Lin. Date: 08/16/2016
		Lin. No.: 00022
		Soln. Date: 10/09/2016
		Soln. No.: 00191
		File Date: 10/09/2016

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWH S3-0289
Control Solution %:	0.100%		Expires: 08/04/2017
Solution Control Lot:	15H140		Bottle No.: 0197

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:03D		
Control 1 EC	0.101%	07:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	07:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:05D		
Control 2 EC	0.100%	07:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	07:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:06D		
Control 3 EC	0.101%	07:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PASCULLI

First Name: NICHOLAS

MI: P

Signature: _____

Nicholas Pasculli #1150

Badge No.: 1150

Date: 10/09/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0186
Location: FRANKLIN TOWNSHIP P.D.
Calibration File No.: 01537 Calib. Date: 08/16/2016 Calib. No.: 00027
Certification File No.: 01538 Cert. Date: 08/16/2016 Cert. No.: 00022
Linearity File No.: 01539 Lin. Date: 08/16/2016 Lin. No.: 00022
Solution File No.: 01548 Soln. Date: 09/16/2016 Soln. No.: 00190
Sequential File No.: 01548 File Date: 09/16/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0289
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0200

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:47D		
Control 1 EC	0.100%	20:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	20:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:48D		
Control 2 EC	0.101%	20:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:49D		
Control 3 EC	0.100%	20:50D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:50D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:50D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: _____

Sgt J MCGUIGAN 1143

Badge No.: 1143

Date: 09/16/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01480	Calib. Date: 02/23/2016
Certification File No.:	01481	Calib. No.: 00025
Linearity File No.:	01482	Cert. Date: 02/23/2016
Solution File No.:	01529	Cert. No.: 00021
Sequential File No.:	01529	Lin. Date: 02/23/2016
		Lin. No.: 00021
		Soln. Date: 06/15/2016
		Soln. No.: 00187
		File Date: 06/15/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWH S3-0286
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0196

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:45D		
Control 1 EC	0.101%	13:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:46D		
Control 2 EC	0.099%	13:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:48D		
Control 3 EC	0.099%	13:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JERNEGAN

First Name: DAVID

MI: A

Signature: _____

Badge No.: 1148

Date: 06/15/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01480	Calib. Date: 02/23/2016
Certification File No.:	01481	Calib. No.: 00025
Linearity File No.:	01482	Cert. Date: 02/23/2016
Solution File No.:	01519	Cert. No.: 00021
Sequential File No.:	01519	Lin. Date: 02/23/2016
		Lin. No.: 00021
		Soln. Date: 05/28/2016
		Soln. No.: 00186
		File Date: 05/28/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWH S3-0286
Control Solution %:	0.100%			Expires:	08/04/2017
Solution Control Lot:	15H140			Bottle No.:	0185

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:15D		
Control 1 EC	0.099%	22:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:16D		
Control 2 EC	0.098%	22:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:17D		
Control 3 EC	0.097%	22:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JERNEGAN

First Name: DAVID

MI: A

Signature: _____

Badge No.: 1148

Date: 05/28/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01480	Calib. Date: 02/23/2016
Certification File No.:	01481	Calib. No.: 00025
Linearity File No.:	01482	Cert. Date: 02/23/2016
Solution File No.:	01517	Cert. No.: 00021
Sequential File No.:	01517	Lin. Date: 02/23/2016
		Lin. No.: 00021
		Soln. Date: 05/27/2016
		Soln. No.: 00185
		File Date: 05/27/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWH S3-0286
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0180

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:36D		
Control 1 EC	0.098%	00:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	00:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:37D		
Control 2 EC	0.097%	00:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:39D		
Control 3 EC	0.098%	00:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MYERS

First Name: OFC. A.

MI: -

Signature: _____

OFC. A. Myers #1151

Badge No.: 1151

Date: 05/27/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.		
Calibration File No.:	01480	Calib. Date:	02/23/2016
Certification File No.:	01481	Cert. Date:	02/23/2016
Linearity File No.:	01482	Lin. Date:	02/23/2016
Solution File No.:	01515	Soln. Date:	05/19/2016
Sequential File No.:	01515	File Date:	05/19/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWH S3-0286
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	0184

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:46D		
Control 1 EC	0.099%	02:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:48D		
Control 2 EC	0.098%	02:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:49D		
Control 3 EC	0.097%	02:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:50D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: NEHER

First Name: MICHAEL

MI: E

Signature: DEC Michael Neher #1155

Badge No.: 1155

Date: 05/19/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01480	Calib. Date: 02/23/2016
Certification File No.:	01481	Calib. No.: 00025
Linearity File No.:	01482	Cert. Date: 02/23/2016
Solution File No.:	01511	Cert. No.: 00021
Sequential File No.:	01511	Lin. Date: 02/23/2016
		Lin. No.: 00021
		Soln. Date: 04/30/2016
		Soln. No.: 00183
		File Date: 04/30/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWH S3-0286
Control Solution %:	0.100%			Expires:	08/04/2017
Solution Control Lot:	15H140			Bottle No.:	0179

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:35D		
Control 1 EC	0.099%	20:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:37D		
Control 2 EC	0.098%	20:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38D		
Control 3 EC	0.098%	20:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	20:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: _____

Badge No.: 1143

Date: 04/30/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01480	Calib. Date: 02/23/2016
Certification File No.:	01481	Calib. No.: 00025
Linearity File No.:	01482	Cert. Date: 02/23/2016
Solution File No.:	01508	Cert. No.: 00021
Sequential File No.:	01508	Lin. Date: 02/23/2016
		Lin. No.: 00021
		Soln. Date: 04/20/2016
		Soln. No.: 00182
		File Date: 04/20/2016

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWH S3-0286
Control Solution %:	0.100%		Expires: 08/04/2017
Solution Control Lot:	15H140		Bottle No.: 0176

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:19D		
Control 1 EC	0.101%	10:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		
Control 2 EC	0.101%	10:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22D		
Control 3 EC	0.100%	10:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: _____

Sgt J MCG 1143

Badge No.: 1143

Date: 04/20/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01480	Calib. No.: 00025
Certification File No.:	01481	Cert. No.: 00021
Linearity File No.:	01482	Lin. No.: 00021
Solution File No.:	01498	Soln. No.: 00181
Sequential File No.:	01498	
	Calib. Date: 02/23/2016	
	Cert. Date: 02/23/2016	
	Lin. Date: 02/23/2016	
	Soln. Date: 03/20/2016	
	File Date: 03/20/2016	
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWH S3-0286
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0178

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:14S		
Control 1 EC	0.099%	04:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	04:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:16S		
Control 2 EC	0.098%	04:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	04:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:17S		
Control 3 EC	0.098%	04:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	04:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: NEHER

First Name: MICHAEL

MI: E

Signature: _____

Off. Michael Neher #1155

Badge No.: 1155

Date: 03/20/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	Calib. No.:	00025
Calibration File No.:	01480	Calib. Date:	02/23/2016
Certification File No.:	01481	Cert. Date:	02/23/2016
Linearity File No.:	01482	Lin. Date:	02/23/2016
Solution File No.:	01493	Soln. Date:	03/17/2016
Sequential File No.:	01493	File Date:	03/17/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWH S3-0286
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	0188

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:39S		
Control 1 EC	0.100%	10:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 2 EC	0.098%	10:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42S		
Control 3 EC	0.099%	10:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MULLER

First Name: GORDON

MI: H

Signature: Sgt. G. Muller #1135

Badge No.: 1135

Date: 03/17/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0186
Location: FRANKLIN TOWNSHIP P.D.
Calibration File No.: 01433 Calib. Date: 09/10/2015 Calib. No.: 00024
Certification File No.: 01434 Cert. Date: 09/10/2015 Cert. No.: 00020
Linearity File No.: 01435 Lin. Date: 09/10/2015 Lin. No.: 00020
Solution File No.: 01479 Soln. Date: 02/16/2016 Soln. No.: 00178
Sequential File No.: 01479 File Date: 02/16/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0286
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0183

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:01S		
Control 1 EC	0.101%	21:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:03S		
Control 2 EC	0.099%	21:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:04S		
Control 3 EC	0.099%	21:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: NEHER First Name: MICHAEL MI: E

Signature: Off. Michael Neher #1155 Badge No.: 1155
Date: 02/16/2016

Signature: Off. Michael Neher #1155 Date: 02/16/2016

Calibrating Unit

New Standard Solution Report

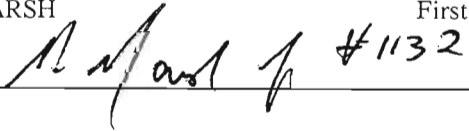

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.		
Calibration File No.:	01433	Calib. Date:	09/10/2015
Certification File No.:	01434	Cert. Date:	09/10/2015
Linearity File No.:	01435	Lin. Date:	09/10/2015
Solution File No.:	01473	Soln. Date:	02/08/2016
Sequential File No.:	01473	File Date:	02/08/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%		Serial No.:
Solution Control Lot:	15H140		DDWH S3-0286
			Expires: 08/04/2017
			Bottle No.: 0177

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:13S		
Control 1 EC	0.102%	18:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:15S		
Control 2 EC	0.101%	18:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:16S		
Control 3 EC	0.100%	18:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MARSH	First Name: MICHAEL	MI: J
Signature: <u></u>	Badge No.: 1132	Date: 02/08/2016
Signature: <u></u>	Badge No.: 1132	Date: 02/08/2016

Calibrating Unit

New Standard Solution Report

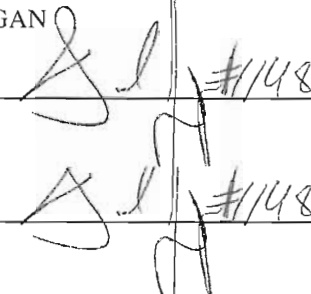

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0186
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	01433	Calib. Date: 09/10/2015
Certification File No.:	01434	Cert. No.: 00024
Linearity File No.:	01435	Cert. Date: 09/10/2015
Solution File No.:	01467	Lin. Date: 09/10/2015
Sequential File No.:	01467	Lin. No.: 00020
		Soln. Date: 01/06/2016
		Soln. No.: 00176
		File Date: 01/06/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWH S3-0286
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0186

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:23S		
Control 1 EC	0.101%	14:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:24S		
Control 2 EC	0.100%	14:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:26S		
Control 3 EC	0.099%	14:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JERNEGAN	First Name: DAVID	MI: A
Signature: _____		Badge No.: 1148
		Date: 01/06/2016
Signature: _____		Badge No.: 1148
		Date: 01/06/2016