

Buena
Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXB-0074
Location: FRANKLIN TOWNSHIP P.D.
Calibration File No.: 00528 Calib. Date: 10/04/2021 Calib. No.: 00037
Certification File No.: 00529 Cert. Date: 10/04/2021 Cert. No.: 00030
Linearity File No.: 00530 Lin. Date: 10/04/2021 Lin. No.: 00030
Solution File No.: 00537 Soln. Date: 11/21/2021 Soln. No.: 00173
Sequential File No.: 00537 File Date: 11/21/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXJ S3-0210
Control Solution %: 0.100% Expires: 03/17/2023
Solution Control Lot: 21090 Bottle No.: 0724

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:46S		
Control 1 EC	0.097%	08:46S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	08:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47S		
Control 2 EC	0.096%	08:47S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:47S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:48S		
Control 3 EC	0.096%	08:49S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: _____



Badge No.: 1143

Date: 11/21/2021

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXB-0074
Location: FRANKLIN TOWNSHIP P.D.
Calibration File No.: 00528 Calib. Date: 10/04/2021 Calib. No.: 00037
Certification File No.: 00529 Cert. Date: 10/04/2021 Cert. No.: 00030
Linearity File No.: 00530 Lin. Date: 10/04/2021 Lin. No.: 00030
Solution File No.: 00534 Soln. Date: 10/29/2021 Soln. No.: 00172
Sequential File No.: 00534 File Date: 10/29/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXJ S3-0210
Control Solution %: 0.100% Expires: 03/17/2023
Solution Control Lot: 21090 Bottle No.: 0098

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:46D		
Control 1 EC	0.097%	22:46D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	22:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:47D		
Control 2 EC	0.098%	22:47D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	22:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:48D		
Control 3 EC	0.097%	22:49D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	22:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GUZMAN

First Name: MICHAEL

MI: C

Signature: _____

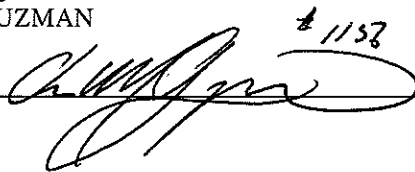

Badge No.: 1156

Date: 10/29/2021

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXB-0074
Location: FRANKLIN TOWNSHIP P.D.
Calibration File No.: 00517 Calib. Date: 04/05/2021 Calib. No.: 00036
Certification File No.: 00518 Cert. Date: 04/05/2021 Cert. No.: 00029
Linearity File No.: 00519 Lin. Date: 04/05/2021 Lin. No.: 00029
Solution File No.: 00526 Soln. Date: 09/04/2021 Soln. No.: 00170
Sequential File No.: 00526 File Date: 09/04/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBJ-0006
Control Solution %: 0.100% Expires: 03/17/2023
Solution Control Lot: 21090 Bottle No.: 0716

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:45D		
Control 1 EC	0.098%	04:45D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:46D		
Control 2 EC	0.098%	04:47D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:47D		
Control 3 EC	0.099%	04:48D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GUZMAN

First Name: MICHAEL

MI: C

Signature: _____

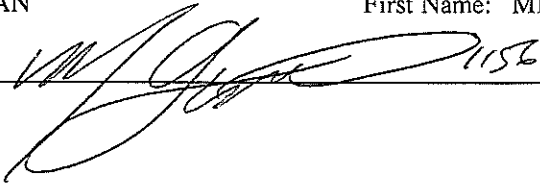

Badge No.: 1156

Date: 09/04/2021