

Buena

# Calibrating Unit New Standard Solution Report

## Equipment

Alcotest 7110 MKIII-C  
 Location: FRANKLIN TOWNSHIP P.D.  
 Calibration File No.: 00552      Calib. Date: 08/31/2022      Calib. No.: 00039  
 Certification File No.: 00553      Cert. Date: 08/31/2022      Cert. No.: 00032  
 Linearity File No.: 00554      Lin. Date: 08/31/2022      Lin. No.: 00032  
 Solution File No.: 00565      Soln. Date: 12/30/2022      Soln. No.: 00183  
 Sequential File No.: 00565      File Date: 12/30/2022

Calibrating Unit: WET      Model No.: CU-34      Serial No.: DDBJ-0006  
 Control Solution %: 0.100%      Expires: 03/17/2023  
 Solution Control Lot: 21090      Bottle No.: 0742

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:32S		
Control 1 EC	0.100%	13:32S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:33S		
Control 2 EC	0.100%	13:34S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:34S		
Control 3 EC	0.100%	13:35S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:36S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_

*Sgt Jeffrey 1143*

Badge No.: 1143

Date: 12/30/2022

# Calibrating Unit

## New Standard Solution Report

Buena

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
Location: FRANKLIN TOWNSHIP P.D.  
Calibration File No.: 00552 Calib. Date: 08/31/2022 Calib. No.: 00039  
Certification File No.: 00553 Cert. Date: 08/31/2022 Cert. No.: 00032  
Linearity File No.: 00554 Lin. Date: 08/31/2022 Lin. No.: 00032  
Solution File No.: 00562 Soln. Date: 12/02/2022 Soln. No.: 00182  
Sequential File No.: 00562 File Date: 12/02/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBJ-0006  
Control Solution %: 0.100% Expires: 03/17/2023  
Solution Control Lot: 21090 Bottle No.: 0729

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:50S		
Control 1 EC	0.101%	11:51S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		
Control 2 EC	0.100%	11:52S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53S		
Control 3 EC	0.100%	11:53S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_

Sgt/aj 1143

Badge No.: 1143

Date: 12/02/2022

# Calibrating Unit *Buena*

## New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C  
 Location: FRANKLIN TOWNSHIP P.D.  
 Calibration File No.: 00552  
 Certification File No.: 00553  
 Linearity File No.: 00554  
 Solution File No.: 00560  
 Sequential File No.: 00560

Serial No.: ARXB-0074

Calib. Date: 08/31/2022  
 Cert. Date: 08/31/2022  
 Lin. Date: 08/31/2022  
 Soln. Date: 11/04/2022  
 File Date: 11/04/2022

Calib. No.: 00039  
 Cert. No.: 00032  
 Lin. No.: 00032  
 Soln. No.: 00181

Calibrating Unit: WET  
 Control Solution %: 0.100%  
 Solution Control Lot: 21090

Model No.: CU-34

Serial No.: DDBJ-0006  
 Expires: 03/17/2023  
 Bottle No.: 0014

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:15S		
Control 1 EC	0.102%	17:16S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:16S		
Control 2 EC	0.101%	17:17S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:18S		
Control 3 EC	0.101%	17:18S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_



Badge No.: 1143

Date: 11/04/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXB-0074
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	00552	Calib. Date: 08/31/2022
Certification File No.:	00553	Calib. No.: 00039
Linearity File No.:	00554	Cert. Date: 08/31/2022
Solution File No.:	00556	Cert. No.: 00032
Sequential File No.:	00556	Lin. Date: 08/31/2022
		Lin. No.: 00032
		Soln. Date: 10/04/2022
		Soln. No.: 00180
		File Date: 10/04/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDBJ-0006
Solution Control Lot:	22110	Expires: 04/04/2024
		Bottle No.: 1292

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:56D		
Control 1 EC	0.102%	14:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57D		
Control 2 EC	0.101%	14:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:59D		
Control 3 EC	0.101%	14:59D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_



Badge No.: 1143

Date: 10/04/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXB-0074
Location:	FRANKLIN TOWNSHIP P.D.	
Calibration File No.:	00538	Calib. Date: 03/24/2022
Certification File No.:	00539	Calib. No.: 00038
Linearity File No.:	00540	Cert. Date: 03/24/2022
Solution File No.:	00550	Cert. No.: 00031
Sequential File No.:	00550	Lin. Date: 03/24/2022
		Lin. No.: 00031
		Soln. Date: 08/24/2022
		Soln. No.: 00178
		File Date: 08/24/2022

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDBJ-0006
Control Solution %: 0.100%		Expires: 04/04/2024
Solution Control Lot: 22110		Bottle No.: 0010

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:15D		
Control 1 EC	0.097%	13:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	13:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16D		
Control 2 EC	0.097%	13:17D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		
Control 3 EC	0.097%	13:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_

Badge No.: 1143

Date: 08/24/2022



- Buena -

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
 Location: FRANKLIN TOWNSHIP P.D.  
 Calibration File No.: 00538 Calib. Date: 03/24/2022 Calib. No.: 00038  
 Certification File No.: 00539 Cert. Date: 03/24/2022 Cert. No.: 00031  
 Linearity File No.: 00540 Lin. Date: 03/24/2022 Lin. No.: 00031  
 Solution File No.: 00543 Soln. Date: 06/24/2022 Soln. No.: 00176  
 Sequential File No.: 00543 File Date: 06/24/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBJ-0006  
 Control Solution %: 0.100% Expires: 04/04/2024  
 Solution Control Lot: 22110 Bottle No.: 0120

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:55D		
Control 1 EC	0.098%	17:56D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	17:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:57D		
Control 2 EC	0.098%	17:57D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:58D		
Control 3 EC	0.098%	17:59D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_

Badge No.: 1143

Date: 06/24/2022

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0074
Location:	FRANKLIN TOWNSHIP P.D.		
Calibration File No.:	00538	Calib. Date:	03/24/2022
Certification File No.:	00539	Cert. Date:	03/24/2022
Linearity File No.:	00540	Lin. Date:	03/24/2022
Solution File No.:	00542	Soln. Date:	04/22/2022
Sequential File No.:	00542	File Date:	04/22/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDBJ-0006
Solution Control Lot:	21090	Expires:	03/17/2023
		Bottle No.:	0025

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:37D		
Control 1 EC	0.100%	14:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:38D		
Control 2 EC	0.099%	14:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:40D		
Control 3 EC	0.099%	14:40D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:41D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

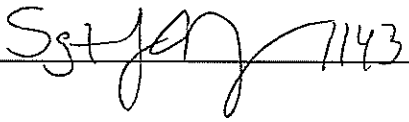Signature: 

Badge No.: 1143

Date: 04/22/2022