

ALCOTEST CHECKLIST

Municipality: LONGPORT

Alcotest Ser.#: ARXA - 0067

County: ATLANTIC

Date of Calibration: 09-15-2016

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC S3 - 0135

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWA P2 - 199

4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 150 649672

5. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDLH P1 - 0071

6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>15</u>	<u>H</u>	<u>141</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>15</u>	<u>H</u>	<u>142</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>14</u>	<u>L</u>	<u>134</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>15</u>	<u>H</u>	<u>144</u>

7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

A. 0.04% used in Calibration/Linearity Testing. DDXD S3 - 0186
 B. 0.08% used in Calibration/Linearity Testing. DDAE - 0017
 C. 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.]
 D. 0.16% used in Calibration/Linearity Testing. DDAE - 0018

8. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 2016032
 D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


1-10-14

SERIAL NUMBER:

ARXA-00107

Draeger Safety Diagnostics, Inc.

BC



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXCS3-0135

Certification Date

7-14-16

Technician

JD

Re-Certification Due Date

7-14-17

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-199

Certification date:

7-13-16

Next Certification due:

7-13-17

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department

BC



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-7019762

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Malsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 150649672 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-256	B01375		
Temperature Probe	128	4/02/16	15-A0P2S-40-1
Thermistor Module	A17118	3/03/16	1000371058
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	3/03/16	1000371058
Temperature Probe	3039	4/02/16	15--A0P2S-20-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5202	11/19/16	6-CV9Y2-1-1
Temperature Calibration Bath TC-309	B3A444		
Thermistor Module	A27129	11/04/15	1000365407
Temperature Probe	5267	11/19/16	6-CV9Y0-1-1

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 8/31/15 Due Date: 8/31/17
 Test Conditions: 23.0°C 47.0 %RH 1017 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.001	0.000	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.000	25.003	Y	24.950	25.050	0.014	3.6:1
°C		N.A.		50.004	50.000	Y	49.954	50.054	0.014	3.6:1
°C		N.A.		100.002	99.999	Y	99.952	100.052	0.014	3.6:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-RvA.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: LONGPORT POLICE
Calibration File No.: 00794
Certification File No.: 00780
Linearity File No.: 00781
Solution File No.: 00793
Sequential File No.: 00794

Serial No.: ARXA-0067

Calib. Date: 09/15/2016 Calib. No.: 00028
Cert. Date: 04/08/2016 Cert. No.: 00021
Lin. Date: 04/08/2016 Lin. No.: 00021
Soln. Date: 08/28/2016 Soln. No.: 00191
File Date: 09/15/2016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 14L134

Model No.: CU-34

Serial No.: DDXC S3-0135
Expires: 12/04/2016
Bottle No.: 0152

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.


Signature: Tr. I K W. G #6704

Badge No.: 6704

Date: 09/15/2016

*Black Key Temperature Probe Serial.....# DALHP1-0071 (KA)

*Digital NIST Temperature Measuring System Serial.....# 150 649 672 (KA)

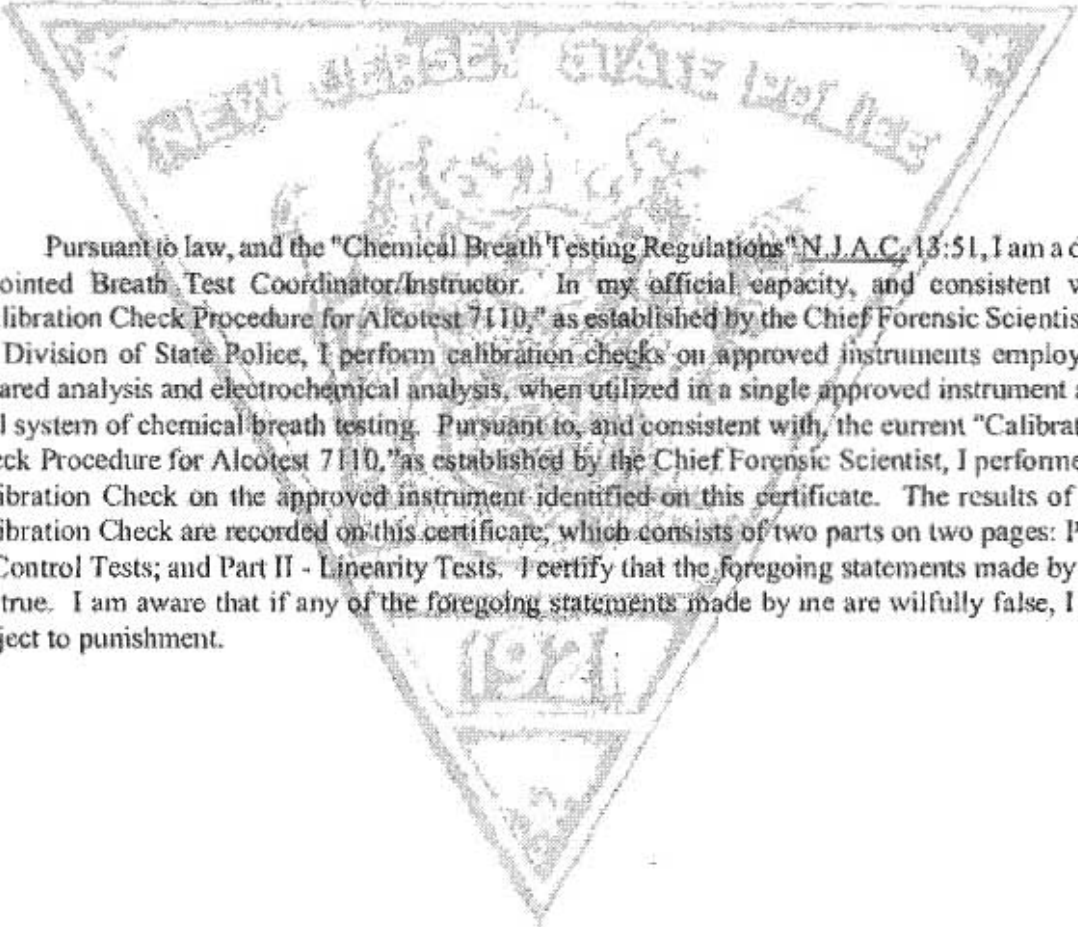

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067		
Location:	LONGPORT POLICE				
Calibration File No.:	00794	Calib. Date:	09/15/2016	Calib. No.:	00028
Certification File No.:	00795	Cert. Date:	09/15/2016	Cert. No.:	00022
Linearity File No.:	00781	Lin. Date:	04/08/2016	Lin. No.:	00021
Solution File No.:	00793	Soln. Date:	08/28/2016	Soln. No.:	00191
Sequential File No.:	00795	File Date:	09/15/2016		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXC S3-0135
Control Solution %:	0.100%			Expires:	12/04/2016
Solution Control Lot:	14L134			Bottle No.:	0152

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:55D		
Control 1 EC	0.099%	08:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56D		
Control 2 EC	0.098%	08:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:58D		
Control 3 EC	0.098%	08:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59D		

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: Tpt. J. K. W. G. #6704

Badge No.: 6704

Date: 09/15/2016

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00794 Calib. Date: 09/15/2016 Calib. No.: 00028
Certification File No.: 00795 Cert. Date: 09/15/2016 Cert. No.: 00022
Linearity File No.: 00796 Lin. Date: 09/15/2016 Lin. No.: 00022
Solution File No.: 00793 Soln. Date: 08/28/2016 Soln. No.: 00191
Sequential File No.: 00796 File Date: 09/15/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0186
Control Solution %: 0.040% Expires: 08/11/2017
Solution Control Lot: 15H141 Bottle No.: 0416

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0017
Control Solution %: 0.080% Expires: 08/13/2017
Solution Control Lot: 15H142 Bottle No.: 0748

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0018
Control Solution %: 0.160% Expires: 08/19/2017
Solution Control Lot: 15H144 Bottle No.: 0404

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:15D		
Control 1 EC	0.041%	09:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	09:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17D		
Control 2 EC	0.041%	09:18D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19D		
Control 3 EC	0.084%	09:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		
Control 4 EC	0.083%	09:22D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:24D		
Control 5 EC	0.160%	09:25D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.158%	09:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:26D		
Control 6 EC	0.160%	09:27D	33.9°C	*** TEST PASSED ***
Control 5 EC	0.160%	09:25D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.158%	09:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:26D		
Control 6 EC	0.160%	09:27D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.158%	09:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: TPF. I K W. 9 #6704

Badge No.: 6704

Date: 09/15/2016

DEPARTMENT OF
Transportation and Public Safety
Works to let us see the light

Kevin W. Alcott

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 140 OF THE LAWS OF 1966 IN THE OPERATION OF THIS ALCOHOL 7110 MKIII-C
 A METHOD TO DETERMINE INTOXICATION.
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 21st DAY OF May

TWO THOUSAND AND Fifteen

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

B.P. 2628 (Rev. 08/13)

DEPARTMENT OF
Transportation and Public Safety
Works to let us see the light

KEVIN W. ALCOTT
 NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 140 OF THE LAWS OF 1966 IN THE OPERATION OF THIS ALCOHOL 7110 MKIII-C
 A METHOD TO DETERMINE INTOXICATION.
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 18th DAY OF APRIL

TWO THOUSAND AND EIGHT

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 8-28-10	BCPA	R. J. [Signature]
2. 1-12-12	Bowers Co PA	C. [Signature]
3. 1-16-14	SAYREVILLE PA	R. J. [Signature]
4. 1/21/16	Lakewood	Dean [Signature]
5.		
6.		
7.		
8.		
9.		

B.P. 2628 (Rev. 07/07)



State of New Jersey
OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/10/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H141

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0487 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.3) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 11, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Ainaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11th day of September, 2015.

Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Soy-based Ink





State of New Jersey
OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRISTON, NJ 08628-0768
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Li. Governor

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. PUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/17/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H142

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0959 to 0.0967 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 13, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of September, 2015.

Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"
New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE

Governor

KIM GUADAÑO

Lt. Governor

JOHN J. HOFFMAN

Acting Attorney General

COLONEL JOSEPH R. FUENTES

Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 12/18/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14L134

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1205 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 04, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Aji M. Alacue]

Aji M. Alacue, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 19th day of December, 2014.

[Handwritten signature of Linda L. Desantis]
Notary

LINDA L. DESANTIS
ID # 2228599
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires August 17, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0968
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/17/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15H144

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1952 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 12, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Signature of Ali M. Alaoui, Ph.D.
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 10 day of September, 2015.

Notary Signature
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXDS3-0186

Certification Date

10-30-15

Technician

72

Re-Certification Due Date

10-30-16



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDAE-0017

Certification Date

7-1-16

Technician

BC

Re-Certification Due Date

7-1-17



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDAE-0018

Certification Date

Technician

Re-Certification Due Date

8-10-16

BC

8-10-17

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDLHP1-0071

8-10-16

8-10-17

Probe Value

103

Dräger Safety Diagnostics, Inc.
Technical Service Department

BC

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00794 Calib. Date: 09/15/2016 Calib. No.: 00028
Certification File No.: 00795 Cert. Date: 09/15/2016 Cert. No.: 00022
Linearity File No.: 00796 Lin. Date: 09/15/2016 Lin. No.: 00022
Solution File No.: 00797 Soln. Date: 09/15/2016 Soln. No.: 00192
Sequential File No.: 00797 File Date: 09/15/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 03/22/2018
Solution Control Lot: 201603L Bottle No.: 0773

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:37D		
Control 1 EC	0.099%	10:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39D		
Control 2 EC	0.098%	10:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40D		
Control 3 EC	0.099%	10:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAPZ-199 (KA)

Changed By:

Last Name: ALCOTT First Name: KEVIN MI: W.

Signature: Tr. I K W. G #6704 Badge No.: 6704
Date: 09/15/2016

Signature: Tr. I K W. G #6704 Badge No.: 6704
Date: 09/15/2016



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

ROBERT T. LOUGY
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 04/13/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 201603L

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1222 to 0.1232 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 22, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature]

Ali M. Alaotio, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 14 day of April, 2016.

[Handwritten signature]
Notary

JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

