

ALCOTEST CHECKLIST

Municipality: LONGPORT Alcotest Ser.#: ARXA-0067
County: ATLANTIC Date of Calibration: 12-01-2011

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC S3-0135
3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWA P2-199
4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 101 733 534
5. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator]
Ser. #: DDWA P2-016
6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
- | | | | | |
|--|-----------------|-----------|----------|------------|
| <input checked="" type="checkbox"/> A. | 0.04% Solution. | <u>11</u> | <u>F</u> | <u>090</u> |
| <input checked="" type="checkbox"/> B. | 0.08% Solution. | <u>11</u> | <u>F</u> | <u>091</u> |
| <input checked="" type="checkbox"/> C. | 0.10% Solution. | <u>10</u> | <u>F</u> | <u>082</u> |
| <input checked="" type="checkbox"/> D. | 0.16% Solution. | <u>11</u> | <u>G</u> | <u>092</u> |
7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
- A. 0.04% used in Calibration/Linearity Testing. DDWE S3-0196
- B. 0.08% used in Calibration/Linearity Testing. DDWE S3-0203
- C. 0.10% used in Calibration/Linearity Testing DDXC S3-0135
[Same as instrument's CU34 unit].
- D. 0.16% used in Calibration/Linearity Testing. DDWE S3-0205
8. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 10 H 081
 D. Alcotest card of operator/coordinator who completed change.

Draeger safety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705.

The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


SERIAL NUMBER:

8-10-2010

ARXA-0067

Draeger Safety Diagnostics, Inc.





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXC53-0135

Certification Date

Technician

Re-Certification Due Date

10-27-11

JS

10-27-12

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWA P2-199

10-27-11

10-27-12

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

JS



Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NC SL Z540-1



Calibration
Certificate No. 1750.01

Cert. No.: 4000-2966289

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, P.O. Box 2158, Secaucus, NJ 07094 U.S.A.

Instrument Identification:

Model: 61220-601 S/N: 101733534 Manufacturer: Control Company

Standards/Equipment:

| Description | Serial Number | Due Date | NIST Traceable Reference |
|-------------------------------------|---------------|----------|--------------------------|
| Temperature Calibration Bath TC-179 | A45240 | | |
| Thermistor Module | A17118 | 11/19/10 | A9B21010 |
| Temperature Probe | 128 | 12/10/10 | A9B23079 |
| Temperature Calibration Bath TC-231 | A79341 | | |
| Temperature Probe | 3039 | 12/10/10 | A9B23080-1 |
| Temperature Calibration Bath TC-218 | A73332 | | |
| Thermistor Module | A27129 | 7/09/10 | 1000264338 |
| Temperature Probe | 5202 | 3/11/11 | B0310050 |
| Temperature Calibration Bath TC-256 | B01375 | | |
| Temperature Probe | 157 | 7/27/10 | A9708011-4 |

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 6/08/10 Cal Due: 6/08/12
 Test Conditions: 24.0°C 42.0 %RH 1015 mBar

Calibration Data: (New Instrument)

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min | Max | ±U | TUR |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|-------|-------|
| °C | | N.A. | | 0.002 | -0.001 | Y | -0.048 | 0.052 | 0.013 | 3.8:1 |
| °C | | N.A. | | 24.999 | 25.000 | Y | 24.949 | 25.049 | 0.013 | 3.8:1 |
| °C | | N.A. | | 60.001 | 59.998 | Y | 59.951 | 60.051 | 0.018 | 2.8:1 |
| °C | | N.A. | | 100.001 | 100.002 | Y | 99.951 | 100.051 | 0.013 | 3.8:1 |

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = Nominal(Rounded) - Tolerance; Max = Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
 Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2005-AO-HOU-AWAB.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00503 Cert. Date: 07/01/2011 Cert. No.: 00010
Linearity File No.: 00504 Lin. Date: 07/01/2011 Lin. No.: 00010
Solution File No.: 00533 Soln. Date: 11/07/2011 Soln. No.: 00118
Sequential File No.: 00534 File Date: 12/01/2011

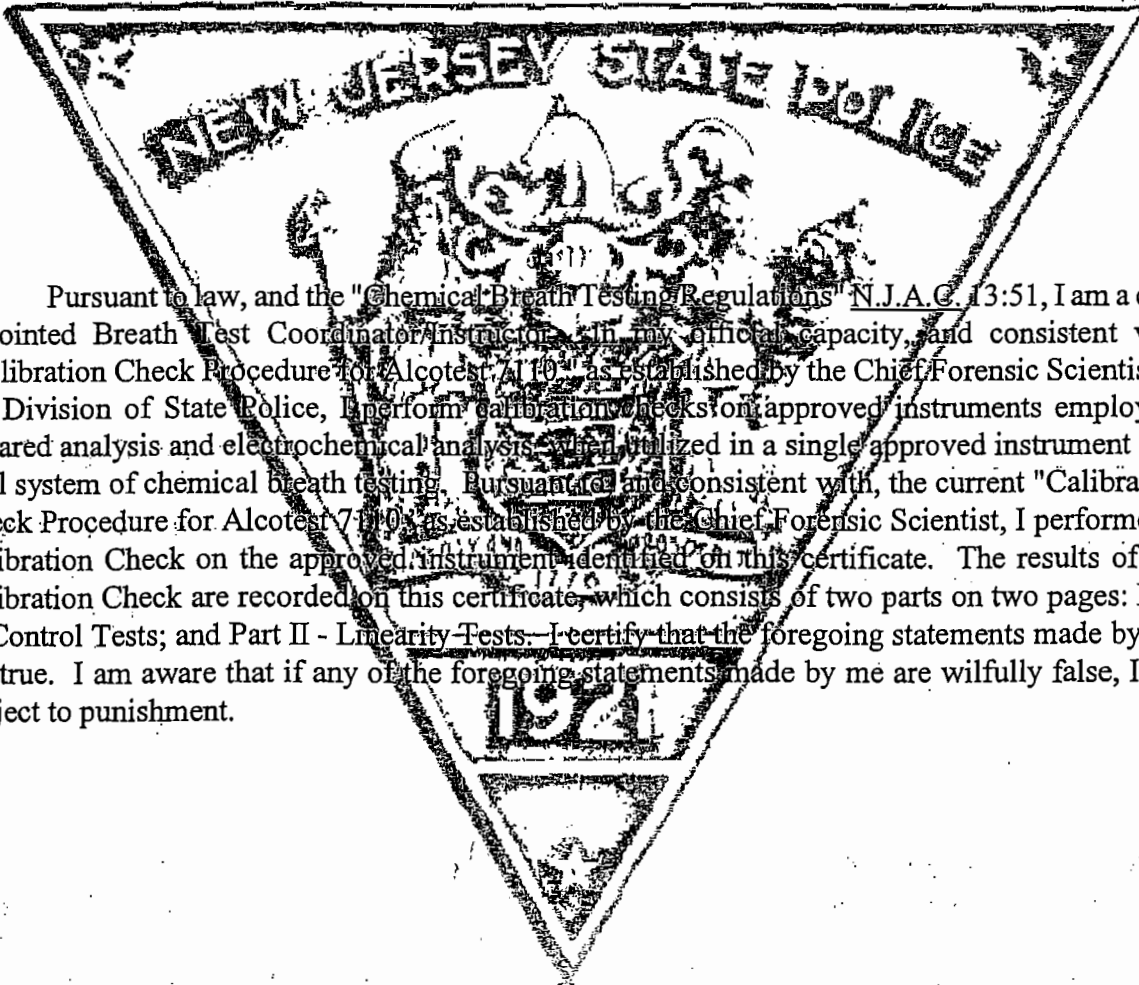
Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 09/09/2012
Solution Control Lot: 10I082 Bottle No.: 0110

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
Signature: Tpr I [Signature] # 6027 Badge No.: 6027
Date: 12/01/2011

*Black Key Temperature Probe Serial.....# DDWAP2-016 *JS*

*Digital NIST Temperature Measuring System Serial.....# 101733534 *JS*



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00504 Lin. Date: 07/01/2011 Lin. No.: 00010
Solution File No.: 00533 Soln. Date: 11/07/2011 Soln. No.: 00118
Sequential File No.: 00535 File Date: 12/01/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 09/09/2012
Solution Control Lot: 10I082 Bottle No.: 0110

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 11:25S | | |
| Control 1 EC | 0.100% | 11:26S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.098% | 11:26S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:26S | | |
| Control 2 EC | 0.098% | 11:27S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.098% | 11:27S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:28S | | |
| Control 3 EC | 0.099% | 11:28S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 11:28S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:29S | | |

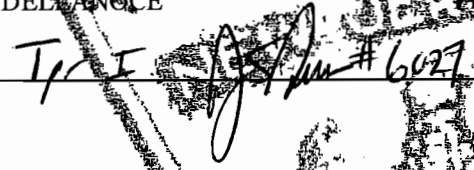
All tests within acceptable tolerance.

Coordinator

Last Name: DELANOCE

First Name: JOSEPH

Badge No.: 6027

Signature: 

Date: 12/01/2011

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00536 Lin. Date: 12/01/2011 Lin. No.: 00011
Solution File No.: 00533 Soln. Date: 11/07/2011 Soln. No.: 00118
Sequential File No.: 00536 File Date: 12/01/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0196
Control Solution %: 0.040% Expires: 06/27/2013
Solution Control Lot: 11F090 Bottle No.: 1109

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0203
Control Solution %: 0.080% Expires: 06/30/2013
Solution Control Lot: 11F091 Bottle No.: 0674

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0205
Control Solution %: 0.160% Expires: 07/03/2013
Solution Control Lot: 11G092 Bottle No.: 1014

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 11:42S | | |
| Control 1 EC | 0.041% | 11:42S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.040% | 11:42S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:44S | | |
| Control 2 EC | 0.041% | 11:44S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.039% | 11:44S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:46S | | |
| Control 3 EC | 0.081% | 11:46S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.078% | 11:46S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:48S | | |
| Control 4 EC | 0.081% | 11:48S | 34.0°C | *** TEST PASSED *** |
| Control 4 IR | 0.079% | 11:48S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:50S | | |
| Control 5 EC | 0.160% | 11:50S | 34.0°C | *** TEST PASSED *** |
| Control 5 IR | 0.158% | 11:50S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:52S | | |
| Control 6 EC | 0.161% | 11:52S | 34.0°C | *** TEST PASSED *** |
| Control 6 IR | 0.158% | 11:52S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:54S | | |

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tpc I [Signature] #6027

Badge No.: 6027

Date: 12/01/2011

DEPARTMENT OF
Law and Public Safety

Joseph S. Dellanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT COURSE AS A REFRESHER COURSE PURSUANT TO CHAPTER 10 OF
 THE LAWS OF 1986 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
 A METHOD TO DETERMINE INTOXICATION.
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND FIVE

[Signature]
 ALBERT S. BRIGHT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES


| | DATE | Refresher Course PLACE | INSTRUCTOR |
|----|---------|---------------------------|--------------|
| 1. | 2/15/07 | GCFA | C. Pottler |
| 2. | 12/7/09 | OLPA | Adam Stambor |
| 3. | 7/20/11 | STOCKTON | Adam Stambor |
| 4. | | | |
| 5. | | | |
| 6. | | | |
| 7. | | | |
| 8. | | | |
| 9. | | | |


DEPARTMENT OF
Public Safety
Office of the Attorney General

Joseph S. Dellanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 10 OF
 THE LAWS OF 1944 IN THE OPERATION OF THE Breath Test Coordinator/Instructor
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 14th DAY OF January

TWO THOUSAND AND EIGHT


 JOSEPH S. DELLANOCE
 NEW JERSEY STATE POLICE


 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course | | INSTRUCTOR |
|-------------|------------------|--|----------------|
| | PLACE | | |
| 1. 12/17/09 | DCPD | | Adam Stankovic |
| 2. 7/20/11 | STOCKTON | | Adam Stankovic |
| 3. | | | |
| 4. | | | |
| 5. | | | |
| 6. | | | |
| 7. | | | |
| 8. | | | |
| 9. | | | |

DEPARTMENT OF
Internal Public Safety

This is to certify that
Joseph B. Bellanocè
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT PHYSICAL BREATH ANALYSES PURSUANT TO CHAPTER
113 OF THE LAWS OF 1946 IN THE OPERATION OF THE **Breathalyzer**
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 13th DAY OF Dec.
TWO THOUSAND AND 01

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES: 8/30 - 9/3/99

Refresher Course

| | DATE | PLACE | INSTRUCTOR |
|----|-----------------|-----------------|--------------------|
| 1. | <u>12/12/01</u> | <u>A.G.E.C.</u> | <u>Potter</u> |
| 2. | <u>2-28-03</u> | <u>CCRA</u> | <u>C. Potter</u> |
| 3. | <u>10/3-05</u> | <u>ACTE</u> | <u>C. S. S. S.</u> |
| 4. | | | |
| 5. | | | |
| 6. | | | |
| 7. | | | |
| 8. | | | |
| 9. | | | |

SP-293B (Rev. 4/00)



JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
PO Box 080
TRENTON, NJ 08625-0080

ANNE MILGRAM
Attorney General

January 14, 2008

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -
Trooper Joseph S. Dellanoce #6027

Dear Colonel Fuentes:

Pursuant to the provisions of N.J.A.C. 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of N.J.S.A. 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Trooper Joseph S. Dellanoce #6027, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

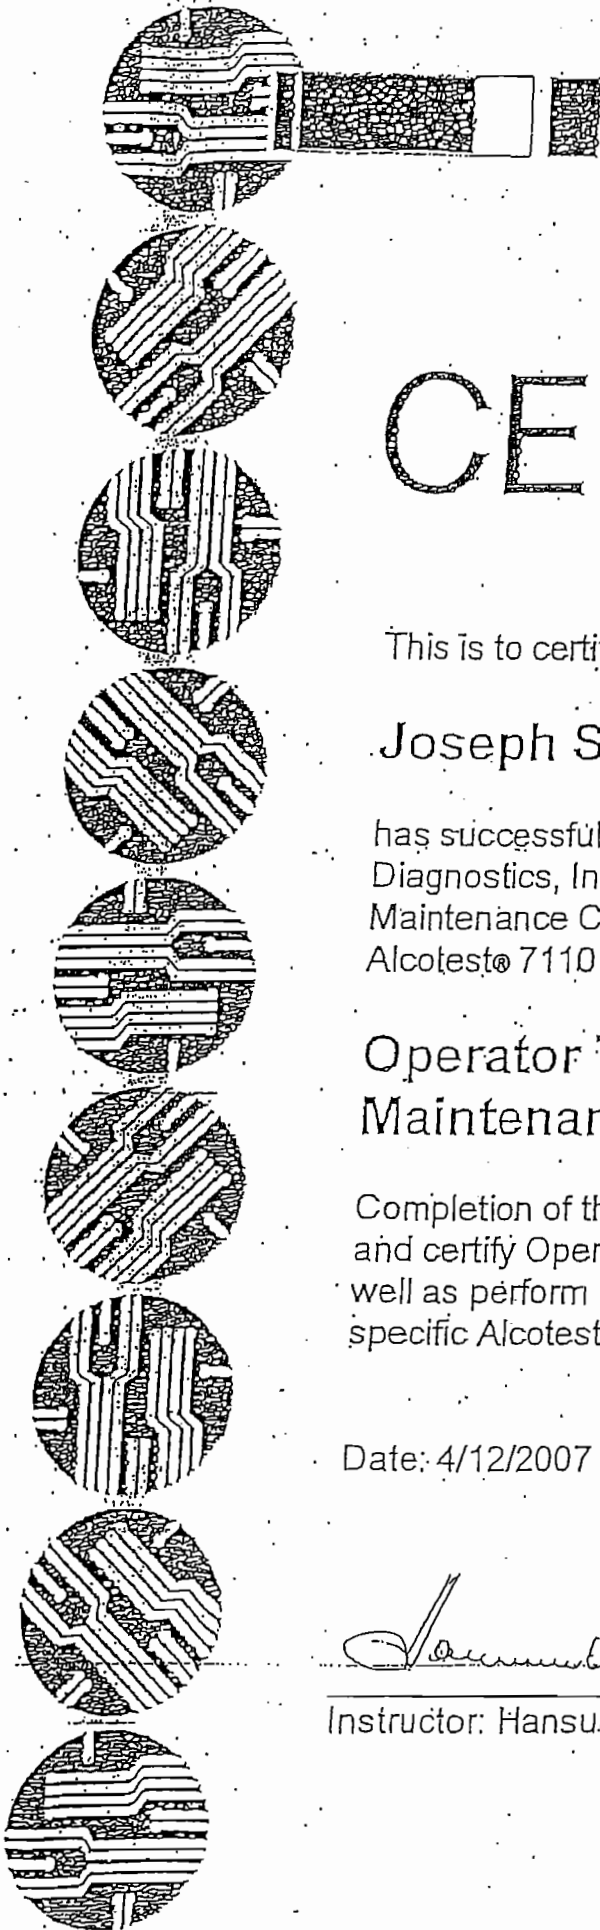
Anne Milgram
Attorney General

jk

c. Trooper Joseph S. Dellanoce #6027, Alcohol/Drug Test Unit, Division of State Police
Lt. Mark Kolodziecki, Unit Head, Alcohol/Drug Test Unit, Division of State Police



32001711



CERTIFICATE

This is to certify that

Joseph S. Dellanoce #6027

has successfully completed the two day Draeger Safety
Diagnostics, Inc. Operator Training and Preventive
Maintenance Course on the New Jersey specific
Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train
and certify Operators in the proper use and operation as
well as perform Preventive Maintenance on the New Jersey
specific Alcotest® 7110 MKIII-C.

Date: 4/12/2007

Instructor: Hansueli Rysler

Draeger



Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-016

Certification date:

February 7, 2011

Next Certification due:

February 7, 2012

Probe Value

107

Dräger Safety Diagnostics, Inc.
Technical Service Department





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

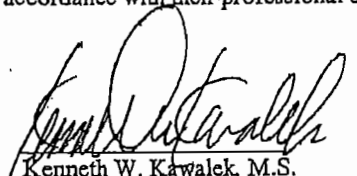
MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F090


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.


Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

PAULA T. DOW
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.

Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

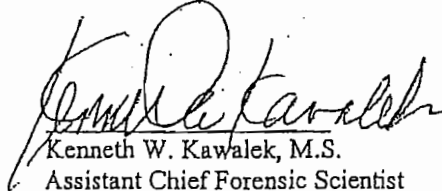
ANALYSIS DATE: 9/23/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10I082


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1190 to 0.1194 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 9, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 28th day of September, 2010.


 Notary

Linda L. Desantis
 Notary Public, New Jersey
 My Commission Expires 8-17-14





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

PAULA T. DOW
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

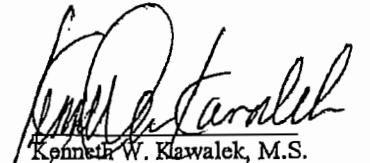
MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 7/25/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G092


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Kenneth W. Klawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.


Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWE 53-0196

Certification Date

Technician

Re-Certification Due Date

2/28/11

DM

2/28/12



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0203

Certification Date

Technician

Re-Certification Due Date

February 7, 2011

ZM

February 7, 2012



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0205

Certification Date

Technician

Re-Certification Due Date

February 7, 2011

JM

February 7, 2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00536 Lin. Date: 12/01/2011 Lin. No.: 00011
Solution File No.: 00537 Soln. Date: 12/01/2011 Soln. No.: 00119
Sequential File No.: 00537 File Date: 12/01/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0157

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 13:01S | | |
| Control 1 EC | 0.101% | 13:01S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 13:01S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:02S | | |
| Control 2 EC | 0.100% | 13:03S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 13:03S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:03S | | |
| Control 3 EC | 0.100% | 13:04S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 13:04S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:05S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWAP2-199₁₀

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: _____

Tpr J Dellanoce # 6027

Badge No.: 6027

Date: 12/01/2011



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

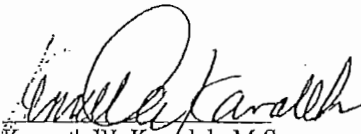
ANALYSIS DATE: 8/26/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10H081


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1185 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 4, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 9 day of September, 2010.


 Notary
 JOHN R. LEAVER
 NOTARY PUBLIC STATE OF NEW JERSEY
 MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable

