

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00704	Calib. Date: 06/30/2014
Certification File No.:	00705	Calib. No.: 00023
Linearity File No.:	00706	Cert. Date: 06/30/2014
Solution File No.:	00729	Cert. No.: 00017
Sequential File No.:	00729	Lin. Date: 06/30/2014
		Lin. No.: 00017
		Soln. Date: 11/21/2014
		Soln. No.: 00165
		File Date: 11/21/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	13I119	Expires: 09/10/2015
		Bottle No.: 0495

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:58S		
Control 1 EC	0.101%	17:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:59S		
Control 2 EC	0.100%	18:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:01S		
Control 3 EC	0.100%	18:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER	First Name: JOSEPH	MI: T
Signature: <u>Joseph T. Baumgardner #312</u>	Badge No.: 312	Date: 11/21/2014
	11/21/2014	

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00704	Calib. Date: 06/30/2014
Certification File No.:	00705	Calib. No.: 00023
Linearity File No.:	00706	Cert. Date: 06/30/2014
Solution File No.:	00727	Cert. No.: 00017
Sequential File No.:	00727	Lin. Date: 06/30/2014
		Lin. No.: 00017
		Soln. Date: 10/25/2014
		Soln. No.: 00164
		File Date: 10/25/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	131119	Expires: 09/10/2015
		Bottle No.: 0480

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:50D		
Control 1 EC	0.099%	14:51D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51D		
Control 2 EC	0.098%	14:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:53D		
Control 3 EC	0.100%	14:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

*Joseph T. Baumgardner #312 10/25/14*

Badge No.: 312

Date: 10/25/2014

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00704 Calib. Date: 06/30/2014 Calib. No.: 00023  
Certification File No.: 00705 Cert. Date: 06/30/2014 Cert. No.: 00017  
Linearity File No.: 00706 Lin. Date: 06/30/2014 Lin. No.: 00017  
Solution File No.: 00721 Soln. Date: 09/18/2014 Soln. No.: 00163  
Sequential File No.: 00721 File Date: 09/18/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154  
Control Solution %: 0.100% Expires: 09/10/2015  
Solution Control Lot: 131119 Bottle No.: 0482

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:39D		
Control 1 EC	0.099%	08:39D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:40D		
Control 2 EC	0.098%	08:41D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:41D		
Control 3 EC	0.099%	08:42D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: \_\_\_\_\_

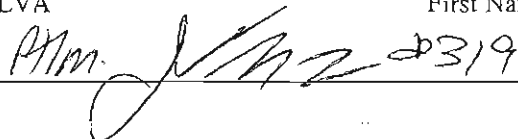

Badge No.: 319

Date: 09/18/2014

# Calibrating Unit

## New Standard Solution Report


<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00704	Calib. Date: 06/30/2014
Certification File No.:	00705	Calib. No.: 00023
Linearity File No.:	00706	Cert. Date: 06/30/2014
Solution File No.:	00719	Cert. No.: 00017
Sequential File No.:	00719	Lin. Date: 06/30/2014
		Lin. No.: 00017
		Soln. Date: 08/23/2014
		Soln. No.: 00162
		File Date: 08/23/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	13I119	Expires: 09/10/2015
		Bottle No.: 0499

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:54D		
Control 1 EC	0.099%	06:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:55D		
Control 2 EC	0.098%	06:56D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:56D		
Control 3 EC	0.098%	06:57D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:58D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

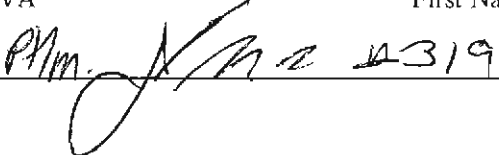Last Name: SILVA	First Name: JAMES	MI: F
Signature: <u></u>	Badge No.: 319	Date: 08/23/2014

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00704 Calib. Date: 06/30/2014 Calib. No.: 00023  
Certification File No.: 00705 Cert. Date: 06/30/2014 Cert. No.: 00017  
Linearity File No.: 00706 Lin. Date: 06/30/2014 Lin. No.: 00017  
Solution File No.: 00715 Soln. Date: 07/29/2014 Soln. No.: 00161  
Sequential File No.: 00715 File Date: 07/29/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154  
Control Solution %: 0.100% Expires: 09/10/2015  
Solution Control Lot: 131119 Bottle No.: 0479

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:32D		
Control 1 EC	0.098%	20:32D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	20:32D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:33D		
Control 2 EC	0.097%	20:34D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:34D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:34D		
Control 3 EC	0.098%	20:35D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: \_\_\_\_\_

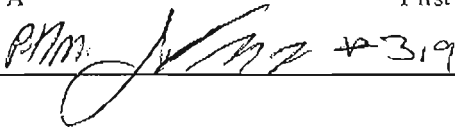

Badge No.: 319

Date: 07/29/2014

# Calibrating Unit

## New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00703	Cert. No.: 00016
Sequential File No.:	00703	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 06/26/2014
		Soln. No.: 00159
		File Date: 06/26/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	13I119	Expires: 09/10/2015
		Bottle No.: 0485

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:55D		
Control 1 EC	0.100%	13:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:56D		
Control 2 EC	0.100%	13:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:57D		
Control 3 EC	0.099%	13:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: \_\_\_\_\_

A/ Sgt. JS/A # 6027

Badge No.: 6027

Date: 06/26/2014

# Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00700	Cert. No.: 00016
Sequential File No.:	00700	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 06/08/2014
		Soln. No.: 00158
		File Date: 06/08/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	131119	Expires: 09/10/2015
		Bottle No.: 0490

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:44D		
Control 1 EC	0.099%	22:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:45D		
Control 2 EC	0.099%	22:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:46D		
Control 3 EC	0.099%	22:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SILVA

First Name: JAMES

M1: F

Signature: \_\_\_\_\_

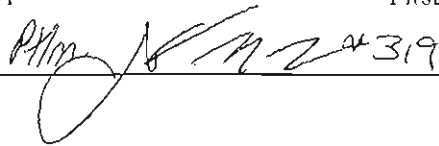

Badge No.: 319

Date: 06/08/2014

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00695	Cert. No.: 00016
Sequential File No.:	00695	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 05/13/2014
		Soln. No.: 00157
		File Date: 05/13/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	131119	Expires: 09/10/2015
		Bottle No.: 0477

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:06D		
Control 1 EC	0.099%	11:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		
Control 2 EC	0.099%	11:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:09D		
Control 3 EC	0.099%	11:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-177


**Changed By:** \_\_\_\_\_ *JS* MJ: S

Last Name: DELLANOCE First Name: JOSEPH

Signature: *TP E JS # 6027* Badge No.: 6027

Date: 05/13/2014





**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXC 53-0154

Certification Date

1-3-14

Technician

BC

Re-Certification Due Date

1-3-15

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWA P2-177

Certification date:

1-3-14

Next Certification due:

1-3-15

Probe Value

105

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

BC

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00692	Cert. No.: 00016
Sequential File No.:	00692	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 05/01/2014
		Soln. No.: 00156
		File Date: 05/01/2014

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %:	0.100%		Expires: 09/10/2015
Solution Control Lot:	131119		Bottle No.: 0478

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:33D		
Control 1 EC	0.099%	23:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:34D		
Control 2 EC	0.098%	23:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:35D		
Control 3 EC	0.098%	23:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

*Joseph T. Baumgardner #312*  
5/1/2014

Badge No.: 312

Date: 05/01/2014

# Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00691	Cert. No.: 00016
Sequential File No.:	00691	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 04/03/2014
		Soln. No.: 00155
		File Date: 04/03/2014

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %:	0.100%		Expires: 09/10/2015
Solution Control Lot:	13F119		Bottle No.: 0476

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:08S		
Control 1 EC	0.097%	07:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:09S		
Control 2 EC	0.097%	07:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	07:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:10S		
Control 3 EC	0.097%	07:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SILVA

First Name: JAMES

MI: F

Signature: \_\_\_\_\_

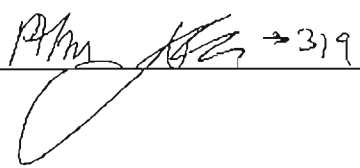

Badge No.: 319

Date: 04/03/2014

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00688	Cert. No.: 00016
Sequential File No.:	00688	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 03/06/2014
		Soln. No.: 00154
		File Date: 03/06/2014

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %: 0.100%		Expires: 09/10/2015
Solution Control Lot: 131119		Bottle No.: 0497

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:27S		
Control 1 EC	0.100%	20:27S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	20:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:28S		
Control 2 EC	0.099%	20:29S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:29S		
Control 3 EC	0.099%	20:30S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:31S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SILVA

First Name: JAMES

MI: F

Signature: \_\_\_\_\_

Badge No.: 319

Date: 03/06/2014

# Calibrating Unit

## New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00681	Calib. Date: 01/10/2014
Certification File No.:	00682	Calib. No.: 00022
Linearity File No.:	00683	Cert. Date: 01/10/2014
Solution File No.:	00685	Cert. No.: 00016
Sequential File No.:	00685	Lin. Date: 01/10/2014
		Lin. No.: 00016
		Soln. Date: 02/06/2014
		Soln. No.: 00153
		File Date: 02/06/2014

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	12D101	Expires: 04/25/2014
		Bottle No.: 0160

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:14S		
Control 1 EC	0.097%	08:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	08:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:15S		
Control 2 EC	0.096%	08:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	08:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:16S		
Control 3 EC	0.096%	08:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SILVA

First Name: JAMES

MJ: F

Signature: \_\_\_\_\_

*[Handwritten Signature]* \*319

Badge No.: 319

Date: 02/06/2014