

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00763	Calib. Date: 11/25/2015
Certification File No.:	00764	Calib. No.: 00026
Linearity File No.:	00765	Cert. Date: 11/25/2015
Solution File No.:	00770	Cert. No.: 00020
Sequential File No.:	00770	Lin. Date: 11/25/2015
		Lin. No.: 00020
		Soln. Date: 12/24/2015
		Soln. No.: 00181
		File Date: 12/24/2015

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	14H132	Expires: 08/22/2016
		Bottle No.: 0992

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:17S		
Control 1 EC	0.100%	17:18S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:19S		
Control 2 EC	0.098%	17:19S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:20S		
Control 3 EC	0.098%	17:21S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: A/Lt. Joseph Baumgardner #312

Badge No.: 312

Date: 12/24/2015

12-24-15

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE		
Calibration File No.:	00750	Calib. Date:	06/11/2015
Certification File No.:	00751	Cert. No.:	00025
Linearity File No.:	00752	Lin. Date:	06/11/2015
Solution File No.:	00762	Cert. No.:	00019
Sequential File No.:	00762	Lin. No.:	00019
		Soln. Date:	11/18/2015
		Soln. No.:	00179
		File Date:	11/18/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0154
Solution Control Lot:	14H132	Expires:	08/22/2016
		Bottle No.:	0991

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:03S		
Control 1 EC	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04S		
Control 2 EC	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		
Control 3 EC	0.099%	10:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER	First Name: JOSEPH	MI: T
Signature: <u><i>Sgt. Joseph T. Baumgardner #312</i></u>	Badge No.: 312	Date: 11/18/2015
		<i>11/18/2015</i>

SOLUTION CONTROL LOT: 14H132

BOTTLE NO.: 0991

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:03S		
Control 1 EC	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04S		
Control 2 EC	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		
Control 3 EC	0.099%	10:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		

All tests within acceptable tolerance.

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00750 Calib. Date: 06/11/2015 Calib. No.: 00025  
Certification File No.: 00751 Cert. Date: 06/11/2015 Cert. No.: 00019  
Linearity File No.: 00752 Lin. Date: 06/11/2015 Lin. No.: 00019  
Solution File No.: 00761 Soln. Date: 10/20/2015 Soln. No.: 00178  
Sequential File No.: 00761 File Date: 10/20/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154  
Control Solution %: 0.100% Expires: 08/22/2016  
Solution Control Lot: 14H132 Bottle No.: 0996

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:46D		
Control 1 EC	0.103%	11:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:48D		
Control 2 EC	0.100%	11:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:49D		
Control 3 EC	0.100%	11:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-177

### Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: SGT. JS # 6027

Badge No.: 6027

Date: 10/20/2015

Signature: SGT. JS # 6027


Badge No.: 6027

Date: 10/20/2015

Signature: SGT. JS # 6027

Badge No.: 6027

Date: 10/20/2015



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXCS3-0154

Certification Date


9-22-15

Technician

JJ

Re-Certification Due Date

9-22-16

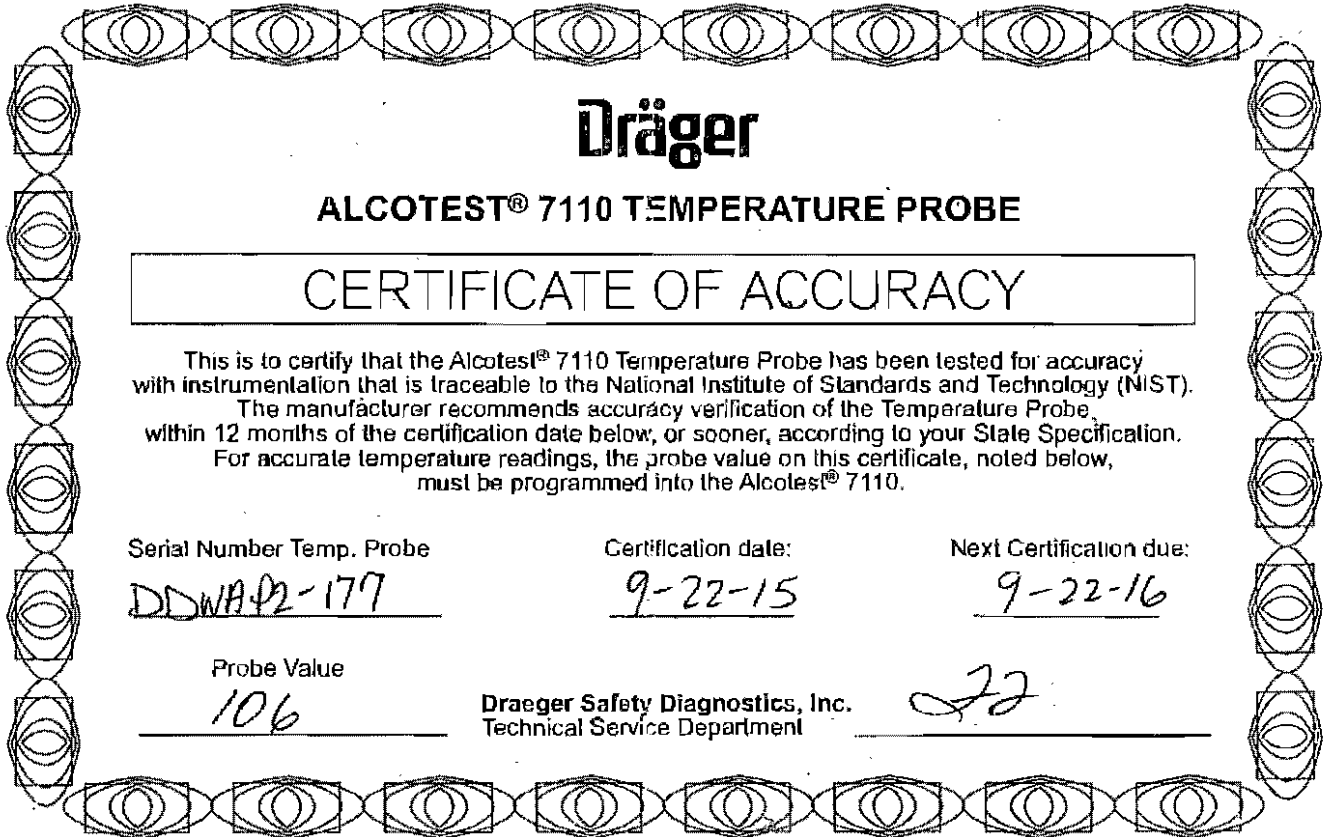

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe, within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWA#2-177

Certification date:

9-22-15

Next Certification due:

9-22-16

Probe Value

106

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

JJ

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE	Calib. Date:	06/11/2015
Calibration File No.:	00750	Calib. No.:	00025
Certification File No.:	00751	Cert. Date:	06/11/2015
Linearity File No.:	00752	Lin. Date:	06/11/2015
Solution File No.:	00760	Soln. Date:	09/30/2015
Sequential File No.:	00760	File Date:	09/30/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0135
Solution Control Lot:	14H132	Expires:	08/22/2016
		Bottle No.:	0998

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:04D		
Control 1 EC	0.100%	11:04D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05D		
Control 2 EC	0.099%	11:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		
Control 3 EC	0.099%	11:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SILVA	First Name: JAMES	M: F
Signature: <u>Sgt. J Silva #319</u>	Badge No.: 319	Date: 09/30/2015

SOLUTION CONTROL LOT: 14H132

BOTTLE NO.: 0998

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:04D		
Control 1 EC	0.100%	11:04D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05D		
Control 2 EC	0.099%	11:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		
Control 3 EC	0.099%	11:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		

All tests within acceptable tolerance.

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00750	Calib. Date: 06/11/2015
Certification File No.:	00751	Calib. No.: 00025
Linearity File No.:	00752	Cert. Date: 06/11/2015
Solution File No.:	00758	Cert. No.: 00019
Sequential File No.:	00758	Lin. Date: 06/11/2015
		Lin. No.: 00019
		Soln. Date: 09/02/2015
		Soln. No.: 00176
		File Date: 09/02/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	14H132	Expires: 08/22/2016
		Bottle No.: 0993

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:11D		
Control 1 EC	0.099%	01:12D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:13D		
Control 2 EC	0.098%	01:13D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:14D		
Control 3 EC	0.098%	01:15D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SILVA

First Name: JAMES

MI: F

Signature: \_\_\_\_\_

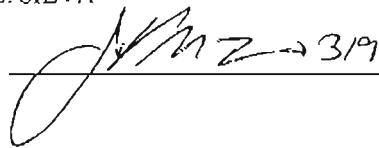

Badge No.: 319

Date: 09/02/2015

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:11D		
Control 1 EC	0.099%	01:12D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:13D		
Control 2 EC	0.098%	01:13D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:14D		
Control 3 EC	0.098%	01:15D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with

# Calibrating Unit New Standard Solution Report


<b>Equipment</b>	Alcotest 7110 MKJII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00750	Calib. Date: 06/11/2015
Certification File No.:	00751	Calib. No.: 00025
Linearity File No.:	00752	Cert. Date: 06/11/2015
Solution File No.:	00756	Cert. No.: 00019
Sequential File No.:	00756	Lin. Date: 06/11/2015
		Lin. No.: 00019
		Soln. Date: 08/05/2015
		Soln. No.: 00175
		File Date: 08/05/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	14H132	Expires: 08/22/2016
		Bottle No.: 0994

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:53D		
Control 1 EC	0.099%	16:54D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:54D		
Control 2 EC	0.098%	16:55D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:56D		
Control 3 EC	0.098%	16:56D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

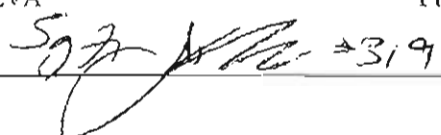Last Name: SILVA	First Name: JAMES	MI: F
Signature: 	Badge No.: 319	Date: 08/05/2015

UNIVERSITY MICROFILMS INTL 341132E

00000 14011 0004

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:53D		
Control 1 EC	0.099%	16:54D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:54D		
Control 2 EC	0.098%	16:55D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:56D		
Control 3 EC	0.098%	16:56D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:57D		

All tests within acceptable tolerance.

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 M&JII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00750	Calib. Date: 06/11/2015
Certification File No.:	00751	Calib. No.: 00025
Linearity File No.:	00752	Cert. Date: 06/11/2015
Solution File No.:	00755	Cert. No.: 00019
Sequential File No.:	00755	Lin. Date: 06/11/2015
		Lin. No.: 00019
		Soln. Date: 07/09/2015
		Soln. No.: 00174
		File Date: 07/09/2015

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %: 0.100%		Expires: 08/22/2016
Solution Control Lot: 14H132		Bottle No.: 0995

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:32D		
Control 1 EC	0.099%	12:33D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		
Control 2 EC	0.098%	12:34D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:34D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35D		
Control 3 EC	0.098%	12:36D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:36D		

A) tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SILVA

First Name: JAMES

MJ: F

Signature: \_\_\_\_\_

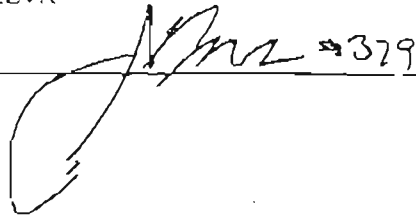

Badge No.: 319

Date: 07/09/2015

Solution Control Lot: 14H132

Bottle No.: 0995

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:32D		
Control 1 EC	0.099%	12:33D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		
Control 2 EC	0.098%	12:34D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:34D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35D		
Control 3 EC	0.098%	12:36D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:36D		

All tests within acceptable tolerance.



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00732	Calib. Date: 12/17/2014
Certification File No.:	00733	Calib. No.: 00024
Linearity File No.:	00734	Cert. Date: 12/17/2014
Solution File No.:	00749	Cert. No.: 00018
Sequential File No.:	00749	Lin. Date: 12/17/2014
		Lin. No.: 00018
		Soln. Date: 06/02/2015
		Soln. No.: 00172
		File Date: 06/02/2015

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %:	0.100%		Expires: 08/22/2016
Solution Control Lot:	14H132		Bottle No.: 0986

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:12D		
Control 1 EC	0.097%	01:13D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	01:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:14D		
Control 2 EC	0.096%	01:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	01:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15D		
Control 3 EC	0.096%	01:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	01:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SILVA

First Name: JAMES

MI: F

Signature: \_\_\_\_\_

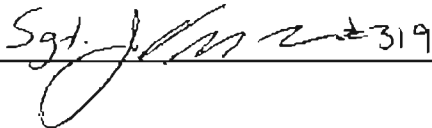

Badge No.: 319

Date: 06/02/2015

Solution Control Lot: 14H132

Bottle No.: 0986

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:12D		
Control 1 EC	0.097%	01:13D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	01:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:14D		
Control 2 EC	0.096%	01:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	01:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15D		
Control 3 EC	0.096%	01:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	01:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:16D		

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00732 Calib. Date: 12/17/2014 Calib. No.: 00024  
Certification File No.: 00733 Cert. Date: 12/17/2014 Cert. No.: 00018  
Linearity File No.: 00734 Lin. Date: 12/17/2014 Lin. No.: 00018  
Solution File No.: 00745 Soln. Date: 05/05/2015 Soln. No.: 00171  
Sequential File No.: 00745 File Date: 05/05/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135  
Control Solution %: 0.100% Expires: 08/22/2016  
Solution Control Lot: 14H132 Bottle No.: 0987

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:37D		
Control 1 EC	0.097%	09:38D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	09:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38D		
Control 2 EC	0.096%	09:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40D		
Control 3 EC	0.096%	09:40D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	09:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: SILVA

First Name: JAMES

M1: F

Signature: \_\_\_\_\_

*Sgt James 319*

Badge No.: 319

Date: 05/05/2015

# Calibrating Unit

## New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE		
Calibration File No.:	00732	Calib. Date:	12/17/2014
Certification File No.:	00733	Cert. Date:	12/17/2014
Linearity File No.:	00734	Lin. Date:	12/17/2014
Solution File No.:	00743	Soln. Date:	04/07/2015
Sequential File No.:	00743	File Date:	04/07/2015

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXC S3-0135
Control Solution %:	0.100%			Expires:	08/22/2016
Solution Control Lot:	14H132			Bottle No.:	0989

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:54D		
Control 1 EC	0.097%	08:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56D		
Control 2 EC	0.097%	08:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	08:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57D		
Control 3 EC	0.097%	08:58D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: NIKA

First Name: JASON

MI: N

Signature: \_\_\_\_\_



Badge No.: 326

Date: 04/07/2015

Solution Control Lot: 14H132

Bottle No.: 0989

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:54D		
Control 1 EC	0.097%	08:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56D		
Control 2 EC	0.097%	08:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	08:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57D		
Control 3 EC	0.097%	08:58D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59D		

All tests within acceptable tolerance.

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00732	Calib. Date: 12/17/2014
Certification File No.:	00733	Calib. No.: 00024
Linearity File No.:	00734	Cert. Date: 12/17/2014
Solution File No.:	00741	Cert. No.: 00018
Sequential File No.:	00741	Lin. Date: 12/17/2014
		Lin. No.: 00018
		Soln. Date: 03/10/2015
		Soln. No.: 00169
		File Date: 03/10/2015

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %: 0.100%		Expires: 08/22/2016
Solution Control Lot: 1411132		Bottle No.: 0990

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:40S		
Control 1 EC	0.100%	21:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:42S		
Control 2 EC	0.099%	21:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	21:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:43S		
Control 3 EC	0.099%	21:44S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: Sgt. Joseph Baumgardner #312

Badge No.: 312

Date: 03/10/2015

3/10/2015

# Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00732	Calib. Date: 12/17/2014
Certification File No.:	00733	Calib. No.: 00024
Linearity File No.:	00734	Cert. Date: 12/17/2014
Solution File No.:	00739	Cert. No.: 00018
Sequential File No.:	00739	Lin. Date: 12/17/2014
		Lin. No.: 00018
		Soln. Date: 02/10/2015
		Soln. No.: 00168
		File Date: 02/10/2015


Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %: 0.100%		Expires: 09/10/2015
Solution Control Lot: 131119		Bottle No.: 0500

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:02S		
Control 1 EC	0.099%	15:03S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03S		
Control 2 EC	0.099%	15:04S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:05S		
Control 3 EC	0.099%	15:05S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

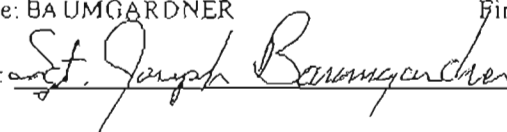Last Name: BAUMGARDNER	First Name: JOSEPH	M/I: T
Signature: 	#312	Badge No.: 312
	2/10/2015	Date: 02/10/2015

Solution Control Lot: 131119	Bottle No.: 0500
------------------------------	------------------

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:02S		
Control 1 EC	0.099%	15:03S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03S		
Control 2 EC	0.099%	15:04S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:05S		
Control 3 EC	0.099%	15:05S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:06S		

# Calibrating Unit

## New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE		
Calibration File No.:	00732	Calib. Date:	12/17/2014
Certification File No.:	00733	Cert. No.:	00024
Linearity File No.:	00734	Lin. Date:	12/17/2014
Solution File No.:	00738	Lin. No.:	00018
Sequential File No.:	00738	Soln. Date:	01/13/2015
		Soln. No.:	00167
		File Date:	01/13/2015

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXC S3-0135
Control Solution %:	0.100%			Expires:	09/10/2015
Solution Control Lot:	131119			Bottle No.:	0491

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:10S		
Control 1 EC	0.100%	22:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	22:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:12S		
Control 2 EC	0.099%	22:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	22:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:13S		
Control 3 EC	0.098%	22:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

*Joseph T. Baumgardner* # 312  
1/13/2015

Badge No.: 312

Date: 01/13/2015