

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00804	Calib. Date: 01/30/2017
Certification File No.:	00805	Calib. No.: 00029
Linearity File No.:	00806	Cert. Date: 01/30/2017
Solution File No.:	00811	Cert. No.: 00023
Sequential File No.:	00811	Lin. Date: 01/30/2017
		Lin. No.: 00023
		Soln. Date: 03/12/2017
		Soln. No.: 00198
		File Date: 03/12/2017

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0154
Control Solution %:	0.100%		Expires: 06/07/2018
Solution Control Lot:	16140		Bottle No.: 1074

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:08S		
Control 1 EC	0.097%	22:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	22:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:10S		
Control 2 EC	0.096%	22:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	22:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:11S		
Control 3 EC	0.096%	22:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	22:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

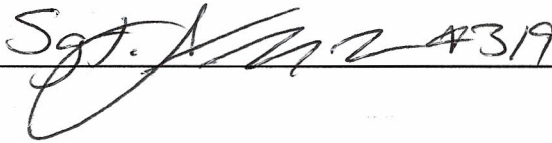

Badge No.: 319

Date: 03/12/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00804 Calib. Date: 01/30/2017 Calib. No.: 00029
Certification File No.: 00805 Cert. Date: 01/30/2017 Cert. No.: 00023
Linearity File No.: 00806 Lin. Date: 01/30/2017 Lin. No.: 00023
Solution File No.: 00809 Soln. Date: 02/14/2017 Soln. No.: 00197
Sequential File No.: 00809 File Date: 02/14/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 06/07/2018
Solution Control Lot: 16140 Bottle No.: 0960

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:51S		
Control 1 EC	0.097%	23:52S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	23:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:52S		
Control 2 EC	0.096%	23:53S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	23:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:54S		
Control 3 EC	0.096%	23:54S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	23:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:55S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINGOTTA

First Name: DAVID

MI: P

Signature:  321

Badge No.: 321

Date: 02/14/2017