

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00852 Calib. Date: 09/12/2018 Calib. No.: 00033
Certification File No.: 00853 Cert. Date: 09/12/2018 Cert. No.: 00027
Linearity File No.: 00854 Lin. Date: 09/12/2018 Lin. No.: 00027
Solution File No.: 00858 Soln. Date: 12/19/2018 Soln. No.: 00222
Sequential File No.: 00858 File Date: 12/19/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/31/2020
Solution Control Lot: 18050 Bottle No.: 0388

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:08S		
Control 1 EC	0.101%	01:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:09S		
Control 2 EC	0.099%	01:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:11S		
Control 3 EC	0.099%	01:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature:  321

Badge No.: 321

Date: 12/19/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00852	Calib. Date: 09/12/2018
Certification File No.:	00853	Cert. No.: 00033
Linearity File No.:	00854	Cert. Date: 09/12/2018
Solution File No.:	00857	Cert. No.: 00027
Sequential File No.:	00857	Lin. Date: 09/12/2018
		Lin. No.: 00027
		Soln. Date: 11/13/2018
		Soln. No.: 00221
		File Date: 11/13/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0157

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:25S		
Control 1 EC	0.100%	11:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:26S		
Control 2 EC	0.099%	11:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:28S		
Control 3 EC	0.099%	11:28S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:29S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature:  321

Badge No.: 321

Date: 11/13/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00852	Calib. Date: 09/12/2018
Certification File No.:	00853	Cert. No.: 00033
Linearity File No.:	00854	Cert. Date: 09/12/2018
Solution File No.:	00856	Lin. No.: 00027
Sequential File No.:	00856	Lin. Date: 09/12/2018
		Soln. No.: 00220
		Soln. Date: 10/13/2018
		File Date: 10/13/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0161

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:24D		
Control 1 EC	0.098%	02:25D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:25D		
Control 2 EC	0.097%	02:26D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:27D		
Control 3 EC	0.097%	02:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:28D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature:  321

Badge No.: 321

Date: 10/13/2018

Calibrating Unit

New Standard Solution Report

COPY

Equipment Alcotest 7110 MKIII-C
Location: LONGPORT POLICE
Calibration File No.: 00852
Certification File No.: 00853
Linearity File No.: 00854
Solution File No.: 00855
Sequential File No.: 00855

Serial No.: ARXA-0067

Calib. Date: 09/12/2018 **Calib. No.:** 00033
Cert. Date: 09/12/2018 **Cert. No.:** 00027
Lin. Date: 09/12/2018 **Lin. No.:** 00027
Soln. Date: 09/12/2018 **Soln. No.:** 00219
File Date: 09/12/2018

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 18050

Model No.: CU-34

Serial No.: DDXC S3-0135
Expires: 01/31/2020
Bottle No.: 0092

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:58D		
Control 1 EC	0.101%	14:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:59D		
Control 2 EC	0.100%	15:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		
Control 3 EC	0.099%	15:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: _____

DQWAP2-199 (KA)

Changed By:

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: _____

Sgt. K. W. #6704

Badge No.: 6704

Date: 09/12/2018

original with
Calibration Record

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00837 Calib. Date: 03/28/2018 Calib. No.: 00032
Certification File No.: 00838 Cert. Date: 03/28/2018 Cert. No.: 00026
Linearity File No.: 00839 Lin. Date: 03/28/2018 Lin. No.: 00026
Solution File No.: 00850 Soln. Date: 08/17/2018 Soln. No.: 00218
Sequential File No.: 00850 File Date: 08/17/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/31/2020
Solution Control Lot: 18050 Bottle No.: 0321

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:58D		
Control 1 EC	0.098%	12:59D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	12:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:59D		
Control 2 EC	0.097%	13:00D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	13:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:01D		
Control 3 EC	0.096%	13:01D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	13:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature: David Cincotta 321

Badge No.: 321

Date: 08/17/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00837	Calib. Date: 03/28/2018
Certification File No.:	00838	Calib. No.: 00032
Linearity File No.:	00839	Cert. Date: 03/28/2018
Solution File No.:	00849	Cert. No.: 00026
Sequential File No.:	00849	Lin. Date: 03/28/2018
		Lin. No.: 00026
		Soln. Date: 08/17/2018
		Soln. No.: 00217
		File Date: 08/17/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0104

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:13D		
Control 1 EC	0.095%	11:13D	33.9°C	CONTROL TEST FAILED
Control 1 IR	0.094%	11:13D	33.9°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	11:14D		
Control 2 EC	0.095%	11:15D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	11:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		
Control 3 EC	0.095%	11:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.095%	11:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature: _____

David Cincotta 321

Badge No.: 321

Date: 08/17/2018

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00837 Calib. Date: 03/28/2018 Calib. No.: 00032
Certification File No.: 00838 Cert. Date: 03/28/2018 Cert. No.: 00026
Linearity File No.: 00839 Lin. Date: 03/28/2018 Lin. No.: 00026
Solution File No.: 00848 Soln. Date: 07/17/2018 Soln. No.: 00216
Sequential File No.: 00848 File Date: 07/17/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/31/2020
Solution Control Lot: 18050 Bottle No.: 0108

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:36D		
Control 1 EC	0.097%	22:37D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	22:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:38D		
Control 2 EC	0.096%	22:38D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	22:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:39D		
Control 3 EC	0.096%	22:40D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.095%	22:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

SGT. James Silva


Badge No.: 319

Date: 07/17/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00837	Calib. Date: 03/28/2018
Certification File No.:	00838	Calib. No.: 00032
Linearity File No.:	00839	Cert. Date: 03/28/2018
Solution File No.:	00846	Cert. No.: 00026
Sequential File No.:	00846	Lin. Date: 03/28/2018
		Lin. No.: 00026
		Soln. Date: 07/07/2018
		Soln. No.: 00215
		File Date: 07/07/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0330

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:37D		
Control 1 EC	0.096%	20:37D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.095%	20:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38D		
Control 2 EC	0.095%	20:39D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	20:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:39D		
Control 3 EC	0.095%	20:40D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	20:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature: _____

David Cincotta 321

Badge No.: 321

Date: 07/07/2018

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00837 Calib. Date: 03/28/2018 Calib. No.: 00032
Certification File No.: 00838 Cert. Date: 03/28/2018 Cert. No.: 00026
Linearity File No.: 00839 Lin. Date: 03/28/2018 Lin. No.: 00026
Solution File No.: 00845 Soln. Date: 06/14/2018 Soln. No.: 00214
Sequential File No.: 00845 File Date: 06/14/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/31/2020
Solution Control Lot: 18050 Bottle No.: 0275

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:51D		
Control 1 EC	0.096%	06:52D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	06:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:53D		
Control 2 EC	0.095%	06:53D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	06:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:54D		
Control 3 EC	0.095%	06:55D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	06:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

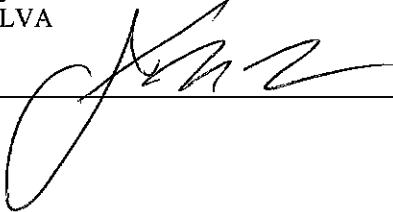

Badge No.: 319

Date: 06/14/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00837	Calib. Date: 03/28/2018
Certification File No.:	00838	Cert. No.: 00032
Linearity File No.:	00839	Cert. Date: 03/28/2018
Solution File No.:	00842	Lin. Date: 03/28/2018
Sequential File No.:	00842	Lin. No.: 00026
		Soln. Date: 05/24/2018
		Soln. No.: 00213
		File Date: 05/24/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0271

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:04D		
Control 1 EC	0.096%	14:05D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	14:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05D		
Control 2 EC	0.095%	14:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	14:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07D		
Control 3 EC	0.095%	14:08D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	14:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature:  # 321

Badge No.: 321

Date: 05/24/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00837	Calib. Date: 03/28/2018
Certification File No.:	00838	Calib. No.: 00032
Linearity File No.:	00839	Cert. Date: 03/28/2018
Solution File No.:	00841	Cert. No.: 00026
Sequential File No.:	00841	Lin. Date: 03/28/2018
		Lin. No.: 00026
		Soln. Date: 04/26/2018
		Soln. No.: 00212
		File Date: 04/26/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0389

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:11D		
Control 1 EC	0.097%	04:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	04:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:13D		
Control 2 EC	0.096%	04:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	04:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:14D		
Control 3 EC	0.096%	04:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	04:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature: _____

David Cincotta 321

Badge No.: 321

Date: 04/26/2018

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00827	Calib. Date: 10/20/2017
Certification File No.:	00828	Calib. No.: 00031
Linearity File No.:	00829	Cert. Date: 10/20/2017
Solution File No.:	00836	Cert. No.: 00025
Sequential File No.:	00836	Lin. Date: 10/20/2017
		Lin. No.: 00025
		Soln. Date: 03/14/2018
		Soln. No.: 00210
		File Date: 03/14/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 0105

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:27S		
Control 1 EC	0.097%	09:28S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28S		
Control 2 EC	0.098%	09:29S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		
Control 3 EC	0.098%	09:30S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature:  321

Badge No.: 321

Date: 03/14/2018

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00827 Calib. Date: 10/20/2017 Calib. No.: 00031
Certification File No.: 00828 Cert. Date: 10/20/2017 Cert. No.: 00025
Linearity File No.: 00829 Lin. Date: 10/20/2017 Lin. No.: 00025
Solution File No.: 00835 Soln. Date: 02/10/2018 Soln. No.: 00209
Sequential File No.: 00835 File Date: 02/10/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 1247

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:04S		
Control 1 EC	0.097%	09:04S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	09:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05S		
Control 2 EC	0.096%	09:06S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	09:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:07S		
Control 3 EC	0.095%	09:07S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	09:07S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:08S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature:  321

Badge No.: 321

Date: 02/10/2018

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00827 Calib. Date: 10/20/2017 Calib. No.: 00031
Certification File No.: 00828 Cert. Date: 10/20/2017 Cert. No.: 00025
Linearity File No.: 00829 Lin. Date: 10/20/2017 Lin. No.: 00025
Solution File No.: 00833 Soln. Date: 01/19/2018 Soln. No.: 00208
Sequential File No.: 00833 File Date: 01/19/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 1384

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:48S		
Control 1 EC	0.102%	02:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:50S		
Control 2 EC	0.100%	02:50S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:51S		
Control 3 EC	0.099%	02:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CINCOTTA

First Name: DAVID

MI: P

Signature: David Cincotta 321

Badge No.: 321

Date: 01/19/2018