

Calibrating Unit New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00598 | Calib. Date: 10/17/2012 |
| Certification File No.: | 00599 | Calib. No.: 00018 |
| Linearity File No.: | 00600 | Cert. Date: 10/17/2012 |
| Solution File No.: | 00610 | Cert. No.: 00013 |
| Sequential File No.: | 00610 | Lin. Date: 10/17/2012 |
| | | Lin. No.: 00013 |
| | | Soln. Date: 12/13/2012 |
| | | Soln. No.: 00133 |
| | | File Date: 12/13/2012 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXC S3-0154 |
| Solution Control Lot: | 12D101 | Expires: 04/25/2014 |
| | | Bottle No.: 0173 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 22:16S | | |
| Control 1 EC | 0.101% | 22:17S | 34.1°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 22:17S | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:17S | | |
| Control 2 EC | 0.099% | 22:18S | 34.1°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 22:18S | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:19S | | |
| Control 3 EC | 0.099% | 22:19S | 34.1°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 22:19S | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:20S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 12/13/12

Badge No.: 312

Date: 12/13/2012

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00598 | Calib. Date: 10/17/2012 |
| Certification File No.: | 00599 | Calib. No.: 00018 |
| Linearity File No.: | 00600 | Cert. Date: 10/17/2012 |
| Solution File No.: | 00605 | Cert. No.: 00013 |
| Sequential File No.: | 00605 | Lin. Date: 10/17/2012 |
| | | Lin. No.: 00013 |
| | | Soln. Date: 11/15/2012 |
| | | Soln. No.: 00132 |
| | | File Date: 11/15/2012 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXC S3-0154 |
| Solution Control Lot: | 12D101 | Expires: 04/25/2014 |
| | | Bottle No.: 0163 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 09:07S | | |
| Control 1 EC | 0.099% | 09:07S | 34.1°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 09:07S | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:08S | | |
| Control 2 EC | 0.098% | 09:09S | 34.1°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 09:09S | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:09S | | |
| Control 3 EC | 0.099% | 09:10S | 34.1°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 09:10S | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:10S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

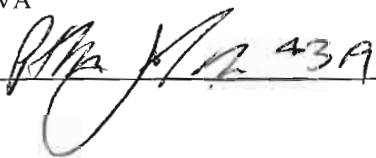

Badge No.: 319

Date: 11/15/2012

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00554 | Calib. Date: 05/16/2012 |
| Certification File No.: | 00555 | Calib. No.: 00017 |
| Linearity File No.: | 00556 | Cert. Date: 05/16/2012 |
| Solution File No.: | 00596 | Cert. No.: 00012 |
| Sequential File No.: | 00596 | Lin. Date: 05/16/2012 |
| | | Lin. No.: 00012 |
| | | Soln. Date: 09/28/2012 |
| | | Soln. No.: 00130 |
| | | File Date: 09/28/2012 |

| | | | |
|-----------------------|--------|------------------|--------------------------|
| Calibrating Unit: | WET | Model No.: CU-34 | Serial No.: DDXC S3-0135 |
| Control Solution %: | 0.100% | | Expires: 04/25/2014 |
| Solution Control Lot: | 12D101 | | Bottle No.: 0169 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 20:49D | | |
| Control 1 EC | 0.100% | 20:50D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 20:50D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:50D | | |
| Control 2 EC | 0.100% | 20:51D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 20:51D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:51D | | |
| Control 3 EC | 0.099% | 20:52D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 20:52D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:53D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

Badge No.: 319

Date: 09/28/2012

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00554 | Calib. Date: 05/16/2012 |
| Certification File No.: | 00555 | Calib. No.: 00017 |
| Linearity File No.: | 00556 | Cert. Date: 05/16/2012 |
| Solution File No.: | 00585 | Cert. No.: 00012 |
| Sequential File No.: | 00585 | Lin. Date: 05/16/2012 |
| | | Lin. No.: 00012 |
| | | Soln. Date: 09/01/2012 |
| | | Soln. No.: 00129 |
| | | File Date: 09/01/2012 |

| | | |
|------------------------------|------------------|--------------------------|
| Calibrating Unit: WET | Model No.: CU-34 | Serial No.: DDXC S3-0135 |
| Control Solution %: 0.100% | | Expires: 04/25/2014 |
| Solution Control Lot: 12D101 | | Bottle No.: 0168 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 08:10D | | |
| Control 1 EC | 0.100% | 08:10D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 08:10D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 08:11D | | |
| Control 2 EC | 0.100% | 08:12D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 08:12D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 08:12D | | |
| Control 3 EC | 0.100% | 08:13D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 08:13D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 08:14D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

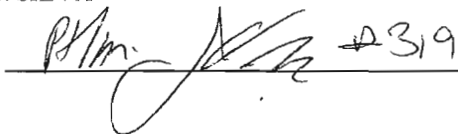

Badge No.: 319

Date: 09/01/2012

Calibrating Unit New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00554 | Calib. Date: 05/16/2012 |
| Certification File No.: | 00555 | Calib. No.: 00017 |
| Linearity File No.: | 00556 | Cert. Date: 05/16/2012 |
| Solution File No.: | 00581 | Cert. No.: 00012 |
| Sequential File No.: | 00581 | Lin. Date: 05/16/2012 |
| | | Lin. No.: 00012 |
| | | Soln. Date: 08/03/2012 |
| | | Soln. No.: 00128 |
| | | File Date: 08/03/2012 |

| | | | |
|-----------------------|--------|------------------|--------------------------|
| Calibrating Unit: | WET | Model No.: CU-34 | Serial No.: DDXC S3-0135 |
| Control Solution %: | 0.100% | | Expires: 04/25/2014 |
| Solution Control Lot: | 12D101 | | Bottle No.: 0158 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 21:09D | | |
| Control 1 EC | 0.100% | 21:10D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 21:10D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:10D | | |
| Control 2 EC | 0.099% | 21:11D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 21:11D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:12D | | |
| Control 3 EC | 0.099% | 21:12D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 21:12D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:13D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 08/03/2012

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00554 | Calib. Date: 05/16/2012 |
| Certification File No.: | 00555 | Calib. No.: 00017 |
| Linearity File No.: | 00556 | Cert. Date: 05/16/2012 |
| Solution File No.: | 00568 | Cert. No.: 00012 |
| Sequential File No.: | 00568 | Lin. Date: 05/16/2012 |
| | | Lin. No.: 00012 |
| | | Soln. Date: 07/12/2012 |
| | | Soln. No.: 00127 |
| | | File Date: 07/12/2012 |

| | | | |
|-----------------------|--------|------------------|--------------------------|
| Calibrating Unit: | WET | Model No.: CU-34 | Serial No.: DDXC S3-0135 |
| Control Solution %: | 0.100% | | Expires: 11/23/2013 |
| Solution Control Lot: | 11K096 | | Bottle No.: 0724 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 11:30D | | |
| Control 1 EC | 0.100% | 11:30D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 11:30D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:31D | | |
| Control 2 EC | 0.099% | 11:31D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 11:31D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:32D | | |
| Control 3 EC | 0.100% | 11:33D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 11:33D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:33D | | |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

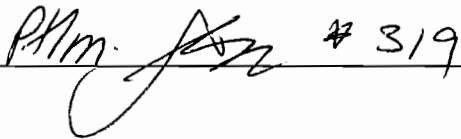Signature:  # 319

Badge No.: 319

Date: 07/12/2012



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

PAULA T. DOW
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 12/16/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11K096

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1217 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 23, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Handwritten signature of Kenneth W. Kawalek

Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 3rd day of January, 2012.

Handwritten signature of Linda L. Desantis

Notary



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|-------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00554 | Calib. Date: 05/16/2012 |
| Certification File No.: | 00555 | Calib. No.: 00017 |
| Linearity File No.: | 00556 | Cert. Date: 05/16/2012 |
| Solution File No.: | 00562 | Cert. No.: 00012 |
| Sequential File No.: | 00562 | Lin. Date: 05/16/2012 |
| | | Lin. No.: 00012 |
| | | Soln. Date: 06/14/2012 |
| | | Soln. No.: 00126 |
| | | File Date: 06/14/2012 |

| | | |
|------------------------------|------------------|--------------------------|
| Calibrating Unit: WET | Model No.: CU-34 | Serial No.: DDXC S3-0135 |
| Control Solution %: 0.100% | | Expires: 08/04/2012 |
| Solution Control Lot: 10H081 | | Bottle No.: 0173 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 20:29D | | |
| Control 1 EC | 0.099% | 20:29D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 20:29D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:30D | | |
| Control 2 EC | 0.098% | 20:30D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 20:30D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:31D | | |
| Control 3 EC | 0.099% | 20:32D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 20:32D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:32D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 06/14/2012

Calibrating Unit New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00534 | Calib. Date: 12/01/2011 |
| Certification File No.: | 00535 | Calib. No.: 00016 |
| Linearity File No.: | 00536 | Cert. Date: 12/01/2011 |
| Solution File No.: | 00552 | Cert. No.: 00011 |
| Sequential File No.: | 00552 | Lin. Date: 12/01/2011 |
| | | Lin. No.: 00011 |
| | | Soln. Date: 04/19/2012 |
| | | Soln. No.: 00124 |
| | | File Date: 04/19/2012 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXC S3-0135 |
| Solution Control Lot: | 10H081 | Expires: 08/04/2012 |
| | | Bottle No.: 0156 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 20:02D | | |
| Control 1 EC | 0.098% | 20:02D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 20:02D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:03D | | |
| Control 2 EC | 0.097% | 20:04D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 20:04D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:04D | | |
| Control 3 EC | 0.097% | 20:05D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 20:05D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:06D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

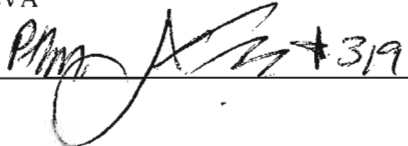

Badge No.: 319

Date: 04/19/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00536 Lin. Date: 12/01/2011 Lin. No.: 00011
Solution File No.: 00550 Soln. Date: 03/22/2012 Soln. No.: 00123
Sequential File No.: 00550 File Date: 03/22/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0151

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 07:18S | | |
| Control 1 EC | 0.098% | 07:19S | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 07:19S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:19S | | |
| Control 2 EC | 0.098% | 07:20S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 07:20S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:21S | | |
| Control 3 EC | 0.098% | 07:21S | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 07:21S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:22S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 03/22/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00536 Lin. Date: 12/01/2011 Lin. No.: 00011
Solution File No.: 00544 Soln. Date: 02/23/2012 Soln. No.: 00122
Sequential File No.: 00544 File Date: 02/23/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0174

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 20:13S | | |
| Control 1 EC | 0.099% | 20:14S | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.098% | 20:14S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:15S | | |
| Control 2 EC | 0.097% | 20:15S | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.098% | 20:15S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:16S | | |
| Control 3 EC | 0.098% | 20:17S | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 20:17S | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 20:17S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature:  # 319

Badge No.: 319

Date: 02/23/2012

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00536 Lin. Date: 12/01/2011 Lin. No.: 00011
Solution File No.: 00541 Soln. Date: 01/26/2012 Soln. No.: 00121
Sequential File No.: 00541 File Date: 01/26/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0166

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 10:27S | | |
| Control 1 EC | 0.101% | 10:28S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 10:28S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:29S | | |
| Control 2 EC | 0.098% | 10:29S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.098% | 10:29S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:30S | | |
| Control 3 EC | 0.099% | 10:31S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 10:31S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:31S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 1/26/12

Badge No.: 312

Date: 01/26/2012