

ALCOTEST CHECKLIST

Municipality: MERCHANTVILLE Alcotest Ser. #: ARUM-0073

County: BURLINGTON Date of Calibration: 09-10-2012

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDWA S3-0011
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDUJ P2-168
- 4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 122172175
- 5.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDLH P1-0073
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

| | | | | |
|--|-----------------|-----------|----------|------------|
| <input checked="" type="checkbox"/> A. | 0.04% Solution. | <u>11</u> | <u>F</u> | <u>090</u> |
| <input checked="" type="checkbox"/> B. | 0.08% Solution. | <u>11</u> | <u>F</u> | <u>091</u> |
| <input checked="" type="checkbox"/> C. | 0.10% Solution. | <u>12</u> | <u>B</u> | <u>099</u> |
| <input checked="" type="checkbox"/> D. | 0.16% Solution. | <u>11</u> | <u>G</u> | <u>092</u> |
- 7. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - A. 0.04% used in Calibration/Linearity Testing. DDCB-0001
 - B. 0.08% used in Calibration/Linearity Testing DDCB-0002
 - C. 0.10% used in Calibration/Linearity Testing DDWA S3-0011 [Same as instrument's CU34 unit].
 - D. 0.16% used in Calibration/Linearity Testing. DDBN-0007
- 8.
 - A. New Standard Solution Report following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 11 K 096
 - D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

3-9-12

SERIAL NUMBER:

ARUM-0073

Draeger Safety Diagnostics, Inc.

AS



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWA 53-0011

Certification Date

Technician

Re-Certification Due Date

2/7/12

ZM

2/7/13

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUJP2-168

2/7/12

2/7/13

Probe Value

102

Dräger Safety Diagnostics, Inc.
Technical Service Department

ZM



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCCL Z540-1, and 9001



Cert. No.: 4000-4269984

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087
Instrument Identification:

Model: 61220-601 S/N: 122172175 Manufacturer: Control Company

Standards/Equipment:

| Description | Serial Number | Due Date | NIST Traceable Reference |
|-------------------------------------|---------------|----------|--------------------------|
| Temperature Calibration Bath TC-275 | A9A237 | | |
| Digital Thermometer | B18815 | 6/06/12 | B1606038 |
| PRT Temperature Probe | 01841 | 5/28/12 | B1526085 |
| Temperature Calibration Bath TC-258 | B01375 | | |
| Thermistor Module | A27129 | 10/31/12 | 1000306945 |
| Temperature Probe | 157 | 11/13/12 | 6-BL72N-1-1 |
| Temperature Calibration Bath TC-179 | A45240 | | |
| Thermistor Module | A17118 | 2/01/13 | 1000311439 |
| Temperature Probe | 128 | 2/14/13 | 6-BN9WZ-27-1 |

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 3/30/12 Cal Due: 3/30/14
Test Conditions: 23.0°C 44.0 %RH 1012 mBar

Calibration Data: (New Instrument)

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min | Max | ±U | TUR |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|-------|-------|
| °C | | N.A. | | -0.000 | -0.002 | Y | -0.050 | 0.050 | 0.013 | 3.8:1 |
| °C | | N.A. | | 25.001 | 25.000 | Y | 24.951 | 25.051 | 0.014 | 3.6:1 |
| °C | | N.A. | | 80.000 | 80.998 | Y | 59.950 | 60.050 | 0.018 | 2.8:1 |
| °C | | N.A. | | 100.001 | 100.002 | Y | 99.951 | 100.051 | 0.018 | 2.8:1 |

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading, As Left=Instrument's Reading, In Tol=In Tolerance, Min/Max=Acceptance Range, ±U=Expanded Measurement Uncertainty, TUR=Test Uncertainty Ratio, Accuracy=±(Max-Min)/2, Min = As Left Nominal(Rounded) - Tolerance, Max = As Left Nominal(Rounded) + Tolerance, Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4466 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

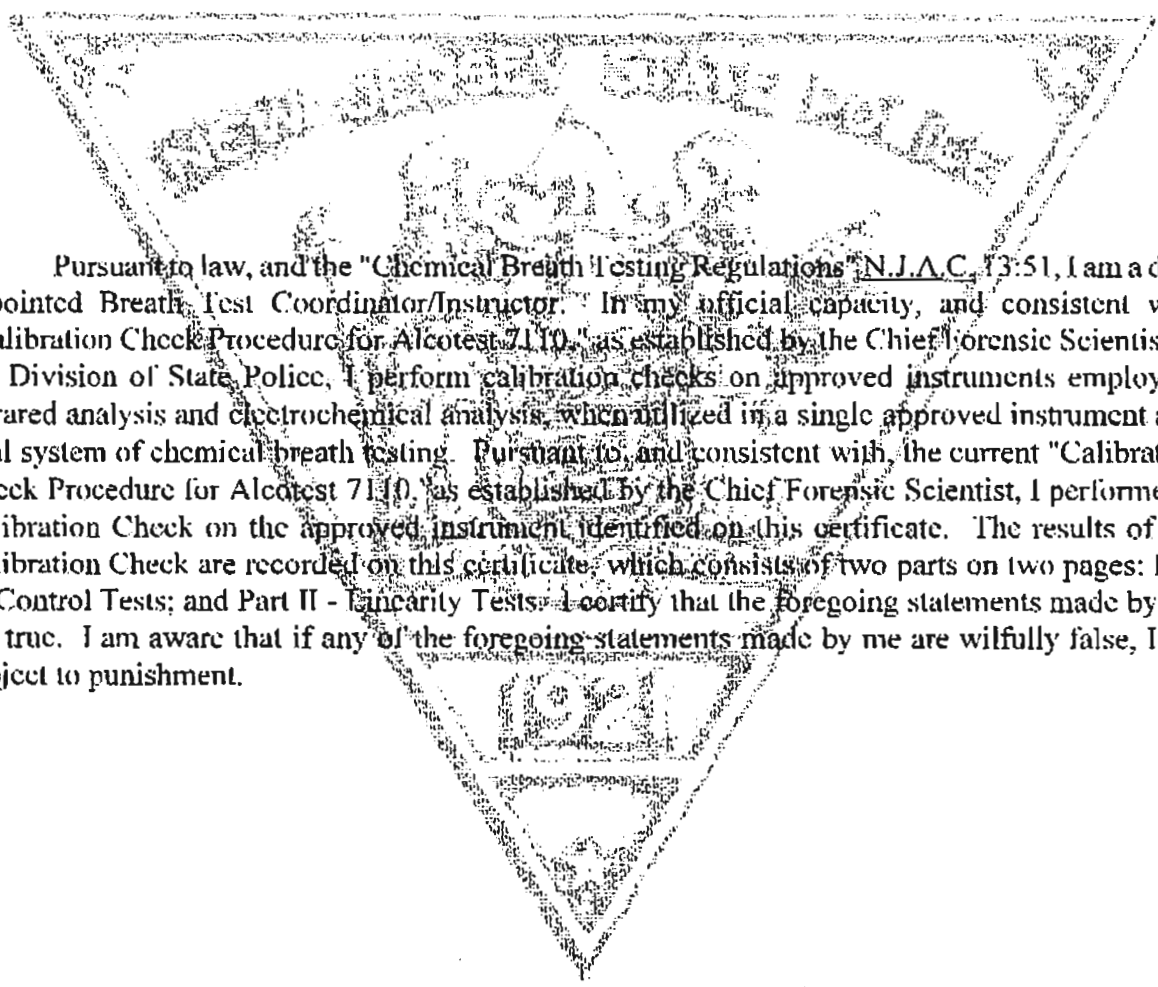
| | | | | | |
|-------------------------|-----------------------|--------------|------------|-------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARUM-0073 | | |
| Location: | MERCHANTVILLE POLICE | | | | |
| Calibration File No.: | 00676 | Calib. Date: | 09/10/2012 | Calib. No.: | 00022 |
| Certification File No.: | 00636 | Cert. Date: | 03/21/2012 | Cert. No.: | 00015 |
| Linearity File No.: | 00637 | Lin. Date: | 03/21/2012 | Lin. No.: | 00015 |
| Solution File No.: | 00675 | Soln. Date: | 09/08/2012 | Soln. No.: | 00133 |
| Sequential File No.: | 00676 | File Date: | 09/10/2012 | | |
| Calibrating Unit: | WET | Model No.: | CU 34 | Serial No.: | DDWA S3-0011 |
| Control Solution %: | 0.100% | | | Expires: | 02/20/2014 |
| Solution Control Lot: | 12B099 | | | Bottle No.: | 1120 |

Coordinator

Last Name: GIBSON First Name: MICHAEL MI: P.
Signature: Michael P. Gibson #6353 Badge No.: 6353
Date: 09/10/2012

- *Black Key Temperature Probe Serial.....# DDLHP1-0073 (MPA)
- *Digital NIST Temperature Measuring System Serial.....# 122172175 (MPA)

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.



Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 00676 **Calib. Date:** 09/10/2012 **Calib. No.:** 00022
Certification File No.: 00677 **Cert. Date:** 09/10/2012 **Cert. No.:** 00016
Linearity File No.: 00637 **Lin. Date:** 03/21/2012 **Lin. No.:** 00015
Solution File No.: 00675 **Soln. Date:** 09/08/2012 **Soln. No.:** 00133
Sequential File No.: 00677 **File Date:** 09/10/2012

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWA S3 0011
Control Solution %: 0.100% **Expires:** 02/20/2014
Solution Control Lot: 12B099 **Bottle No.:** 1120

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 14:03D | | |
| Control 1 EC | 0.098% | 14:04D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 14:04D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:04D | | |
| Control 2 EC | 0.099% | 14:05D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 14:05D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:06D | | |
| Control 3 EC | 0.099% | 14:06D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 14:06D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:07D | | |

All tests within acceptable tolerance.

Coordinator

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature:

John H. Michael P. Gibson #6353

Badge No.: 6353

Date: 09/10/2012

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 00676 Calib. Date: 09/10/2012 Calib. No.: 00022
Certification File No.: 00677 Cert. Date: 09/10/2012 Cert. No.: 00016
Linearity File No.: 00678 Lin. Date: 09/10/2012 Lin. No.: 00016
Solution File No.: 00675 Soln. Date: 09/08/2012 Soln. No.: 00133
Sequential File No.: 00678 File Date: 09/10/2012

Calibrating Unit: WET Model No.: CU 34 Serial No.: DDCB-0001
Control Solution %: 0.040% Expires: 06/27/2013
Solution Control Lot: 11F090 Bottle No.: 0047

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCB-0002
Control Solution %: 0.080% Expires: 06/30/2013
Solution Control Lot: 11F091 Bottle No.: 0370

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBN-0007
Control Solution %: 0.160% Expires: 07/03/2013
Solution Control Lot: 11G092 Bottle No.: 1322


| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 14:18D | | |
| Control 1 EC | 0.040% | 14:19D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.040% | 14:19D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:20D | | |
| Control 2 EC | 0.040% | 14:21D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.040% | 14:21D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:23D | | |
| Control 3 EC | 0.080% | 14:23D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.079% | 14:23D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:25D | | |
| Control 4 EC | 0.080% | 14:25D | 34.0°C | *** TEST PASSED *** |
| Control 4 IR | 0.079% | 14:25D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:27D | | |
| Control 5 EC | 0.158% | 14:28D | 34.0°C | *** TEST PASSED *** |
| Control 5 IR | 0.158% | 14:28D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:29D | | |
| Control 6 EC | 0.158% | 14:30D | 34.0°C | *** TEST PASSED *** |
| Control 6 IR | 0.158% | 14:30D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:31D | | |

All tests within acceptable tolerance.

Coordinator

Last Name: GIBSON First Name: MICHAEL

Signature:

# 6353

MI: P.

Badge No.: 6353

Date: 09/10/2012

DEPARTMENT OF
Law and Public Safety
This is to certify that

Michael P. Gibson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CORRECTLY OPERATE BREATHALYZER PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE
A METHOD TO DETERMINE DRUG ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, ON 10th DAY OF June

TWO THOUSAND AND FIVE
SHERIFF/TREASURER
NEW JERSEY STATE POLICE
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|---------|------------------------|---------------|
| 12/3/07 | OCPA | Wm. [unclear] |
| 3-13-09 | SCPA | Wm. [unclear] |
| 2-3-11 | OCPA | Wm. [unclear] |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |

S.P. 2938 (Rev. 06/03)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Michael Gibson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CORRECTLY OPERATE BREATHALYZER PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE
A METHOD TO DETERMINE DRUG ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, ON 10th DAY OF June

TWO THOUSAND AND ELEVEN
SHERIFF/TREASURER
NEW JERSEY STATE POLICE
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------|------------------------|------------|
| 1. | | |
| 2. | | |
| 3. | | |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |

S.P. 2938 (Rev. 09/10)

DEPARTMENT OF
Law and Public Safety
This is to certify that

MICHAEL P. GIBSON
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CORRECTLY OPERATE BREATHALYZER PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE
A METHOD TO DETERMINE DRUG ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, ON 11th DAY OF October

TWO THOUSAND AND FOUR
SHERIFF/TREASURER
NEW JERSEY STATE POLICE
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 07/21 TO 07/25/2003

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------------|------------------------|------------|
| 1. 7-14-06 | OCPA | [unclear] |
| 2. | | |
| 3. | | |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |

S.P. 2938 (Rev. 03/03)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Michael P. Gibson
North Woodbury City Police

IS QUALIFIED AND COMPETENT TO CORRECTLY OPERATE BREATHALYZER PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE
A METHOD TO DETERMINE DRUG ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, ON 15th DAY OF July

TWO THOUSAND AND 03
SHERIFF/TREASURER
NEW JERSEY STATE POLICE
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------|------------------------|------------|
| 1. | | |
| 2. | | |
| 3. | | |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |

S.P. 2938 (Rev. 06/03)



CERTIFICATE

This is to certify that


Michael P. Gibson #6353

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 18, 2011



Instructor: Hansueli Ryser

Dräger



CIRIUS CHRISTIE
Governor

KIM GUADAGINO
Lieutenant Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF CRIMINAL JUSTICE
PO BOX 085
TRENTON, NJ 08645-0085
TELEPHONE: (609) 984-6560

PAULA T. DOW
Attorney General

STEPHEN J. TAYLOR
Director

June 10, 2011

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification - Trooper Michael Gibson #6353

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C.* 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A.* 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Trooper Michael Gibson #6353, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Paula Dow
Attorney General

- c. Trooper Michael Gibson #6353, Alcohol/Drug Test Unit, Division of State Police
Lt. Craig Potter, Unit Head, Alcohol/Drug Test Unit, Division of State Police





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.


ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F090


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalck, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.


 Notary

Linda L. Decantis
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

PAULA T. DOW
Attorney General

KIM GUADAGNO
Lt. Governor

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 10th day of August, 2011.

Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JEFFREY S. CHIESA
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 3/20/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12B099

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1211 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 20, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Monica L. Tramontin

Monica L. Tramontin
Forensic Scientist III
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 22nd day of March, 2012.

Handwritten signature of Mary Elizabeth McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN
NOTARY PUBLIC OF NEW JERSEY
MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 7/25/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G092

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Kenneth W. Kowalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.

[Signature]
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 9-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDCB-0001

Certification Date

Technician

Re-Certification Due Date

2/2/12

DM

2/2/13



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDCB-0002

Certification Date

Technician

Re-Certification Due Date

3/20/12

DM

3/20/13



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDBN-0007

Certification Date

Technician

Re-Certification Due Date

2/2/12

ZM

2/2/13

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDLHP1-0073

2/3/12

2/3/13

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

ZM

Calibrating Unit

New Standard Solution Report

| | | | |
|--------------------------------|-----------------------|---------------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARUM 0073 |
| Location: | MERCHANTVILLE POLICE | | |
| Calibration File No.: | 00676 | Calib. Date: | 09/10/2012 |
| Certification File No.: | 00677 | Cert. No.: | 00022 |
| Linearity File No.: | 00678 | Cert. Date: | 09/10/2012 |
| Solution File No.: | 00679 | Lin. No.: | 00016 |
| Sequential File No.: | 00679 | Soln. Date: | 09/10/2012 |
| | | Soln. No.: | 00134 |
| | | File Date: | 09/10/2012 |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | DDWA S3-0011 |
| Solution Control Lot: | 11K096 | Expires: | 11/23/2013 |
| | | Bottle No.: | 0777 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 15:34D | | |
| Control 1 EC | 0.100% | 15:35D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 15:35D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:36D | | |
| Control 2 EC | 0.099% | 15:36D | 34.1°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 15:36D | 34.1°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:37D | | |
| Control 3 EC | 0.099% | 15:38D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 15:38D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:38D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDVJP2-168 (MA)

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature:

Michael P. Gibson #6353

Badge No.: 6353

Date: 09/10/2012



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 12/16/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11K096

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1217 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 23, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 5th day of January, 2012.

Handwritten signature of Linda L. Desantis
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

