

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 01020 Calib. Date: 12/08/2020 Calib. No.: 00042
Certification File No.: 01021 Cert. Date: 12/08/2020 Cert. No.: 00035
Linearity File No.: 01022 Lin. Date: 12/08/2020 Lin. No.: 00035
Solution File No.: 01025 Soln. Date: 12/14/2020 Soln. No.: 00277
Sequential File No.: 01025 File Date: 12/14/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0011
Control Solution %: 0.100% Expires: 09/09/2021
Solution Control Lot: 19240 Bottle No.: 0851

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:53S		
Control 1 EC	0.100%	07:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:54S		
Control 2 EC	0.100%	07:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	07:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:56S		
Control 3 EC	0.101%	07:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: Sgt Tom Whalen

Badge No.: 61

Date: 12/14/2020

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0073
Location:	MERCHANTVILLE POLICE	
Calibration File No.:	01004	Calib. Date: 06/30/2020
Certification File No.:	01005	Calib. No.: 00041
Linearity File No.:	01006	Cert. Date: 06/30/2020
Solution File No.:	01019	Cert. No.: 00034
Sequential File No.:	01019	Lin. Date: 06/30/2020
		Lin. No.: 00034
		Soln. Date: 12/01/2020
		Soln. No.: 00275
		File Date: 12/01/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0012
Solution Control Lot:	19240	Expires: 09/09/2021
		Bottle No.: 0847

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:17S		
Control 1 EC	0.099%	18:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:18S		
Control 2 EC	0.099%	18:19S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:19S		
Control 3 EC	0.099%	18:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: _____



Badge No.: 61

Date: 12/01/2020

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 01004 Calib. Date: 06/30/2020 Calib. No.: 00041
Certification File No.: 01005 Cert. Date: 06/30/2020 Cert. No.: 00034
Linearity File No.: 01006 Lin. Date: 06/30/2020 Lin. No.: 00034
Solution File No.: 01018 Soln. Date: 11/08/2020 Soln. No.: 00274
Sequential File No.: 01018 File Date: 11/08/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0012
Control Solution %: 0.100% Expires: 09/09/2021
Solution Control Lot: 19240 Bottle No.: 1178

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:31S		
Control 1 EC	0.101%	10:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33S		
Control 2 EC	0.101%	10:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:34S		
Control 3 EC	0.100%	10:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: 

Badge No.: 61

Date: 11/08/2020

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 01004 Calib. Date: 06/30/2020 Calib. No.: 00041
Certification File No.: 01005 Cert. Date: 06/30/2020 Cert. No.: 00034
Linearity File No.: 01006 Lin. Date: 06/30/2020 Lin. No.: 00034
Solution File No.: 01014 Soln. Date: 10/10/2020 Soln. No.: 00273
Sequential File No.: 01014 File Date: 10/10/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0012
Control Solution %: 0.100% Expires: 09/09/2021
Solution Control Lot: 19240 Bottle No.: 1012

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:45D		
Control 1 EC	0.100%	06:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:46D		
Control 2 EC	0.100%	06:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	06:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:48D		
Control 3 EC	0.100%	06:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	06:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: Sgt. Tom Whalen

Badge No.: 61

Date: 10/10/2020

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0073
Location:	MERCHANTVILLE POLICE	
Calibration File No.:	01004	Calib. Date: 06/30/2020
Certification File No.:	01005	Cert. No.: 00041
Linearity File No.:	01006	Cert. Date: 06/30/2020
Solution File No.:	01012	Lin. No.: 00034
Sequential File No.:	01012	Lin. Date: 06/30/2020
		Soln. No.: 00272
		Soln. Date: 09/17/2020
		File Date: 09/17/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0012
Solution Control Lot:	19240	Expires: 09/09/2021
		Bottle No.: 0854

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:48D		
Control 1 EC	0.101%	02:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:50D		
Control 2 EC	0.100%	02:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:51D		
Control 3 EC	0.100%	02:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	02:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: TALARICO

First Name: FRANK

MI: D

Signature: _____



Badge No.: 59

Date: 09/17/2020

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0073
Location:	MERCHANTVILLE POLICE	
Calibration File No.:	01004	Calib. Date: 06/30/2020
Certification File No.:	01005	Cert. No.: 00041
Linearity File No.:	01006	Cert. Date: 06/30/2020
Solution File No.:	01010	Lin. No.: 00034
Sequential File No.:	01010	Lin. Date: 06/30/2020
		Soln. No.: 00271
		Soln. Date: 08/20/2020
		File Date: 08/20/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0012
Solution Control Lot:	19240	Expires: 09/09/2021
		Bottle No.: 0859

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:37D		
Control 1 EC	0.100%	08:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:39D		
Control 2 EC	0.100%	08:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:40D		
Control 3 EC	0.100%	08:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: _____



Badge No.: 61

Date: 08/20/2020

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0073
Location:	MERCHANTVILLE POLICE	
Calibration File No.:	01004	Calib. Date: 06/30/2020
Certification File No.:	01005	Cert. No.: 00041
Linearity File No.:	01006	Cert. Date: 06/30/2020
Solution File No.:	01008	Lin. No.: 00034
Sequential File No.:	01008	Lin. Date: 06/30/2020
		Soln. No.: 00270
		Soln. Date: 07/22/2020
		File Date: 07/22/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWA S3-0012
Solution Control Lot:	19240	Expires: 09/09/2021
		Bottle No.: 1181

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:38D		
Control 1 EC	0.100%	14:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	14:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:39D		
Control 2 EC	0.100%	14:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	14:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:41D		
Control 3 EC	0.101%	14:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: 

Badge No.: 61

Date: 07/22/2020

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0073
Location:	MERCHANTVILLE POLICE	
Calibration File No.:	00995	Calib. Date: 01/30/2020
Certification File No.:	00996	Calib. No.: 00040
Linearity File No.:	00997	Cert. Date: 01/30/2020
Solution File No.:	01003	Cert. No.: 00033
Sequential File No.:	01003	Lin. Date: 01/30/2020
		Lin. No.: 00033
		Soln. Date: 06/11/2020
		Soln. No.: 00268
		File Date: 06/11/2020

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0011
Control Solution %:	0.100%		Expires: 09/09/2021
Solution Control Lot:	19240		Bottle No.: 0842

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:24D		
Control 1 EC	0.102%	04:24D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:25D		
Control 2 EC	0.101%	04:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:26D		
Control 3 EC	0.101%	04:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: _____



Badge No.: 61

Date: 06/11/2020

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 00995 Calib. Date: 01/30/2020 Calib. No.: 00040
Certification File No.: 00996 Cert. Date: 01/30/2020 Cert. No.: 00033
Linearity File No.: 00997 Lin. Date: 01/30/2020 Lin. No.: 00033
Solution File No.: 01001 Soln. Date: 05/09/2020 Soln. No.: 00267
Sequential File No.: 01001 File Date: 05/09/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0011
Control Solution %: 0.100% Expires: 09/09/2021
Solution Control Lot: 19240 Bottle No.: 0845

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:01D		
Control 1 EC	0.100%	08:01D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		
Control 2 EC	0.099%	08:03D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:04D		
Control 3 EC	0.100%	08:04D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:05D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TALARICO

First Name: FRANK

MI: D

Signature: 

Badge No.: 59

Date: 05/09/2020

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0073
Location:	MERCHANTVILLE POLICE	
Calibration File No.:	00995	Calib. Date: 01/30/2020
Certification File No.:	00996	Cert. No.: 00040
Linearity File No.:	00997	Cert. Date: 01/30/2020
Solution File No.:	01000	Lin. No.: 00033
Sequential File No.:	01000	Soln. Date: 03/23/2020
		Soln. No.: 00266
		File Date: 03/23/2020

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWA S3-0011
Control Solution %:	0.100%		Expires: 09/09/2021
Solution Control Lot:	19240		Bottle No.: 0895

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:01S		
Control 1 EC	0.099%	07:01S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	07:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:02S		
Control 2 EC	0.097%	07:03S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:04S		
Control 3 EC	0.098%	07:04S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHALEN	First Name: TOMAS	MI: F
Signature: <u></u>	Badge No.: 61	Date: 03/23/2020

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0073
Location: MERCHANTVILLE POLICE
Calibration File No.: 00995 Calib. Date: 01/30/2020 Calib. No.: 00040
Certification File No.: 00996 Cert. Date: 01/30/2020 Cert. No.: 00033
Linearity File No.: 00997 Lin. Date: 01/30/2020 Lin. No.: 00033
Solution File No.: 00999 Soln. Date: 02/25/2020 Soln. No.: 00265
Sequential File No.: 00999 File Date: 02/25/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0011
Control Solution %: 0.100% Expires: 09/09/2021
Solution Control Lot: 19240 Bottle No.: 0862

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:13S		
Control 1 EC	0.103%	20:13S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:13S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:14S		
Control 2 EC	0.100%	20:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:15S		
Control 3 EC	0.101%	20:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	20:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:17S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WHALEN

First Name: TOMAS

MI: F

Signature: 

Badge No.: 61

Date: 02/25/2020



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 06/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19150


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 10, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

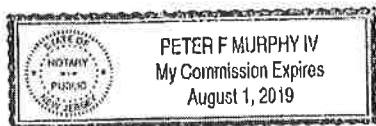

Sworn to and subscribed before me this 26th day of June, 2019.

[Signature]
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0073
Location:	MERCHANTVILLE POLICE		
Calibration File No.:	00973	Calib. Date:	08/29/2019
Certification File No.:	00974	Cert. Date:	08/29/2019
Linearity File No.:	00975	Lin. Date:	08/29/2019
Solution File No.:	00994	Soln. Date:	01/08/2020
Sequential File No.:	00994	File Date:	01/08/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0012
Solution Control Lot:	19150	Expires:	06/10/2021
		Bottle No.:	0182

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:57S		
Control 1 EC	0.099%	11:57S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58S		
Control 2 EC	0.099%	11:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:00S		
Control 3 EC	0.100%	12:00S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:01S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: TALARICO

First Name: FRANK

MI: D

Signature: _____



Badge No.: 59

Date: 01/08/2020