

# Alcotest 7110 Calibration Record


**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 02772 Calib. Date: 10/07/2019 Calib. No.: 00042  
Certification File No.: 02722 Cert. Date: 05/10/2019 Cert. No.: 00031  
Linearity File No.: 02723 Lin. Date: 05/10/2019 Lin. No.: 00030  
Solution File No.: 02761 Soln. Date: 09/20/2019 Soln. No.: 00313  
Sequential File No.: 02772 File Date: 10/07/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
Control Solution %: 0.100% Expires: 07/23/2020  
Solution Control Lot: 18220 Bottle No.: 0456

## Coordinator

Last Name: GAMBONE First Name: BRIAN MI: M  
Signature: TPMI BmG #7029 Badge No.: 7029  
Date: 10/07/2019

\*Black Key Temperature Probe Serial.....# DDMBPI-0016 (BMG)  
\*Digital NIST Temperature Measuring System Serial.....# 191959034 (BMG)

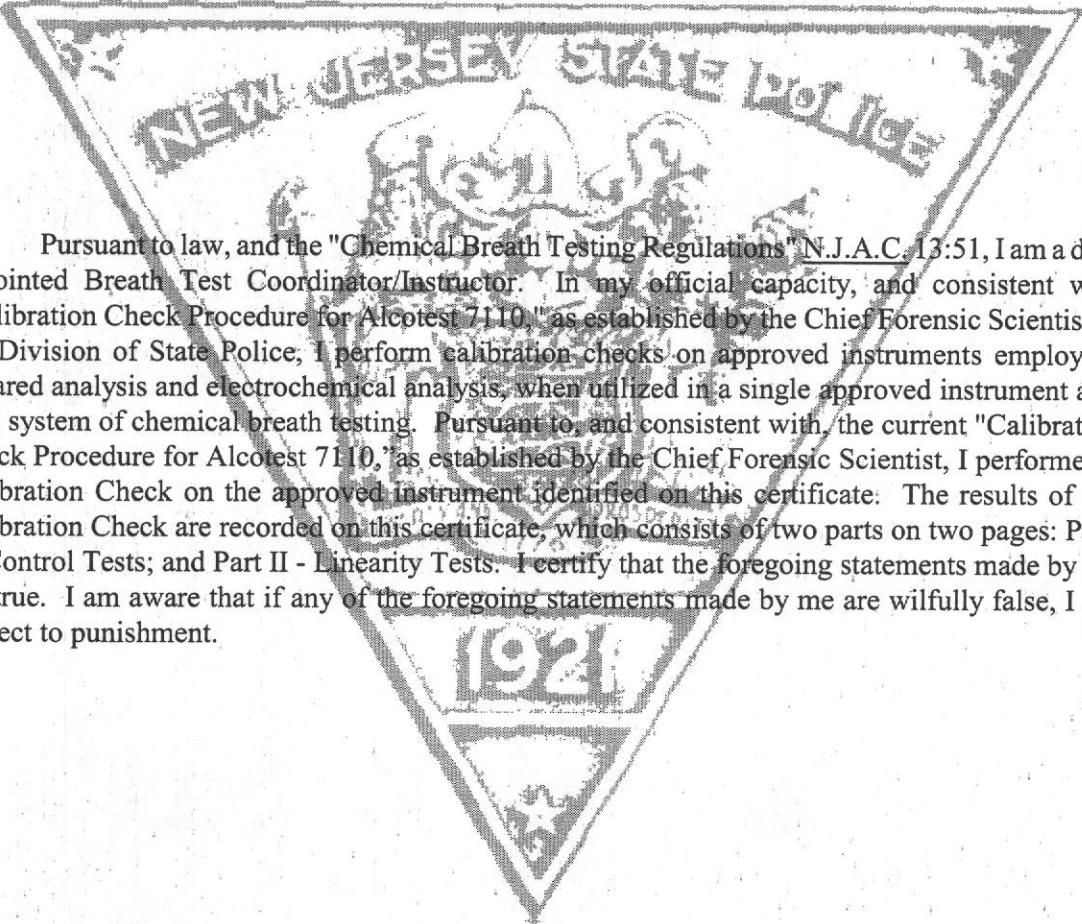

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

### Equipment

Alcotest 7110 MKIII-C  
Location: STRATFORD POLICE DEPT. Serial No.: ARNK-0039  
Calibration File No.: 02772 Calib. Date: 10/07/2019 Calib. No.: 00042  
Certification File No.: 02773 Cert. Date: 10/07/2019 Cert. No.: 00032  
Linearity File No.: 02723 Lin. Date: 05/10/2019 Lin. No.: 00030  
Solution File No.: 02761 Soln. Date: 09/20/2019 Soln. No.: 00313  
Sequential File No.: 02773 File Date: 10/07/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
Control Solution %: 0.100% Expires: 07/23/2020  
Solution Control Lot: 18220 Bottle No.: 0456

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:19D		
Control 1 EC	0.099%	15:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:21D		
Control 2 EC	0.098%	15:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:22D		
Control 3 EC	0.099%	15:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:24D		

All tests within acceptable tolerance.

### Coordinator

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature: TPA. I B. M

# 7029

Badge No.: 7029

Date: 10/07/2019

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.