

# Calibrating Unit New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C  
Location: STRATFORD POLICE DEPT. Serial No.: ARNK-0039  
Calibration File No.: 01136 Calib. Date: 11/23/2011 Calib. No.: 00018  
Certification File No.: 01137 Cert. Date: 11/23/2011 Cert. No.: 00014  
Linearity File No.: 01138 Lin. Date: 11/23/2011 Lin. No.: 00013  
Solution File No.: 01160 Soln. Date: 12/23/2011 Soln. No.: 00135  
Sequential File No.: 01160 File Date: 12/23/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 08/17/2013  
Solution Control Lot: 11H094 Bottle No.: 0693

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:35S		
Control 1 EC	0.100%	10:36S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:37S		
Control 2 EC	0.099%	10:38S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		
Control 3 EC	0.100%	10:39S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

M1: M

Signature:  63200

Badge No.: 3200

Date: 12/23/2011

# Calibrating Unit

## New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C		Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.		
Calibration File No.: 01136	Calib. Date: 11/23/2011	Calib. No.: 00018
Certification File No.: 01137	Cert. Date: 11/23/2011	Cert. No.: 00014
Linearity File No.: 01138	Lin. Date: 11/23/2011	Lin. No.: 00013
Solution File No.: 01148	Soln. Date: 12/02/2011	Soln. No.: 00134
Sequential File No.: 01148	File Date: 12/02/2011	

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %: 0.100%		Expires: 10/04/2012
Solution Control Lot: 10J083		Bottle No.: 1051

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:23S		
Control 1 EC	0.099%	03:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	03:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:24S		
Control 2 EC	0.097%	03:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:25S		
Control 3 EC	0.097%	03:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	03:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: \_\_\_\_\_

*# 322*

Badge No.: 3202

Date: 12/02/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01024	Calib. Date:	06/23/2011
Certification File No.:	01025	Cert. Date:	06/23/2011
Linearity File No.:	01026	Lin. Date:	06/23/2011
Solution File No.:	01127	Soln. Date:	11/12/2011
Sequential File No.:	01127	File Date:	11/12/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	10J083	Expires:	10/04/2012
		Bottle No.:	1071

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:49S		
Control 1 EC	0.098%	11:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50S		
Control 2 EC	0.098%	11:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		
Control 3 EC	0.098%	11:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_



Badge No.: 3200

Date: 11/12/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01024	Calib. Date: 06/23/2011
Certification File No.:	01025	Calib. No.: 00017
Linearity File No.:	01026	Cert. Date: 06/23/2011
Solution File No.:	01111	Cert. No.: 00013
Sequential File No.:	01111	Lin. Date: 06/23/2011
		Lin. No.: 00012
		Soln. Date: 10/23/2011
		Soln. No.: 00131
		File Date: 10/23/2011

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 10/04/2012
Solution Control Lot:	10J083		Bottle No.: 1072

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:28D		
Control 1 EC	0.099%	12:28D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29D		
Control 2 EC	0.098%	12:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 3 EC	0.099%	12:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_



Badge No.: 3200

Date: 10/23/2011

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01107 Soln. Date: 10/19/2011 Soln. No.: 00130  
Sequential File No.: 01107 File Date: 10/19/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1052

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:16D		
Control 1 EC	0.098%	13:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	13:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		
Control 2 EC	0.097%	13:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18D		
Control 3 EC	0.097%	13:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 10/19/2011

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01105 Soln. Date: 10/09/2011 Soln. No.: 00129  
Sequential File No.: 01105 File Date: 10/09/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1065

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:50D		
Control 1 EC	0.098%	02:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:51D		
Control 2 EC	0.097%	02:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:52D		
Control 3 EC	0.098%	02:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	02:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: \_\_\_\_\_

*Sgt. R Kelly*

# 304

Badge No.: 3204

Date: 10/09/2011

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01089 Soln. Date: 09/27/2011 Soln. No.: 00128  
Sequential File No.: 01089 File Date: 09/27/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1066

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:52D		
Control 1 EC	0.099%	15:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:53D		
Control 2 EC	0.097%	15:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:54D		
Control 3 EC	0.098%	15:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:56D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 09/27/2011

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01085 Soln. Date: 09/24/2011 Soln. No.: 00127  
Sequential File No.: 01085 File Date: 09/24/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1074

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:17D		
Control 1 EC	0.099%	05:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:18D		
Control 2 EC	0.097%	05:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	05:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:20D		
Control 3 EC	0.098%	05:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	05:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: Sgt. R.A. Kelly # 3204

Badge No.: 3204

Date: 09/24/2011



# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01073 Soln. Date: 09/10/2011 Soln. No.: 00126  
Sequential File No.: 01073 File Date: 09/10/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1075

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:14D		
Control 1 EC	0.098%	06:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	06:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:15D		
Control 2 EC	0.097%	06:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	06:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:16D		
Control 3 EC	0.097%	06:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	06:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: KELLY

First Name: ROBERT

M1: J

Signature: \_\_\_\_\_



Badge No.: 3204

Date: 09/10/2011

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01062 Soln. Date: 08/21/2011 Soln. No.: 00125  
Sequential File No.: 01062 File Date: 08/21/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1068

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:17D		
Control 1 EC	0.097%	04:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	04:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:18D		
Control 2 EC	0.096%	04:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	04:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:20D		
Control 3 EC	0.097%	04:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	04:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: \_\_\_\_\_

*Sgt R Kelly #3204*

Badge No.: 3204

Date: 08/21/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01024	Calib. Date:	06/23/2011
Certification File No.:	01025	Cert. Date:	06/23/2011
Linearity File No.:	01026	Lin. Date:	06/23/2011
Solution File No.:	01051	Soln. Date:	08/07/2011
Sequential File No.:	01051	File Date:	08/07/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	10J083	Expires:	10/04/2012
		Bottle No.:	1061

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:51D		
Control 1 EC	0.098%	03:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	03:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:52D		
Control 2 EC	0.097%	03:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:54D		
Control 3 EC	0.097%	03:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	03:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: \_\_\_\_\_

*[Handwritten Signature]* # 32-2

Badge No.: 3202

Date: 08/07/2011

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01024 Calib. Date: 06/23/2011 Calib. No.: 00017  
Certification File No.: 01025 Cert. Date: 06/23/2011 Cert. No.: 00013  
Linearity File No.: 01026 Lin. Date: 06/23/2011 Lin. No.: 00012  
Solution File No.: 01048 Soln. Date: 08/02/2011 Soln. No.: 00123  
Sequential File No.: 01048 File Date: 08/02/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1067

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:00D		
Control 1 EC	0.098%	11:01D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	11:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:02D		
Control 2 EC	0.098%	11:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03D		
Control 3 EC	0.098%	11:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GAGLIARDI

First Name: FRANK

MI: J

Signature: 

Badge No.: 3203

Date: 08/02/2011

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01024	Calib. Date: 06/23/2011
Certification File No.:	01025	Calib. No.: 00017
Linearity File No.:	01026	Cert. Date: 06/23/2011
Solution File No.:	01041	Cert. No.: 00013
Sequential File No.:	01041	Lin. Date: 06/23/2011
		Lin. No.: 00012
		Soln. Date: 07/10/2011
		Soln. No.: 00122
		File Date: 07/10/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1062

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:06D		
Control 1 EC	0.099%	23:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:07D		
Control 2 EC	0.098%	23:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	23:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:08D		
Control 3 EC	0.099%	23:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:10D		

All tests within acceptable tolerance.



On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: KELLY

First Name: ROBERT

MI: J

Signature:  

Badge No.: 3204

Date: 07/10/2011

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 00933 Calib. Date: 01/19/2011 Calib. No.: 00016  
Certification File No.: 00934 Cert. Date: 01/19/2011 Cert. No.: 00012  
Linearity File No.: 00935 Lin. Date: 01/19/2011 Lin. No.: 00011  
Solution File No.: 01011 Soln. Date: 05/29/2011 Soln. No.: 00119  
Sequential File No.: 01011 File Date: 05/29/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
Control Solution %: 0.100% Expires: 10/04/2012  
Solution Control Lot: 10J083 Bottle No.: 1060

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:06D		
Control 1 EC	0.101%	14:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07D		
Control 2 EC	0.100%	14:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:09D		
Control 3 EC	0.100%	14:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	14:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: \_\_\_\_\_



Badge No.: 3204

Date: 05/29/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00933	Calib. Date: 01/19/2011
Certification File No.:	00934	Calib. No.: 00016
Linearity File No.:	00935	Cert. Date: 01/19/2011
Solution File No.:	00994	Cert. No.: 00012
Sequential File No.:	00994	Lin. Date: 01/19/2011
		Lin. No.: 00011
		Soln. Date: 05/04/2011
		Soln. No.: 00118
		File Date: 05/04/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1055

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:11D		
Control 1 EC	0.101%	15:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:12D		
Control 2 EC	0.102%	15:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:13D		
Control 3 EC	0.101%	15:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	15:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

Badge No.: 3200

Date: 05/04/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00933	Calib. No.: 00016
Certification File No.:	00934	Cert. No.: 00012
Linearity File No.:	00935	Lin. No.: 00011
Solution File No.:	00982	Soln. No.: 00117
Sequential File No.:	00982	File Date: 04/09/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1064

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:53D		
Control 1 EC	0.101%	15:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	15:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:54D		
Control 2 EC	0.101%	15:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	15:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:56D		
Control 3 EC	0.102%	15:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	15:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: \_\_\_\_\_



Badge No.: 3204

Date: 04/09/2011



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00933	Calib. Date: 01/19/2011
Certification File No.:	00934	Calib. No.: 00016
Linearity File No.:	00935	Cert. Date: 01/19/2011
Solution File No.:	00981	Cert. No.: 00012
Sequential File No.:	00981	Lin. Date: 01/19/2011
		Lin. No.: 00011
		Soln. Date: 04/09/2011
		Soln. No.: 00116
		File Date: 04/09/2011

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %:	0.100%		Expires: 10/04/2012
Solution Control Lot:	10J083		Bottle No.: 1056

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:00D		
Control 1 EC	0.102%	12:00D	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	-.---%	12:00D	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	12:01D		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

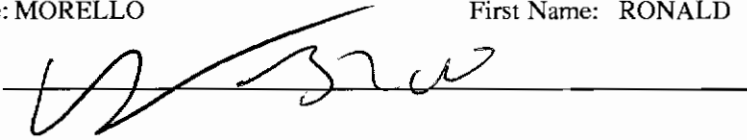

Badge No.: 3200

Date: 04/09/2011

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	00933	Calib. Date:	01/19/2011
Certification File No.:	00934	Cert. Date:	01/19/2011
Linearity File No.:	00935	Lin. Date:	01/19/2011
Solution File No.:	00960	Soln. Date:	03/14/2011
Sequential File No.:	00960	File Date:	03/14/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	10J083	Expires:	10/04/2012
		Bottle No.:	1054

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:29S		
Control 1 EC	0.101%	16:29S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:30S		
Control 2 EC	0.101%	16:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:31S		
Control 3 EC	0.101%	16:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	16:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

Badge No.: 3200

Date: 03/14/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00933	Calib. No.: 00016
Certification File No.:	00934	Cert. No.: 00012
Linearity File No.:	00935	Lin. No.: 00011
Solution File No.:	00946	Soln. No.: 00113
Sequential File No.:	00946	File Date: 02/15/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	10J083	Expires: 10/04/2012
		Bottle No.: 1057

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:40S		
Control 1 EC	0.100%	10:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 2 EC	0.100%	10:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		
Control 3 EC	0.099%	10:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

[Handwritten Signature]

63200

Badge No.: 3200

Date: 02/15/2011

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00858	Calib. Date: 08/24/2010
Certification File No.:	00859	Calib. No.: 00013
Linearity File No.:	00860	Cert. Date: 08/24/2010
Solution File No.:	00929	Cert. No.: 00011
Sequential File No.:	00929	Lin. Date: 08/24/2010
		Lin. No.: 00010
		Soln. Date: 01/03/2011
		Soln. No.: 00109
		File Date: 01/03/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0691

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:03S		
Control 1 EC	0.100%	04:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:05S		
Control 2 EC	0.098%	04:05S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:05S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:06S		
Control 3 EC	0.098%	04:07S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:07S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: \_\_\_\_\_

*# 3202*

Badge No.: 3202

Date: 01/03/2011