

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02647	Calib. Date: 11/29/2018
Certification File No.:	02648	Calib. No.: 00040
Linearity File No.:	02649	Cert. Date: 11/29/2018
Solution File No.:	02659	Cert. No.: 00030
Sequential File No.:	02659	Lin. Date: 11/29/2018
		Lin. No.: 00029
		Soln. Date: 12/21/2018
		Soln. No.: 00299
		File Date: 12/21/2018

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	18090	Expires: 03/13/2020
		Bottle No.: 0672

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:03S		
Control 1 EC	0.101%	11:04S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04S		
Control 2 EC	0.101%	11:05S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06S		
Control 3 EC	0.101%	11:07S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:07S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 12/21/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02572	Calib. Date:	06/13/2018
Certification File No.:	02573	Cert. Date:	06/13/2018
Linearity File No.:	02574	Lin. Date:	06/13/2018
Solution File No.:	02639	Soln. Date:	11/15/2018
Sequential File No.:	02639	File Date:	11/15/2018

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	03/13/2020
Solution Control Lot:	18090			Bottle No.:	0299

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:39S		
Control 1 EC	0.097%	16:40S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	16:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:41S		
Control 2 EC	0.096%	16:41S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	16:41S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:42S		
Control 3 EC	0.096%	16:43S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	16:43S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:44S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 11/15/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02572	Calib. Date: 06/13/2018
Certification File No.:	02573	Calib. No.: 00039
Linearity File No.:	02574	Cert. Date: 06/13/2018
Solution File No.:	02637	Cert. No.: 00029
Sequential File No.:	02637	Lin. Date: 06/13/2018
		Lin. No.: 00028
		Soln. Date: 11/10/2018
		Soln. No.: 00296
		File Date: 11/10/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	18090	Expires: 03/13/2020
		Bottle No.: 0661

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:53S		
Control 1 EC	0.098%	15:54S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:54S		
Control 2 EC	0.098%	15:55S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:56S		
Control 3 EC	0.098%	15:56S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 11/10/2018

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: STRATFORD POLICE DEPT.
Serial No.: ARNK-0039
Calibration File No.: 02572 Calib. Date: 06/13/2018 Calib. No.: 00039
Certification File No.: 02573 Cert. Date: 06/13/2018 Cert. No.: 00029
Linearity File No.: 02574 Lin. Date: 06/13/2018 Lin. No.: 00028
Solution File No.: 02633 Soln. Date: 10/22/2018 Soln. No.: 00295
Sequential File No.: 02633 File Date: 10/22/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 03/13/2020
Solution Control Lot: 18090 Bottle No.: 0365

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:39D		
Control 1 EC	0.095%	10:39D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	10:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40D		
Control 2 EC	0.096%	10:41D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41D		
Control 3 EC	0.096%	10:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 10/22/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02572	Calib. Date:	06/13/2018
Certification File No.:	02573	Cert. Date:	06/13/2018
Linearity File No.:	02574	Lin. Date:	06/13/2018
Solution File No.:	02628	Soln. Date:	10/17/2018
Sequential File No.:	02628	File Date:	10/17/2018
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0310

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:43D		
Control 1 EC	0.095%	08:44D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	08:44D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:45D		
Control 2 EC	0.095%	08:45D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	08:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:46D		
Control 3 EC	0.096%	08:47D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	08:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



3201

Badge No.: 3201

Date: 10/17/2018

Calibrating Unit

New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02572	Calib. Date:	06/13/2018
Certification File No.:	02573	Cert. No.:	00039
Linearity File No.:	02574	Cert. Date:	06/13/2018
Solution File No.:	02617	Lin. Date:	06/13/2018
Sequential File No.:	02617	Lin. No.:	00028
		Soln. Date:	09/23/2018
		Soln. No.:	00293
		File Date:	09/23/2018
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0496

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:17D		
Control 1 EC	0.097%	10:18D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	10:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:18D		
Control 2 EC	0.097%	10:19D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		
Control 3 EC	0.097%	10:20D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO	First Name: RONALD	MI: M
Signature: 		Badge No.: 3200
		Date: 09/23/2018

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
 Location: STRATFORD POLICE DEPT.
 Calibration File No.: 02572 Calib. Date: 06/13/2018 Cafib. No.: 00039
 Certification File No.: 02573 Cert. Date: 06/13/2018 Cert. No.: 00029
 Linearity File No.: 02574 Lin. Date: 06/13/2018 Lin. No.: 00028
 Solution File No.: 02604 Soln. Date: 09/01/2018 Soln. No.: 00291
 Sequential File No.: 02604 File Date: 09/01/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
 Control Solution %: 0.100% Expires: 03/13/2020
 Solution Control Lot: 18090 Bottle No.: 0668

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:12D		
Control 1 EC	0.097%	10:12D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13D		
Control 2 EC	0.097%	10:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:15D		
Control 3 EC	0.097%	10:15D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3201

Date: 09/01/2018

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 02572 Calib. Date: 06/13/2018 Calib. No.: 00039
Certification File No.: 02573 Cert. Date: 06/13/2018 Cert. No.: 00029
Linearity File No.: 02574 Lin. Date: 06/13/2018 Lin. No.: 00028
Solution File No.: 02600 Soln. Date: 08/18/2018 Soln. No.: 00290
Sequential File No.: 02600 File Date: 08/18/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 03/13/2020
Solution Control Lot: 18090 Bottle No.: 0187

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:39D		
Control 1 EC	0.097%	14:39D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	14:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:40D		
Control 2 EC	0.096%	14:41D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	14:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:41D		
Control 3 EC	0.096%	14:42D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:43D		

All tests within acceptable tolerance.

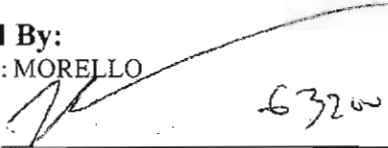
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 08/18/2018



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 04/04/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18090

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1215 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 13, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Ali M. Alaoui, Ph.D.
Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of April, 2018.

Handwritten signature of Notary
Notary

PETER F MURPHY IV
My Commission Expires
August 1, 2019



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.	Calib. No.:	00039
Calibration File No.:	02572	Calib. Date:	06/13/2018
Certification File No.:	02573	Cert. Date:	06/13/2018
Linearity File No.:	02574	Lin. Date:	06/13/2018
Solution File No.:	02594	Soln. Date:	07/26/2018
Sequential File No.:	02594	File Date:	07/26/2018
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0669

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:13D		
Control 1 EC	0.099%	10:14D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14D		
Control 2 EC	0.098%	10:15D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16D		
Control 3 EC	0.098%	10:17D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 07/26/2018

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02572	Calib. Date: 06/13/2018
Certification File No.:	02573	Calib. No.: 00039
Linearity File No.:	02574	Cert. Date: 06/13/2018
Solution File No.:	02591	Cert. No.: 00029
Sequential File No.:	02591	Lin. Date: 06/13/2018
		Lin. No.: 00028
		Soln. Date: 07/14/2018
		Soln. No.: 00288
		File Date: 07/14/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	17420	Expires: 12/11/2019
		Bottle No.: 1472

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:24D		
Control 1 EC	0.098%	12:25D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:25D		
Control 2 EC	0.097%	12:26D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	12:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:27D		
Control 3 EC	0.098%	12:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3201

Date: 07/14/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02572	Calib. Date: 06/13/2018
Certification File No.:	02573	Calib. No.: 00039
Linearity File No.:	02574	Cert. Date: 06/13/2018
Solution File No.:	02590	Cert. No.: 00029
Sequential File No.:	02590	Lin. Date: 06/13/2018
		Lin. No.: 00028
		Soln. Date: 07/14/2018
		Soln. No.: 00287
		File Date: 07/14/2018

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 12/11/2019
Solution Control Lot:	17420		Bottle No.: 1491

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:39D		
Control 1 EC	0.096%	10:40D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	10:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40D		
Control 2 EC	0.096%	10:41D	33.9°C	CONTROL TEST FAILED
Control 2 IR	0.094%	10:41D	33.9°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	10:42D		
Control 3 EC	0.096%	10:43D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	10:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3201

Date: 07/14/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02572	Calib. Date: 06/13/2018
Certification File No.:	02573	Calib. No.: 00039
Linearity File No.:	02574	Cert. Date: 06/13/2018
Solution File No.:	02582	Cert. No.: 00029
Sequential File No.:	02582	Lin. Date: 06/13/2018
		Lin. No.: 00028
		Soln. Date: 06/27/2018
		Soln. No.: 00286
		File Date: 06/27/2018

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 12/11/2019
Solution Control Lot:	17420		Bottle No.: 1461

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:09D		
Control 1 EC	0.097%	08:10D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	08:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:11D		
Control 2 EC	0.096%	08:11D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	08:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12D		
Control 3 EC	0.097%	08:13D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3201

Date: 06/27/2018

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 02519 Calib. Date: 12/22/2017 Calib. No.: 00038
Certification File No.: 02520 Cert. Date: 12/22/2017 Cert. No.: 00028
Linearity File No.: 02521 Lin. Date: 12/22/2017 Lin. No.: 00027
Solution File No.: 02560 Soln. Date: 05/17/2018 Soln. No.: 00284
Sequential File No.: 02560 File Date: 05/17/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
Control Solution %: 0.100% Expires: 12/11/2019
Solution Control Lot: 17420 Bottle No.: 1471

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:34D		
Control 1 EC	0.103%	01:35D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	01:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:35D		
Control 2 EC	0.101%	01:36D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	01:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:37D		
Control 3 EC	0.101%	01:37D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:38D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GAGLIARDI

First Name: FRANK

MI: J

Signature:  *3203

Badge No.: 3203

Date: 05/17/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02519	Calib. Date:	12/22/2017
Certification File No.:	02520	Cert. Date:	12/22/2017
Linearity File No.:	02521	Lin. Date:	12/22/2017
Solution File No.:	02559	Soln. Date:	05/16/2018
Sequential File No.:	02559	File Date:	05/16/2018

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0163
Control Solution %:	0.100%			Expires:	12/11/2019
Solution Control Lot:	17420			Bottle No.:	1477

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:32D		
Control 1 EC	-.---%	22:33D	21.8°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	22:33D	21.8°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

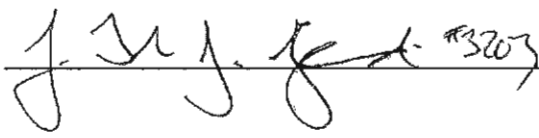
Changed By:

Last Name: GAGLIARDI

First Name: FRANK

MI: J

Signature: _____



Badge No.: 3203

Date: 05/16/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02519	Calib. Date:	12/22/2017
Certification File No.:	02520	Cert. No.:	00038
Linearity File No.:	02521	Cert. Date:	12/22/2017
Solution File No.:	02556	Lin. No.:	00027
Sequential File No.:	02556	Soln. Date:	04/25/2018
		Soln. No.:	00282
		File Date:	04/25/2018
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	16140	Expires:	06/07/2018
		Bottle No.:	1158

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:23D		
Control 1 EC	0.099%	10:24D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:25D		
Control 2 EC	0.099%	10:25D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:26D		
Control 3 EC	0.098%	10:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:27D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 04/25/2018

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02519	Calib. Date: 12/22/2017
Certification File No.:	02520	Calib. No.: 00038
Linearity File No.:	02521	Cert. Date: 12/22/2017
Solution File No.:	02547	Cert. No.: 00028
Sequential File No.:	02547	Lin. Date: 12/22/2017
		Lin. No.: 00027
		Soln. Date: 03/23/2018
		Soln. No.: 00281
		File Date: 03/23/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	16140	Expires: 06/07/2018
		Bottle No.: 0799

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:48S		
Control 1 EC	0.099%	09:48S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:48S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49S		
Control 2 EC	0.098%	09:50S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50S		
Control 3 EC	0.097%	09:51S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 03/23/2018

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02519	Calib. Date: 12/22/2017
Certification File No.:	02520	Calib. No.: 00038
Linearity File No.:	02521	Cert. Date: 12/22/2017
Solution File No.:	02543	Cert. No.: 00028
Sequential File No.:	02543	Lin. Date: 12/22/2017
		Lin. No.: 00027
		Soln. Date: 02/27/2018
		Soln. No.: 00280
		File Date: 02/27/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	16140	Expires: 06/07/2018
		Bottle No.: 1451

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:34S		
Control 1 EC	0.099%	10:35S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		
Control 2 EC	0.098%	10:36S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:36S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:37S		
Control 3 EC	0.098%	10:38S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 02/27/2018

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02519	Calib. Date: 12/22/2017
Certification File No.:	02520	Calib. No.: 00038
Linearity File No.:	02521	Cert. Date: 12/22/2017
Solution File No.:	02531	Cert. No.: 00028
Sequential File No.:	02531	Lin. Date: 12/22/2017
		Lin. No.: 00027
		Soln. Date: 02/02/2018
		Soln. No.: 00279
		File Date: 02/02/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	16140	Expires: 06/07/2018
		Bottle No.: 1493

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:53S		
Control 1 EC	0.099%	10:54S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:55S		
Control 2 EC	0.098%	10:55S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:56S		
Control 3 EC	0.098%	10:57S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:58S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



3201

Badge No.: 3201

Date: 02/02/2018

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 02519 Calib. Date: 12/22/2017 Calib. No.: 00038
Certification File No.: 02520 Cert. Date: 12/22/2017 Cert. No.: 00028
Linearity File No.: 02521 Lin. Date: 12/22/2017 Lin. No.: 00027
Solution File No.: 02526 Soln. Date: 01/07/2018 Soln. No.: 00278
Sequential File No.: 02526 File Date: 01/07/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
Control Solution %: 0.100% Expires: 06/07/2018
Solution Control Lot: 16140 Bottle No.: 1284

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:51S		
Control 1 EC	0.098%	11:52S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.095%	11:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53S		
Control 2 EC	0.097%	11:54S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	11:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54S		
Control 3 EC	0.097%	11:55S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	11:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3201

Date: 01/07/2018