

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	03078	Calib. Date:	10/13/2022
Certification File No.:	03079	Cert. No.:	00049
Linearity File No.:	03080	Cert. Date:	10/13/2022
Solution File No.:	03091	Lin. No.:	00038
Sequential File No.:	03091	Soln. Date:	12/28/2022
		Soln. No.:	00367
		File Date:	12/28/2022

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0163
Control Solution %:	0.100%			Expires:	05/09/2024
Solution Control Lot:	22160			Bottle No.:	1056

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:35S		
Control 1 EC	0.100%	02:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	02:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:36S		
Control 2 EC	0.100%	02:37S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:38S		
Control 3 EC	0.100%	02:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:39S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3204

Date: 12/28/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03078	Calib. No.: 00049
Certification File No.:	03079	Cert. No.: 00039
Linearity File No.:	03080	Lin. No.: 00038
Solution File No.:	03089	Soln. No.: 00366
Sequential File No.:	03089	File Date: 12/03/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 0837

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:16S		
Control 1 EC	0.099%	13:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18S		
Control 2 EC	0.099%	13:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19S		
Control 3 EC	0.099%	13:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3205

Date: 12/03/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03078	Calib. Date: 10/13/2022
Certification File No.:	03079	Calib. No.: 00049
Linearity File No.:	03080	Cert. Date: 10/13/2022
Solution File No.:	03086	Cert. No.: 00039
Sequential File No.:	03086	Lin. Date: 10/13/2022
		Lin. No.: 00038
		Soln. Date: 11/09/2022
		Soln. No.: 00365
		File Date: 11/09/2022

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 1292

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:46S		
Control 1 EC	0.100%	03:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:47S		
Control 2 EC	0.099%	03:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	03:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:49S		
Control 3 EC	0.100%	03:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	03:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3205

Date: 11/09/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03031	Calib. Date: 05/03/2022
Certification File No.:	03032	Calib. No.: 00048
Linearity File No.:	03033	Cert. Date: 05/03/2022
Solution File No.:	03077	Cert. No.: 00038
Sequential File No.:	03077	Lin. Date: 05/03/2022
		Lin. No.: 00037
		Soln. Date: 10/07/2022
		Soln. No.: 00363
		File Date: 10/07/2022

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 0959

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:56D		
Control 1 EC	0.100%	21:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:57D		
Control 2 EC	0.099%	21:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	21:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:59D		
Control 3 EC	0.099%	21:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	21:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3205

Date: 10/07/2022

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03031	Calib. Date: 05/03/2022
Certification File No.:	03032	Calib. No.: 00048
Linearity File No.:	03033	Cert. Date: 05/03/2022
Solution File No.:	03066	Cert. No.: 00038
Sequential File No.:	03066	Lin. Date: 05/03/2022
		Lin. No.: 00037
		Soln. Date: 09/09/2022
		Soln. No.: 00362
		File Date: 09/09/2022

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 1211

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:58D		
Control 1 EC	0.100%	16:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00D		
Control 2 EC	0.099%	17:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:01D		
Control 3 EC	0.100%	17:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3205

Date: 09/09/2022



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 05/23/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22160

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is May 9, 2024.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 26 day of May, 2022.

Notary signature

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 6/19/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03031	Calib. Date: 05/03/2022
Certification File No.:	03032	Calib. No.: 00048
Linearity File No.:	03033	Cert. Date: 05/03/2022
Solution File No.:	03064	Cert. No.: 00038
Sequential File No.:	03064	Lin. Date: 05/03/2022
		Lin. No.: 00037
		Soln. Date: 08/19/2022
		Soln. No.: 00361
		File Date: 08/19/2022

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %: 0.100%		Expires: 09/22/2022
Solution Control Lot: 20390		Bottle No.: 0965

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:43D		
Control 1 EC	0.099%	16:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:45D		
Control 2 EC	0.098%	16:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:46D		
Control 3 EC	0.099%	16:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3205

Date: 08/19/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03031	Calib. Date: 05/03/2022
Certification File No.:	03032	Calib. No.: 00048
Linearity File No.:	03033	Cert. Date: 05/03/2022
Solution File No.:	03059	Cert. No.: 00038
Sequential File No.:	03059	Lin. Date: 05/03/2022
		Lin. No.: 00037
		Soln. Date: 07/24/2022
		Soln. No.: 00360
		File Date: 07/24/2022

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 09/02/2022
Solution Control Lot:	20390		Bottle No.: 1104

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:20D		
Control 1 EC	0.100%	23:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:21D		
Control 2 EC	0.098%	23:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	23:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:22D		
Control 3 EC	0.099%	23:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3205

Date: 07/24/2022



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03031	Calib. Date: 05/03/2022
Certification File No.:	03032	Calib. No.: 00048
Linearity File No.:	03033	Cert. Date: 05/03/2022
Solution File No.:	03051	Cert. No.: 00038
Sequential File No.:	03051	Lin. Date: 05/03/2022
		Lin. No.: 00037
		Soln. Date: 06/27/2022
		Soln. No.: 00359
		File Date: 06/27/2022

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	20390	Expires: 09/02/2022
		Bottle No.: 0940

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:12D		
Control 1 EC	0.100%	23:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:13D		
Control 2 EC	0.100%	23:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	23:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:15D		
Control 3 EC	0.100%	23:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3205

Date: 06/27/2022

# Calibrating Unit New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C  
Location: STRATFORD POLICE DEPT. Serial No.: ARNK-0039  
Calibration File No.: 03031 Calib. Date: 05/03/2022 Calib. No.: 00048  
Certification File No.: 03032 Cert. Date: 05/03/2022 Cert. No.: 00038  
Linearity File No.: 03033 Lin. Date: 05/03/2022 Lin. No.: 00037  
Solution File No.: 03045 Soln. Date: 06/03/2022 Soln. No.: 00358  
Sequential File No.: 03045 File Date: 06/03/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 09/02/2022  
Solution Control Lot: 20390 Bottle No.: 1086

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:42D		
Control 1 EC	0.101%	04:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	04:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:44D		
Control 2 EC	0.100%	04:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	04:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:45D		
Control 3 EC	0.100%	04:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:47D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: 

Badge No.: 3205

Date: 06/03/2022

# Calibrating Unit New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C		Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02989	Calib. Date: 12/09/2021
Certification File No.:	02990	Calib. No.: 00047
Linearity File No.:	02991	Cert. Date: 12/09/2021
Solution File No.:	03028	Lin. No.: 00036
Sequential File No.:	03028	Soln. Date: 04/20/2022
		Soln. No.: 00356
		File Date: 04/20/2022

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0163
Control Solution %:	0.100%			Expires:	09/02/2022
Solution Control Lot:	20390			Bottle No.:	0880

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:48D		
Control 1 EC	0.099%	19:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	19:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:49D		
Control 2 EC	0.097%	19:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:51D		
Control 3 EC	0.098%	19:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

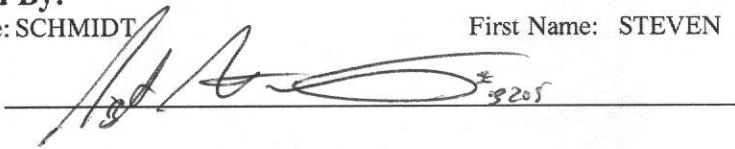

Badge No.: 3205

Date: 04/20/2022

# Calibrating Unit

## New Standard Solution Report

### Equipment

Alcotest 7110 MKIII-C  
Location: STRATFORD POLICE DEPT. Serial No.: ARNK-0039  
Calibration File No.: 02989 Calib. Date: 12/09/2021 Calib. No.: 00047  
Certification File No.: 02990 Cert. Date: 12/09/2021 Cert. No.: 00037  
Linearity File No.: 02991 Lin. Date: 12/09/2021 Lin. No.: 00036  
Solution File No.: 03020 Soln. Date: 03/25/2022 Soln. No.: 00355  
Sequential File No.: 03020 File Date: 03/25/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
Control Solution %: 0.100% Expires: 09/02/2022  
Solution Control Lot: 20390 Bottle No.: 0878

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:23S		
Control 1 EC	0.100%	18:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:25S		
Control 2 EC	0.098%	18:25S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:25S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:26S		
Control 3 EC	0.098%	18:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:28S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

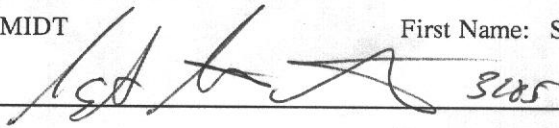

Badge No.: 3205

Date: 03/25/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02989	Calib. Date:	12/09/2021
Certification File No.:	02990	Cert. No.:	00047
Linearity File No.:	02991	Calib. No.:	00037
Solution File No.:	03013	Lin. Date:	12/09/2021
Sequential File No.:	03013	Lin. No.:	00036
		Soln. No.:	00354
		File Date:	02/28/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	20390	Expires:	09/02/2022
		Bottle No.:	1068

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:24S		
Control 1 EC	0.100%	01:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:26S		
Control 2 EC	0.098%	01:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:27S		
Control 3 EC	0.099%	01:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	01:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:29S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3205

Date: 02/28/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02989	Calib. Date: 12/09/2021
Certification File No.:	02990	Calib. No.: 00047
Linearity File No.:	02991	Cert. Date: 12/09/2021
Solution File No.:	03005	Cert. No.: 00037
Sequential File No.:	03005	Lin. Date: 12/09/2021
		Lin. No.: 00036
		Soln. Date: 01/30/2022
		Soln. No.: 00353
		File Date: 01/30/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	20390	Expires: 09/02/2022
		Bottle No.: 0998

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:35S		
Control 1 EC	0.100%	17:36S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	17:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:37S		
Control 2 EC	0.099%	17:37S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:38S		
Control 3 EC	0.100%	17:39S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:40S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3205

Date: 01/30/2022

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02989	Calib. Date: 12/09/2021
Certification File No.:	02990	Cert. No.: 00047
Linearity File No.:	02991	Cert. Date: 12/09/2021
Solution File No.:	03001	Lin. No.: 00037
Sequential File No.:	03001	Lin. Date: 12/09/2021
		Soln. No.: 00036
		Soln. Date: 01/04/2022
		File Date: 01/04/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	20390	Expires: 09/02/2022
		Bottle No.: 1076

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:40S		
Control 1 EC	0.099%	23:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:41S		
Control 2 EC	0.097%	23:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:43S		
Control 3 EC	0.098%	23:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	23:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

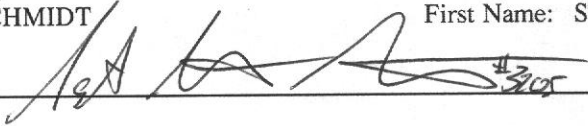

Badge No.: 3205

Date: 01/04/2022