

# Calibrating Unit

## New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C		Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03171	Calib. Date: 01/12/2024
Certification File No.:	03172	Calib. No.: 00052
Linearity File No.:	03173	Cert. Date: 01/12/2024
Solution File No.:	03188	Cert. No.: 00042
Sequential File No.:	03188	Lin. Date: 01/12/2024
		Lin. No.: 00041
		Soln. Date: 03/31/2024
		Soln. No.: 00391
		File Date: 03/31/2024

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	09/12/2025
Solution Control Lot:	23330			Bottle No.:	0603

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:38S		
Control 1 EC	0.097%	10:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39S		
Control 2 EC	0.096%	10:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 3 EC	0.098%	10:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: JESS

First Name: VINCENT

MI: N

Signature: \_\_\_\_\_

*Sgt JESS #3203*

Badge No.: 3203

Date: 03/31/2024

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03171	Calib. Date: 01/12/2024
Certification File No.:	03172	Calib. No.: 00052
Linearity File No.:	03173	Cert. Date: 01/12/2024
Solution File No.:	03184	Cert. No.: 00042
Sequential File No.:	03184	Lin. Date: 01/12/2024
		Lin. No.: 00041
		Soln. Date: 03/20/2024
		Soln. No.: 00390
		File Date: 03/20/2024

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	23330	Expires: 09/12/2025
		Bottle No.: 0638

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:03S		
Control 1 EC	0.099%	22:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:05S		
Control 2 EC	0.098%	22:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:07S		
Control 3 EC	0.099%	22:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	22:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3204

Date: 03/20/2024

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	03171	Calib. Date:	01/12/2024
Certification File No.:	03172	Cert. Date:	01/12/2024
Linearity File No.:	03173	Lin. Date:	01/12/2024
Solution File No.:	03181	Soln. Date:	02/25/2024
Sequential File No.:	03181	File Date:	02/25/2024

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	09/12/2025
Solution Control Lot:	23330			Bottle No.:	0261

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:58S		
Control 1 EC	0.099%	00:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	00:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:59S		
Control 2 EC	0.097%	01:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:01S		
Control 3 EC	0.098%	01:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:03S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

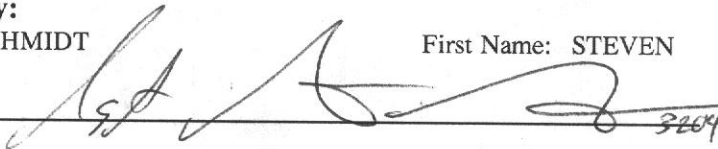

Badge No.: 3204

Date: 02/25/2024

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	03171	Calib. Date:	01/12/2024
Certification File No.:	03172	Cert. No.:	00052
Linearity File No.:	03173	Calib. No.:	00042
Solution File No.:	03179	Cert. Date:	01/12/2024
Sequential File No.:	03179	Lin. Date:	01/12/2024
		Soln. Date:	01/29/2024
		File Date:	01/29/2024
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	23330	Expires:	09/12/2025
		Bottle No.:	0318

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:25S		
Control 1 EC	0.098%	02:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:27S		
Control 2 EC	0.097%	02:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:28S		
Control 3 EC	0.098%	02:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3204

Date: 01/29/2024

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 03137 Calib. Date: 08/01/2023 Calib. No.: 00051  
Certification File No.: 03138 Cert. Date: 08/01/2023 Cert. No.: 00041  
Linearity File No.: 03139 Lin. Date: 08/01/2023 Lin. No.: 00040  
Solution File No.: 03170 Soln. Date: 01/07/2024 Soln. No.: 00386  
Sequential File No.: 03170 File Date: 01/07/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
Control Solution %: 0.100% Expires: 05/09/2024  
Solution Control Lot: 22160 Bottle No.: 0956

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:37S		
Control 1 EC	0.102%	23:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:39S		
Control 2 EC	0.101%	23:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	23:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:40S		
Control 3 EC	0.100%	23:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

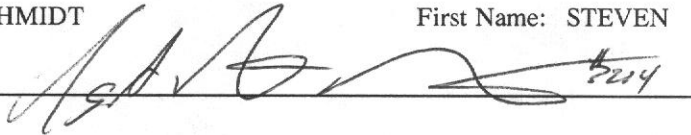

Badge No.: 3204

Date: 01/07/2024