

ALCOTEST CHECKLIST

Municipality: WESTAMPTON

Alcotest Ser. #: ARNK-0025

County: BURLINGTON

Date of Calibration: 10-04-2022

- ☒ 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- ☒ 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDUT 53-0116
- ☒ 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent
Ser. #: DDSF P2-0433
- ☒ 4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 210 216 802
- ☒ 5. **NIST - Traceable Digital Thermometer Readings.**
- ☒ 6.
 - ☒ A. Alcotest 7110 Calibration Record
 - ☒ B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - ☒ C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - ☒ D. **Alcotest Card** of operator/coordinator who performed tests.
 - ☒ E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDXK P2-390
- ☒ 7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
 - ☒ A. 0.04% Solution. 21250
 - ☒ B. 0.08% Solution. 21260
 - ☒ C. 0.10% Solution. 21210
 - ☒ D. 0.16% Solution. 21290
- ☒ 8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - ☒ A. 0.04% used in Calibration/Linearity Testing. DDCB-0001
 - ☒ B. 0.08% used in Calibration/Linearity Testing. DDCB-0002
 - ☒ C. 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.]
 - ☒ D. 0.16% used in Calibration/Linearity Testing. DDBN-0007
- ☒ 9.
 - ☒ A. New Standard Solution Report following Calibration.
 - ☒ B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - ☒ C. Certificate of Analysis 0.10% solution for same.
Lot #: 21360
 - ☒ D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest 7110

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

07/21/2020

ARKK-0035

Dräger, Inc.



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDUS3-D114

Certification Date:

8.3.22

Technician:

MB/JS

Re-Certification Due Date:

8.3.23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDSEF2-0433

Certification Date:

8.3.22

Next Certification Due:

8.3.23

Probe Value:

105

Dräger, Inc.

MB/JS



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-12064518

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 210216802

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Thermistor Module	A27129	01 Mar 2022	1000464885
Temperature Calibration Bath	A46240		
Temperature Calibration Bath	A73332		
Temperature Calibration Bath	B01375		
Temperature Probe	5394	08 Mar 2022	C1228019
Temperature Calibration Bath	B3A444		
Temperature Probe	5357	09 Jun 2021	C0428083
Thermistor Module	B5C344	06 Jun 2021	1000452872
Thermistor Module	B96381	21 Aug 2021	1000457544
Temperature Probe	5392	04 Aug 2021	C0804062
Temperature Probe	5398	04 Aug 2021	C0804051

Certificate Information:

Technician: 420

Procedure: CAL-06

Cal Date: 17 Mar 2021

Cal Due Date: 17 Mar 2023

Test Conditions: 62.18%RH 22.28°C 1006mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.002	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.002	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.002	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		99.999	100.003	Y	99.949	100.049	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement": (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max=As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Marisa Elms

Marisa Elms, Technical Manager

Note:

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be effected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-12064518

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 17 Mar 2021

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 492-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

Alcotest 7110 MKIII-C Calibration NIST-Traceable Digital Thermometer Readings

Coordinator:

Det. Joshua B. Hall
Name

7750
Badge No.

Location:

Westampton Police
Agency

ARNK-0025
Alcotest Serial No.

Equipment:

210 216802
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDCB-0001	10:58 D	11:59 D	33.9°C
0.08%	DDCB-0002	10:58 D	12:00 D	34.0°C
0.10%	DDUJ S3-0116	10:58 D	12:01 D	33.9°C
0.16%	DDBN-0007	10:58 D	12:03 D	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Det. Joshua B. Hall #7750
Coordinator's Signature

10/04/2022
Date

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: WESTAMPTON POLICE
Calibration File No.: 01040
Certification File No.: 01028
Linearity File No.: 01029
Solution File No.: 01039
Sequential File No.: 01040

Calib. Date: 10/04/2022
Cert. Date: 04/20/2022
Lin. Date: 04/20/2022
Soln. Date: 09/28/2022
File Date: 10/04/2022

Serial No.: ARNK-0025

Calib. No.: 00040
Cert. No.: 00034
Lin. No.: 00035
Soln. No.: 00261

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 21210

Model No.: CU-34

Serial No.: DDUJ S3-0116
Expires: 06/16/2023
Bottle No.: 0092

Coordinator

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

7750

Badge No.: 7750

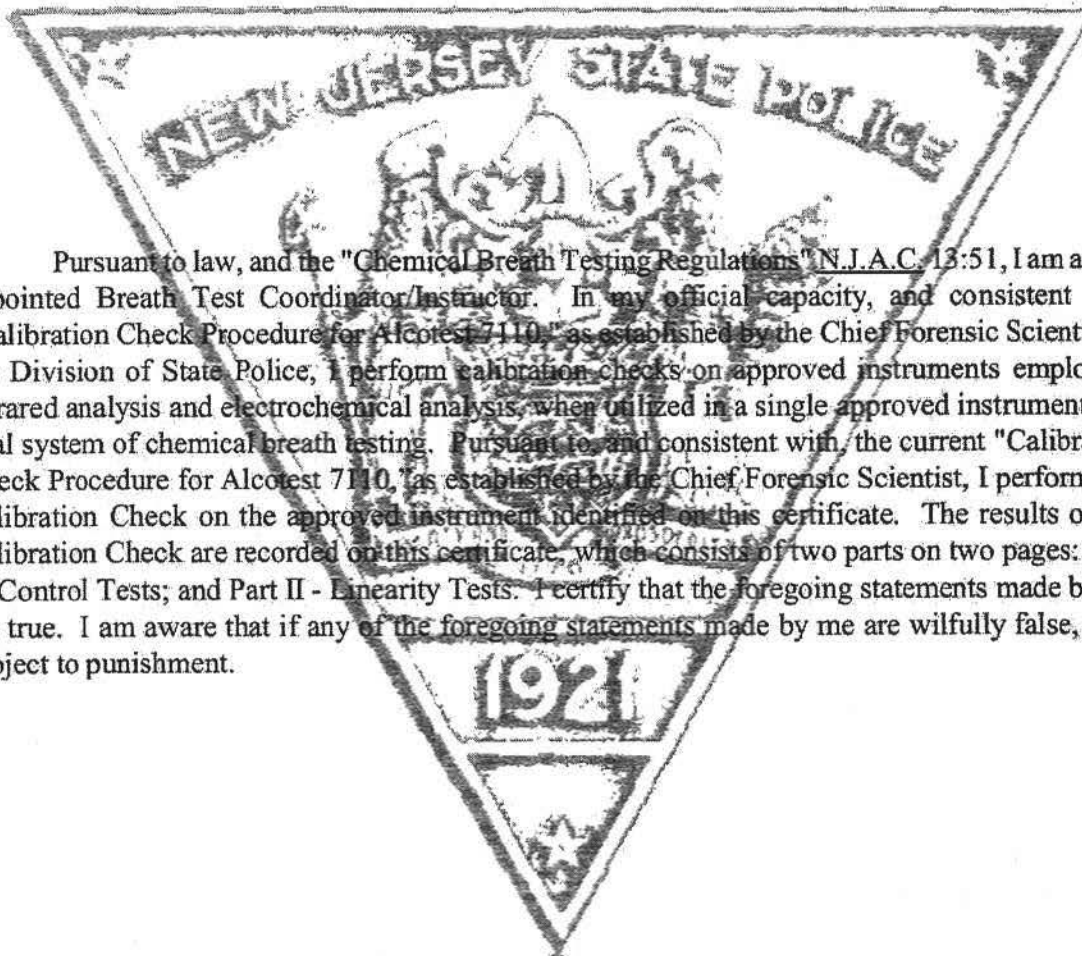
Date: 10/04/2022

*Black Key Temperature Probe Serial.....#

DPXK P2-390 (JBH)

*Digital NIST Temperature Measuring System Serial.....#

210 216 802 (SBW)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: WESTAMPTON POLICE
Calibration File No.: 01040
Certification File No.: 01041
Linearity File No.: 01029
Solution File No.: 01039
Sequential File No.: 01041

Serial No.: ARNK-0025

Calib. Date: 10/04/2022
Cert. Date: 10/04/2022
Lin. Date: 04/20/2022
Soln. Date: 09/28/2022
File Date: 10/04/2022

Calib. No.: 00040
Cert. No.: 00035
Lin. No.: 00035
Soln. No.: 00261

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 21210

Model No.: CU-34

Serial No.: DDUJ S3-0116
Expires: 06/16/2023
Bottle No.: 0092

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:15D		
Control 1 EC	0.100%	12:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16D		
Control 2 EC	0.099%	12:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:17D		
Control 3 EC	0.099%	12:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19D		


All tests within acceptable tolerance.

Coordinator

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 10/04/2022

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	01040	Calib. Date: 10/04/2022
Certification File No.:	01041	Cert. No.: 00040
Linearity File No.:	01042	Cert. No.: 00035
Solution File No.:	01039	Lin. Date: 10/04/2022
Sequential File No.:	01042	Lin. No.: 00036
		Soln. No.: 00261
		File Date: 10/04/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.040%	Serial No.: DDCB-0001
Solution Control Lot:	21250	Expires: 07/06/2023
		Bottle No.: 0487
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.080%	Serial No.: DDCB-0002
Solution Control Lot:	21260	Expires: 07/19/2023
		Bottle No.: 1144
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.160%	Serial No.: DDBN-0007
Solution Control Lot:	21290	Expires: 07/29/2023
		Bottle No.: 0132

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:32D		
Control 1 EC	0.041%	12:33D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	12:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		
Control 2 EC	0.040%	12:35D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	12:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:36D		
Control 3 EC	0.080%	12:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	12:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:38D		
Control 4 EC	0.080%	12:39D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.079%	12:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:40D		
Control 5 EC	0.160%	12:41D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	12:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:42D		
Control 6 EC	0.160%	12:43D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.159%	12:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:44D		


All tests within acceptable tolerance.

Coordinator

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 10/04/2022

DEPARTMENT OF
Traffic and Public Safety
 This is to certify that
Joshua B. Hall
 Breath Test Coordinator/Instructor
 is qualified and competent to conduct chemical breath analyses pursuant to Chapter 142 of
 the laws of the State of New Jersey, as amended, and to administer the
 Alcotest 7110 MKIII-C
 breath testing device at New Jersey State Police, New Jersey, on the 20th day of March
 TWO THOUSAND ONE TWENTY TWO
 [Signature] [Signature]
 COLONEL ATTORNEY GENERAL
 NEW JERSEY STATE POLICE STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2318 (Rev. 12/22)

DEPARTMENT OF
Traffic and Public Safety
 This is to certify that
Joshua B. Hall
 New Jersey State Police
 is qualified and competent to conduct chemical breath analyses pursuant to Chapter 142 of
 the laws of the State of New Jersey, as amended, and to administer the
 Alcotest 7110 MKIII-C
 breath testing device at New Jersey State Police, New Jersey, on the 21st day of December
 TWO THOUSAND ONE SEVENTEEN
 [Signature] [Signature]
 COLONEL ATTORNEY GENERAL
 NEW JERSEY STATE POLICE STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 8/22/19	NYSP Gallaway	[Signature]
2. 1/12/21	ACCC	[Signature]
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2318 (Rev. 12/17)



NEW JERSEY STATE POLICE
Alcohol Drug Testing Unit

Tpr. II Joshua B. Hall #7750

Hamilton Technology Complex
Suite #400
1200 Negron Drive
Hamilton, NJ 08691

Tel#:(609)584-5051 ext 5608
Email:Joshua.Hall@njsp.org
Cell# (609) 947-3179



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 06, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
 Michael Kennedy
 Assistant Chief Forensic Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.
[Signature]
 Notary

KAREN E. STAHL
 NOTARY PUBLIC OF NEW JERSEY
 Commission #: 60110522
 My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0970 to 0.0977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.


Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7058
WEST TRENTON, NJ 08646-0058
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 07/07/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21210


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1199 to 0.1215 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 16, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of July, 2021.
[Signature]
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 842-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 08/11/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1945 to 0.1977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 29, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of August, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDCB-0001

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDCB-0002

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDBN-0007

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe: Certification Date: Next Certification Due:

DDXK P2-390

4.1.22

4.1.23

Probe Value:

106

Draeger, Inc.

MB

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	01040	Calib. Date:	10/04/2022
Certification File No.:	01041	Cert. Date:	10/04/2022
Linearity File No.:	01042	Lin. Date:	10/04/2022
Solution File No.:	01043	Soln. Date:	10/04/2022
Sequential File No.:	01043	File Date:	10/04/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0116
Solution Control Lot:	21360	Expires:	09/01/2023
		Bottle No.:	0057

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:57D		
Control 1 EC	0.101%	13:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58D		
Control 2 EC	0.100%	13:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:59D		
Control 3 EC	0.100%	14:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDSF P2-0433 384

Changed By:

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: [Signature]

Badge No.: 7750

Date: 10/04/2022



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION; Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 09/28/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1216 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 1, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29 day of September, 2021.

Notary 

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110822
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

