

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0025  
Location: WESTAMPTON POLICE  
Calibration File No.: 00765 Calib. Date: 11/21/2016 Calib. No.: 00026  
Certification File No.: 00766 Cert. Date: 11/21/2016 Cert. No.: 00022  
Linearity File No.: 00767 Lin. Date: 11/21/2016 Lin. No.: 00023  
Solution File No.: 00769 Soln. Date: 12/13/2016 Soln. No.: 00188  
Sequential File No.: 00769 File Date: 12/13/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116  
Control Solution %: 0.100% Expires: 07/06/2018  
Solution Control Lot: 16150 Bottle No.: 0014

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:50S		
Control 1 EC	0.103%	13:51S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:52S		
Control 2 EC	0.102%	13:52S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53S		
Control 3 EC	0.101%	13:54S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDSF P2 - 0433 MG

**Changed By:**

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt Michelle Adams #6040

Badge No.: 6040

Date: 12/13/2016



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDUJ53-0116

Certification Date

12-01-16

Technician

KAJ

Re-Certification Due Date

12-01-17

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDSF P2-0433

Certification date:

12-01-16

Next Certification due:

12-01-17

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

KAJ

Westampton Twp Police  
12/30/16  
ORI #: NJ0033800 Sta 270

Incident Maintenance

PL1020D2  
Inquiry  
2016-00014118

Call Date/Time . : 11/21/2016 9:30:00 Monday  
Dispatch Date/Time: 11/21/2016 9:30:00  
Arrive Date/Time : 11/21/2016 9:30:00  
Clear Date Time . : 11/21/2016 9:30:00 Disposition: Incident

Location . . : 710 RANCOCAS RD Type: S  
Cross Street : Venue: 27 Westampton

Nature Of Call:  
Caller . . . : ROWBOTTOM,PTL.,,  
Complainant . :  
Incident Type : 1025 P AdmnReport Phone Number: 6092673000  
Report Req'd . : YES Priority . : 5  
Unit 1 # . . : 2751 ID # 1 : ROWBOTTOM,JOSHUA, ID # 2:  
Unit 2 # . . : ID # 3 : ID # 4:  
Area: 2792 2792 Section: 01 27-01 Grid : L8 L8

F3=Exit F7=Prior F8=Next F9=Cases F10=FI'S F11=NCIC Hist F12=Cancel  
F14=Status/Dispos F15=Suspect Vehicles F16=Names F17=Times F18=Radio Log  
F19=Dispatch F20=Plates F22=Additional F23=Case Doc F24=Documents

Incident Supp: 2016-14118

Ptl. Rowbottom #2751

11-21-2016

On November 21, 2016 at approximately 0930 hours, I started a solution change on the Alcotest 7110 MKIII-C located in processing room #2. While the solution was warming to its optimal temperature, a technician from the NJSP arrived to service the Alcotest machine. The technician stated she canceled my solution change and would complete one when she finished.

Nothing further at this time.

JR

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00738	Calib. Date: 05/27/2016
Certification File No.:	00739	Calib. No.: 00025
Linearity File No.:	00740	Cert. Date: 05/27/2016
Solution File No.:	00757	Cert. No.: 00021
Sequential File No.:	00757	Lin. Date: 05/27/2016
		Lin. No.: 00022
		Soln. Date: 10/22/2016
		Soln. No.: 00185
		File Date: 10/22/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0420

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:36D		
Control 1 EC	0.100%	20:37D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:37D		
Control 2 EC	0.100%	20:38D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38D		
Control 3 EC	0.100%	20:39D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LUTZ

First Name: RALPH

MI: C

Signature: \_\_\_\_\_



2732

Badge No.: 2732

Date: 10/22/2016



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00738	Calib. Date: 05/27/2016
Certification File No.:	00739	Calib. No.: 00025
Linearity File No.:	00740	Cert. Date: 05/27/2016
Solution File No.:	00749	Cert. No.: 00021
Sequential File No.:	00749	Lin. Date: 05/27/2016
		Lin. No.: 00022
		Soln. Date: 09/15/2016
		Soln. No.: 00184
		File Date: 09/15/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0030

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:04D		
Control 1 EC	0.099%	13:04D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:05D		
Control 2 EC	0.099%	13:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:06D		
Control 3 EC	0.099%	13:07D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: \_\_\_\_\_

*STEPHEN 2730*

Badge No.: 2730

Date: 09/15/2016

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00738	Calib. Date: 05/27/2016
Certification File No.:	00739	Calib. No.: 00025
Linearity File No.:	00740	Cert. Date: 05/27/2016
Solution File No.:	00747	Cert. No.: 00021
Sequential File No.:	00747	Lin. Date: 05/27/2016
		Lin. No.: 00022
		Soln. Date: 08/15/2016
		Soln. No.: 00183
		File Date: 08/15/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0018

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:03D		
Control 1 EC	0.099%	11:04D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		
Control 2 EC	0.098%	11:05D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05D		
Control 3 EC	0.099%	11:06D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: \_\_\_\_\_

*Li Stephen* 2730

Badge No.: 2730

Date: 08/15/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00715	Calib. Date: 01/07/2016
Certification File No.:	00716	Cert. No.: 00024
Linearity File No.:	00717	Calib. Date: 01/07/2016
Solution File No.:	00736	Cert. No.: 00020
Sequential File No.:	00736	Lin. Date: 01/07/2016
		Lin. No.: 00021
		Soln. Date: 04/09/2016
		Soln. No.: 00181
		File Date: 04/09/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	14J133	Expires: 10/20/2016
		Bottle No.: 1222

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:31D		
Control 1 EC	0.098%	06:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	06:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:32D		
Control 2 EC	0.098%	06:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	06:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:33D		
Control 3 EC	0.098%	06:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

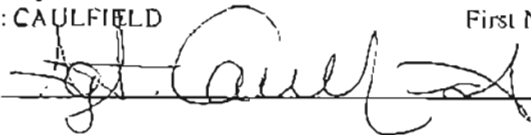
**Changed By:**

Last Name: CAULFIELD

First Name: DARYL

M): B

Signature: \_\_\_\_\_



Badge No.: 2726

Date: 04/09/2016



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00715	Calib. Date:	01/07/2016
Certification File No.:	00716	Cen. Date:	01/07/2016
Linearity File No.:	00717	Lin. Date:	01/07/2016
Solution File No.:	00735	Soln. Date:	04/08/2016
Sequential File No.:	00735	File Date:	04/08/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	15F139	Expires:	06/13/2017
		Bottle No.:	0513

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:38D		
Control 1 EC	0.095%	08:39D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.094%	08:39D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:39D		
Control 2 EC	0.095%	08:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.095%	08:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:41D		
Control 3 EC	0.095%	08:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.095%	08:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:42D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

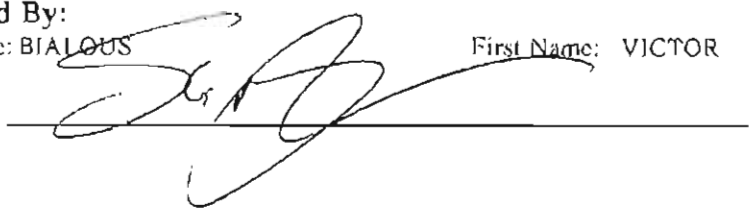
**Changed By:**

Last Name: BIALOUS

First Name: VICTOR

MI: S

Signature: \_\_\_\_\_



Badge No.: 2735

Date: 04/08/2016

Sequential File No.:	00735	File Date:	04/08/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	15F139	Expires:	06/13/2017
		Bottle No.:	0513

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:38D		
Control 1 EC	0.095%	08:39D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.094%	08:39D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	08:39D		
Control 2 EC	0.095%	08:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.095%	08:40D	34.0°C	*** TEST PASSED ***

# Calibrating Unit

## New Standard Solution Report


<b>Equipment</b>	Alcotest 7110 MKII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00715	Calib. Date:	01/07/2016
Certification File No.:	00716	Cert. Date:	01/07/2016
Linearity File No.:	00717	Lin. Date:	01/07/2016
Solution File No.:	00732	Soln. Date:	03/17/2016
Sequential File No.:	00732	File Date:	03/17/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	14J133	Expires:	10/20/2016
		Bottle No.:	1216

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:38S		
Control 1 EC	0.098%	10:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40S		
Control 2 EC	0.098%	10:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 3 EC	0.098%	10:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42S		

All resus within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ENT	First Name: STEPHEN	MI: P
Signature: <u></u>	Badge No.: 2730	Date: 03/17/2016

Sequential File No.:	00732	File Date:	03/17/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	14J133	Expires:	10/20/2016
		Bottle No.:	1216

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:38S		
Control 1 EC	0.098%	10:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40S		
Control 2 EC	0.098%	10:40S	34.0°C	*** TEST PASSED ***

**Equipment** Alcotest 7110 MKII-C Serial No.: ARNK-0025  
 Location: WESTAMPTON POLICE  
 Calibration File No.: 00715 Calib. Date: 01/07/2016 Calib. No.: 00024  
 Certification File No.: 00716 Cert. Date: 01/07/2016 Cert. No.: 00020  
 Linearity File No.: 00717 Lin. Date: 01/07/2016 Lin. No.: 00021  
 Solution File No.: 00731 Soln. Date: 03/04/2016 Soln. No.: 00178  
 Sequential File No.: 00731 File Date: 03/04/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: JDUJ S3-0117  
 Control Solution %: 0.100% Expires: 06/13/2017  
 Solution Control Lot: 15P139 Bottle No.: 0517

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:34S		
Control 1 EC	0.095%	13:35S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	13:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:35S		
Control 2 EC	0.095%	13:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.095%	13:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:37S		
Control 3 EC	0.095%	13:38S	33.9°C	CONTROL TEST FAILED
Control 3 IR	0.094%	13:38S	33.9°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	13:38S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: 

Badge No.: 2730

Date: 03/04/2016

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:34S		
Control 1 EC	0.095%	13:35S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	13:35S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:35S		

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00715	Calib. Date:	01/07/2016
Certification File No.:	00716	Cert. Date:	01/07/2016
Linearity File No.:	00717	Lin. Date:	01/07/2016
Solution File No.:	00729	Soln. Date:	02/29/2016
Sequential File No.:	00729	File Date:	02/29/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	16A150	Expires:	01/05/2017
		Bottle No.:	0510

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:36S		
Control 1 EC	0.099%	12:36S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37S		
Control 2 EC	0.099%	12:38S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:38S		
Control 3 EC	0.099%	12:39S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:39S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:40S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ROWBOTTOM

First Name: PTL

MI: J

Signature: 

Badge No.: 2751

Date: 02/29/2016

Sequential File No.:	00729	File Date:	02/29/2016	Serial No.:	DDUJ S3-0117
Calibrating Unit:	WET	Model No.:	CU-34	Expires:	01/05/2017
Control Solution %:	0.100%			Bottle No.:	0510
Solution Control Lot:	16A150				

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:36S		
Control 1 EC	0.099%	12:36S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37S		
Control 2 EC	0.099%	12:38S	34.0°C	*** TEST PASSED ***

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKJJ-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00715	Calib. Date: 01/07/2016
Certification File No.:	00716	Cert. No.: 00024
Linearity File No.:	00717	Calib. No.: 00020
Solution File No.:	00727	Lin. Date: 01/07/2016
Sequential File No.:	00727	Lin. No.: 00021
		Soln. Date: 02/18/2016
		Soln. No.: 00176
		File Date: 02/18/2016

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	16A150	Expires: 01/05/2017
		Bottle No.: 0511

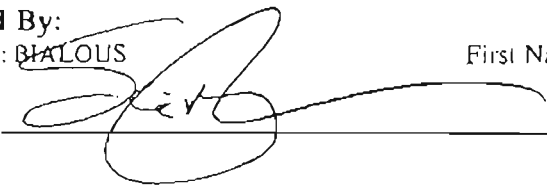
Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:46S		
Control 1 EC	0.100%	08:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47S		
Control 2 EC	0.098%	08:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:48S		
Control 3 EC	0.099%	08:49S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50S		

All tests within acceptable tolerance.

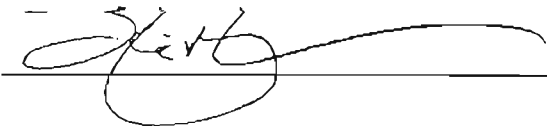
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

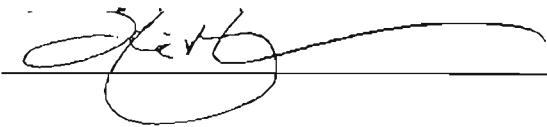
Last Name: **BIALOUS** First Name: **V** MI: **S**

Signature: 

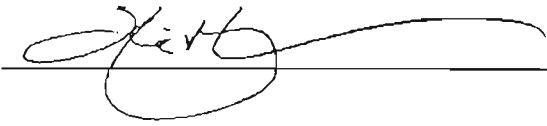
Badge No.: 2735  
Date: 02/18/2016

Signature: 


Badge No.: 2735  
Date: 02/18/2016

Signature: 

Badge No.: 2735  
Date: 02/18/2016

Signature: 

Badge No.: 2735  
Date: 02/18/2016

Signature: 

Badge No.: 2735  
Date: 02/18/2016

# Calibrating Unit

## New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00715	Calib. Date:	01/07/2016
Certification File No.:	00716	Cert. Date:	01/07/2016
Linearity File No.:	00717	Lin. Date:	01/07/2016
Solution File No.:	00723	Soln. Date:	02/07/2016
Sequential File No.:	00723	File Date:	02/07/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	JSF139	Expires:	06/13/2017
		Brute No.:	0511

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:05S		
Control 1 EC	0.096%	08:06S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	08:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07S		
Control 2 EC	0.095%	08:07S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.095%	08:07S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08S		
Control 3 EC	0.095%	08:09S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	08:09S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

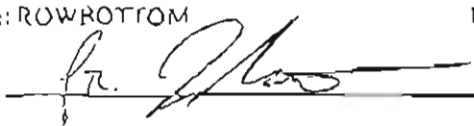
**Changed By:**

Last Name: ROWROTROM

First Name: PTL

MJ:J

Signature: \_\_\_\_\_



Badge No.: 2751

Date: 02/07/2016

Sequential File No.:	00723	File Date:	02/07/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	JSF139	Expires:	06/13/2017
		Brute No.:	0511

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:05S		
Control 1 EC	0.096%	08:06S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	08:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07S		
Control 2 EC	0.095%	08:07S	33.9°C	*** TEST PASSED ***



# Calibrating Unit

## New Standard Solution Report

Equipment	Alcoless 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00715	Calib Date: 01/07/2016
Certification File No.:	00716	Calib. No.: 00024
Linearity File No.:	00717	Cen. Date: 01/07/2016
Solution File No.:	00720	Cen. No.: 00020
Sequential File No.:	00720	Lin. Date: 01/07/2016
		Lin. No.: 00021
		Soln. Date: 02/05/2016
		Soln. No.: 00174
		File Date: 02/05/2016

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	JSF339	Expires: 06/13/2017
		Bottle No.: 0523

Function	Result	Time	Temperature	Comments
	%DAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:38S		
Control 1 EC	0.098%	02:39S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	02:39S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:39S		
Control 2 EC	0.097%	02:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	02:40S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:41S		
Control 3 EC	0.097%	02:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	02:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:42S		

All tests within acceptable tolerance.


On this date I installed the above indicated "NEW SOLUTION" in accordance with Alcoless 7110 operator training and procedures established by the (N/SP) Chief Forensic Scientist.

Changed By:

Last Name: EINSTEIN

First Name: ANDREW

MI: M

Signature: 

Badge No.: 2756

Date: 02/05/2016