

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00786	Calib. Date: 05/10/2017
Certification File No.:	00787	Calib. No.: 00027
Linearity File No.:	00788	Cert. Date: 05/10/2017
Solution File No.:	00799	Cert. No.: 00023
Sequential File No.:	00799	Lin. Date: 05/10/2017
		Lin. No.: 00024
		Soln. Date: 08/16/2017
		Soln. No.: 00197
		File Date: 08/16/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	17110	Expires: 03/20/2019
		Bottle No.: 0739

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:40D		
Control 1 EC	0.103%	13:40D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41D		
Control 2 EC	0.102%	13:42D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:42D		
Control 3 EC	0.102%	13:43D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	13:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:44D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CAULFIELD

First Name: DARYL

MI: B

Signature: _____



Badge No.: 2726

Date: 08/16/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00786	Calib. Date: 05/10/2017
Certification File No.:	00787	Calib. No.: 00027
Linearity File No.:	00788	Cert. Date: 05/10/2017
Solution File No.:	00797	Cert. No.: 00023
Sequential File No.:	00797	Lin. Date: 05/10/2017
		Lin. No.: 00024
		Soln. Date: 07/14/2017
		Soln. No.: 00196
		File Date: 07/14/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	17110	Expires: 03/20/2019
		Bottle No.: 0455

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:54D		
Control 1 EC	0.103%	21:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	21:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:55D		
Control 2 EC	0.103%	21:56D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	21:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:57D		
Control 3 EC	0.103%	21:57D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:58D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CAULFIELD

First Name: DARYL

MI: B

Signature: _____

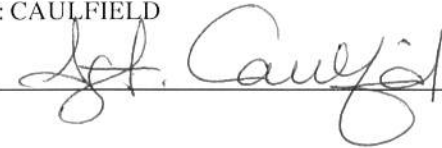

Badge No.: 2726

Date: 07/14/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00786	Calib. Date: 05/10/2017
Certification File No.:	00787	Calib. No.: 00027
Linearity File No.:	00788	Cert. Date: 05/10/2017
Solution File No.:	00791	Cert. No.: 00023
Sequential File No.:	00791	Lin. Date: 05/10/2017
		Lin. No.: 00024
		Soln. Date: 06/07/2017
		Soln. No.: 00195
		File Date: 06/07/2017

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUJ S3-0116
Control Solution %:	0.100%		Expires: 09/17/2018
Solution Control Lot:	201609A		Bottle No.: 1422

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:28D		
Control 1 EC	0.103%	22:29D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	22:29D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:30D		
Control 2 EC	0.103%	22:30D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	22:30D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:31D		
Control 3 EC	0.103%	22:32D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.104%	22:32D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LUTZ

First Name: RALPH

MI: -

Signature: _____

S. J. D. 2732

Badge No.: 2732

Date: 06/07/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00765	Calib. Date: 11/21/2016
Certification File No.:	00766	Calib. No.: 00026
Linearity File No.:	00767	Cert. Date: 11/21/2016
Solution File No.:	00782	Cert. No.: 00022
Sequential File No.:	00782	Lin. Date: 11/21/2016
		Lin. No.: 00023
		Soln. Date: 04/21/2017
		Soln. No.: 00193
		File Date: 04/21/2017

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUJ S3-0116
Control Solution %:	0.100%		Expires: 07/06/2018
Solution Control Lot:	16150		Bottle No.: 0094

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:43D		
Control 1 EC	0.101%	16:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	16:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:44D		
Control 2 EC	0.101%	16:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:46D		
Control 3 EC	0.101%	16:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CAULFIELD

First Name: DARYL

MI: B

Signature: _____

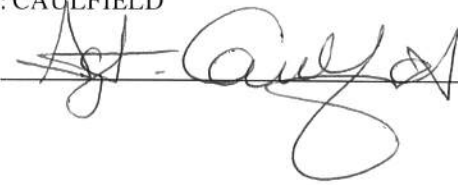

Badge No.: 2726

Date: 04/21/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00765	Calib. Date: 11/21/2016
Certification File No.:	00766	Calib. No.: 00026
Linearity File No.:	00767	Cert. Date: 11/21/2016
Solution File No.:	00778	Cert. No.: 00022
Sequential File No.:	00778	Lin. Date: 11/21/2016
		Lin. No.: 00023
		Soln. Date: 03/20/2017
		Soln. No.: 00192
		File Date: 03/20/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0031

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:14S		
Control 1 EC	0.101%	01:14S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15S		
Control 2 EC	0.101%	01:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	01:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:17S		
Control 3 EC	0.101%	01:17S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ROWBOTTOM

First Name: PTL.

MI: J

Signature: _____



Badge No.: 2751

Date: 03/20/2017

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00765 Calib. Date: 11/21/2016 Calib. No.: 00026
Certification File No.: 00766 Cert. Date: 11/21/2016 Cert. No.: 00022
Linearity File No.: 00767 Lin. Date: 11/21/2016 Lin. No.: 00023
Solution File No.: 00776 Soln. Date: 02/17/2017 Soln. No.: 00191
Sequential File No.: 00776 File Date: 02/17/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 07/06/2018
Solution Control Lot: 16150 Bottle No.: 0021

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:55S		
Control 1 EC	0.101%	02:56S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:57S		
Control 2 EC	0.100%	02:57S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:58S		
Control 3 EC	0.101%	02:59S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	02:59S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LUTZ

First Name: RALPH

MI: --

Signature: _____



Badge No.: 2732

Date: 02/17/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00765	Calib. Date: 11/21/2016
Certification File No.:	00766	Calib. No.: 00026
Linearity File No.:	00767	Cert. Date: 11/21/2016
Solution File No.:	00774	Cert. No.: 00022
Sequential File No.:	00774	Lin. Date: 11/21/2016
		Lin. No.: 00023
		Soln. Date: 01/18/2017
		Soln. No.: 00190
		File Date: 01/18/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0010

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:00S		
Control 1 EC	0.101%	16:01S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:02S		
Control 2 EC	0.101%	16:02S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:02S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:03S		
Control 3 EC	0.101%	16:04S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BIALOUS

First Name: VICTOR

MI: S

Signature: _____

Badge No.: 2735

Date: 01/18/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00765	Calib. Date: 11/21/2016
Certification File No.:	00766	Calib. No.: 00026
Linearity File No.:	00767	Cert. Date: 11/21/2016
Solution File No.:	00773	Cert. No.: 00022
Sequential File No.:	00773	Lin. Date: 11/21/2016
		Lin. No.: 00023
		Soln. Date: 01/14/2017
		Soln. No.: 00189
		File Date: 01/14/2017

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUJ S3-0116
Control Solution %:	0.100%		Expires: 07/06/2018
Solution Control Lot:	16150		Bottle No.: 0039

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:23S		
Control 1 EC	0.102%	03:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:24S		
Control 2 EC	0.101%	03:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	03:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:26S		
Control 3 EC	0.101%	03:26S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	03:26S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CAULFIELD

First Name: DARYL

MI: B

Signature: _____

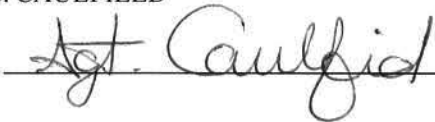

Badge No.: 2726

Date: 01/14/2017