

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00492 Calib. Date: 11/15/2012 Calib. No.: 00016
Certification File No.: 00493 Cert. Date: 11/15/2012 Cert. No.: 00013
Linearity File No.: 00494 Lin. Date: 11/15/2012 Lin. No.: 00014
Solution File No.: 00502 Soln. Date: 12/14/2012 Soln. No.: 00124
Sequential File No.: 00502 File Date: 12/14/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 01/20/2013
Solution Control Lot: 11A085 Bottle No.: 0803

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:15S		
Control 1 EC	0.100%	03:16S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:17S		
Control 2 EC	0.098%	03:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:18S		
Control 3 EC	0.098%	03:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 12/14/2012

Calibrating Unit

New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00492	Calib. Date: 11/15/2012
Certification File No.:	00493	Calib. No.: 00016
Linearity File No.:	00494	Cert. Date: 11/15/2012
Solution File No.:	00501	Cert. No.: 00013
Sequential File No.:	00501	Lin. Date: 11/15/2012
		Lin. No.: 00014
		Soln. Date: 12/13/2012
		Soln. No.: 00123
		File Date: 12/13/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0811

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:36S		
Control 1 EC	-.---%	22:37S	21.0°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	22:37S	21.0°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT	First Name: STEPHEN	MI: P
Signature: 		Badge No.: 2730
		Date: 12/13/2012

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00471 Calib. Date: 06/05/2012 Calib. No.: 00015
Certification File No.: 00472 Cert. Date: 06/05/2012 Cert. No.: 00012
Linearity File No.: 00473 Lin. Date: 06/05/2012 Lin. No.: 00013
Solution File No.: 00491 Soln. Date: 11/07/2012 Soln. No.: 00121
Sequential File No.: 00491 File Date: 11/07/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 01/20/2013
Solution Control Lot: 11A085 Bottle No.: 0813

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:20S		
Control 1 EC	0.100%	08:21S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:21S		
Control 2 EC	0.100%	08:22S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:23S		
Control 3 EC	0.099%	08:24S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:24S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 11/07/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00471	Calib. Date: 06/05/2012
Certification File No.:	00472	Calib. No.: 00015
Linearity File No.:	00473	Cert. Date: 06/05/2012
Solution File No.:	00489	Cert. No.: 00012
Sequential File No.:	00489	Lin. Date: 06/05/2012
		Lin. No.: 00013
		Soln. Date: 10/06/2012
		Soln. No.: 00120
		File Date: 10/06/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0825

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:30D		
Control 1 EC	0.098%	19:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:31D		
Control 2 EC	0.097%	19:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:32D		
Control 3 EC	0.098%	19:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 10/06/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00471 Calib. Date: 06/05/2012 Calib. No.: 00015
Certification File No.: 00472 Cert. Date: 06/05/2012 Cert. No.: 00012
Linearity File No.: 00473 Lin. Date: 06/05/2012 Lin. No.: 00013
Solution File No.: 00488 Soln. Date: 10/05/2012 Soln. No.: 00119
Sequential File No.: 00488 File Date: 10/05/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 01/20/2013
Solution Control Lot: 11A085 Bottle No.: 0806

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:27D		
Control 1 EC	-.---%	21:27D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	21:27D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: 

Badge No.: 2730

Date: 10/05/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00471	Calib. Date:	06/05/2012
Certification File No.:	00472	Cert. No.:	00015
Linearity File No.:	00473	Cert. Date:	06/05/2012
Solution File No.:	00485	Lin. No.:	00012
Sequential File No.:	00485	Lin. Date:	06/05/2012
		Soln. No.:	00118
		Soln. Date:	08/31/2012
		File Date:	08/31/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	11A085	Expires:	01/20/2013
		Bottle No.:	0818

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:55D		
Control 1 EC	0.100%	14:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:56D		
Control 2 EC	0.099%	14:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57D		
Control 3 EC	0.098%	14:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 08/31/2012

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00471 Calib. Date: 06/05/2012 Calib. No.: 00015
Certification File No.: 00472 Cert. Date: 06/05/2012 Cert. No.: 00012
Linearity File No.: 00473 Lin. Date: 06/05/2012 Lin. No.: 00013
Solution File No.: 00483 Soln. Date: 08/02/2012 Soln. No.: 00117
Sequential File No.: 00483 File Date: 08/02/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 01/20/2013
Solution Control Lot: 11A085 Bottle No.: 0815

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:03D		
Control 1 EC	0.098%	20:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:05D		
Control 2 EC	0.097%	20:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	20:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:06D		
Control 3 EC	0.097%	20:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 08/02/2012

Calibrating Unit New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00471	Calib. Date: 06/05/2012
Certification File No.:	00472	Calib. No.: 00015
Linearity File No.:	00473	Cert. Date: 06/05/2012
Solution File No.:	00482	Cert. No.: 00012
Sequential File No.:	00482	Lin. Date: 06/05/2012
		Lin. No.: 00013
		Soln. Date: 08/02/2012
		Soln. No.: 00116
		File Date: 08/02/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0819

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:46D		
Control 1 EC	-.---%	05:46D	22.8°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	05:46D	22.8°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:---		
Control 2 EC	-.---%	--:---	N/A	
Control 2 IR	-.---%	--:---	N/A	
Ambient Air Blank	-.---%	--:---		
Control 3 EC	-.---%	--:---	N/A	
Control 3 IR	-.---%	--:---	N/A	
Ambient Air Blank	-.---%	--:---		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT	First Name: STEPHEN	MI: P
Signature: 		Badge No.: 2730
		Date: 08/02/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00440	Calib. Date: 12/13/2011
Certification File No.:	00441	Calib. No.: 00014
Linearity File No.:	00442	Cert. Date: 12/13/2011
Solution File No.:	00470	Cert. No.: 00011
Sequential File No.:	00470	Lin. Date: 12/13/2011
		Lin. No.: 00012
		Soln. Date: 06/01/2012
		Soln. No.: 00113
		File Date: 06/01/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0804

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:58D		
Control 1 EC	0.099%	20:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:59D		
Control 2 EC	0.098%	21:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	21:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:01D		
Control 3 EC	0.098%	21:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 06/01/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00440 Calib. Date: 12/13/2011 Calib. No.: 00014
Certification File No.: 00441 Cert. Date: 12/13/2011 Cert. No.: 00011
Linearity File No.: 00442 Lin. Date: 12/13/2011 Lin. No.: 00012
Solution File No.: 00463 Soln. Date: 05/05/2012 Soln. No.: 00112
Sequential File No.: 00463 File Date: 05/05/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 01/20/2013
Solution Control Lot: 11A085 Bottle No.: 0810

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:32D		
Control 1 EC	0.100%	08:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:34D		
Control 2 EC	0.098%	08:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:35D		
Control 3 EC	0.098%	08:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:
Last Name: ENT First Name: STEPHEN MI: P
Signature: Sgt. Stephen Badge No.: 2730
Date: 05/05/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00440	Calib. Date: 12/13/2011
Certification File No.:	00441	Calib. No.: 00014
Linearity File No.:	00442	Cert. Date: 12/13/2011
Solution File No.:	00457	Cert. No.: 00011
Sequential File No.:	00457	Lin. Date: 12/13/2011
		Lin. No.: 00012
		Soln. Date: 04/19/2012
		Soln. No.: 00111
		File Date: 04/19/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0817

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:24D		
Control 1 EC	0.099%	15:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:25D		
Control 2 EC	0.097%	15:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:27D		
Control 3 EC	0.097%	15:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 04/19/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00440	Calib. Date: 12/13/2011
Certification File No.:	00441	Calib. No.: 00014
Linearity File No.:	00442	Cert. Date: 12/13/2011
Solution File No.:	00455	Cert. No.: 00011
Sequential File No.:	00455	Lin. Date: 12/13/2011
		Lin. No.: 00012
		Soln. Date: 03/21/2012
		Soln. No.: 00110
		File Date: 03/21/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	11A085	Expires: 01/20/2013
		Bottle No.: 0812

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:58S	10:58D	
Control 1 EC	0.098%	09:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	09:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00S		
Control 2 EC	0.097%	10:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:01S		
Control 3 EC	0.097%	10:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02S	11:02D mps	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DENA P2-116 (MPA)

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature: Tr. A Michael P. Gibson #6353

Badge No.: 6353

Date: 03/21/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00440	Calib. Date:	12/13/2011
Certification File No.:	00441	Cert. Date:	12/13/2011
Linearity File No.:	00442	Lin. Date:	12/13/2011
Solution File No.:	00454	Soln. Date:	03/19/2012
Sequential File No.:	00454	File Date:	03/19/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0116
Solution Control Lot:	11A085	Expires:	01/20/2013
		Bottle No.:	0805

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:32S		
Control 1 EC	0.102%	06:33S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	06:33S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:34S		
Control 2 EC	0.100%	06:35S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	06:35S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:35S		
Control 3 EC	0.100%	06:36S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:36S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:37S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____

Sgt. Stupac

Badge No.: ENT

Date: 03/19/2012

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWA P2-116

Certification date:

3/16/12

Next Certification due:


3/16/13

Probe Value

103

Dräger Safety Diagnostics, Inc.
Technical Service Department

DM



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDUJS3-0117

Certification Date

3/16/12

Technician

DM

Re-Certification Due Date

3/16/13

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00440 Calib. Date: 12/13/2011 Calib. No.: 00014
Certification File No.: 00441 Cert. Date: 12/13/2011 Cert. No.: 00011
Linearity File No.: 00442 Lin. Date: 12/13/2011 Lin. No.: 00012
Solution File No.: 00452 Soln. Date: 02/15/2012 Soln. No.: 00108
Sequential File No.: 00452 File Date: 02/15/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 01/20/2013
Solution Control Lot: 11A085 Bottle No.: 0807

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:14S		
Control 1 EC	0.101%	15:15S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:15S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:16S		
Control 2 EC	0.100%	15:16S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:16S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 3 EC	0.100%	15:18S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:18S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 02/15/2012

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00440 Calib. Date: 12/13/2011 Calib. No.: 00014
Certification File No.: 00441 Cert. Date: 12/13/2011 Cert. No.: 00011
Linearity File No.: 00442 Lin. Date: 12/13/2011 Lin. No.: 00012
Solution File No.: 00447 Soln. Date: 01/14/2012 Soln. No.: 00106
Sequential File No.: 00447 File Date: 01/14/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 03/12/2012
Solution Control Lot: 10C077 Bottle No.: 1400

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:35S		
Control 1 EC	0.101%	10:35S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:35S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		
Control 2 EC	0.098%	10:37S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:37S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		
Control 3 EC	0.099%	10:38S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:38S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: PRINCIOTTA

First Name: WILLIAM

MI: J

Signature: _____

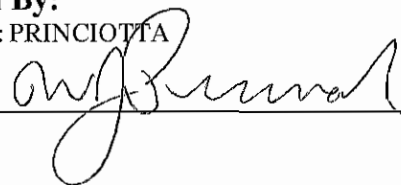

Badge No.: 2729

Date: 01/14/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00414	Calib. Date: 06/28/2011
Certification File No.:	00415	Calib. No.: 00013
Linearity File No.:	00416	Cert. Date: 06/28/2011
Solution File No.:	00438	Cert. No.: 00010
Sequential File No.:	00438	Lin. Date: 06/28/2011
		Lin. No.: 00011
		Soln. Date: 11/15/2011
		Soln. No.: 00104
		File Date: 11/15/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0363

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:00S		
Control 1 EC	0.101%	16:01S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	16:01S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:02S		
Control 2 EC	0.100%	16:02S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:02S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:03S		
Control 3 EC	0.100%	16:04S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:04S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 11/15/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00414	Calib. Date:	06/28/2011
Certification File No.:	00415	Cert. Date:	06/28/2011
Linearity File No.:	00416	Lin. Date:	06/28/2011
Solution File No.:	00431	Soln. Date:	10/14/2011
Sequential File No.:	00431	File Date:	10/14/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0116
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0351

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:20D		
Control 1 EC	0.101%	23:21D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	23:21D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:22D		
Control 2 EC	0.100%	23:22D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	23:22D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:23D		
Control 3 EC	0.100%	23:24D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	23:24D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LANDELL

First Name: PHILIP

MI: M

Signature: _____



Badge No.: 421

Date: 10/14/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00414	Calib. Date: 06/28/2011
Certification File No.:	00415	Calib. No.: 00013
Linearity File No.:	00416	Cert. Date: 06/28/2011
Solution File No.:	00425	Cert. No.: 00010
Sequential File No.:	00425	Lin. Date: 06/28/2011
		Lin. No.: 00011
		Soln. Date: 09/23/2011
		Soln. No.: 00102
		File Date: 09/23/2011

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0356

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:17D		
Control 1 EC	0.100%	13:18D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:18D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19D		
Control 2 EC	0.100%	13:19D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:19D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		
Control 3 EC	0.099%	13:21D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:21D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 09/23/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00414 Calib. Date: 06/28/2011 Calib. No.: 00013
Certification File No.: 00415 Cert. Date: 06/28/2011 Cert. No.: 00010
Linearity File No.: 00416 Lin. Date: 06/28/2011 Lin. No.: 00011
Solution File No.: 00422 Soln. Date: 08/26/2011 Soln. No.: 00101
Sequential File No.: 00422 File Date: 08/26/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0366

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:10D		
Control 1 EC	0.101%	09:11D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:11D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		
Control 2 EC	0.100%	09:12D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:12D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13D		
Control 3 EC	0.100%	09:13D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:13D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 08/26/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00414 Calib. Date: 06/28/2011 Calib. No.: 00013
Certification File No.: 00415 Cert. Date: 06/28/2011 Cert. No.: 00010
Linearity File No.: 00416 Lin. Date: 06/28/2011 Lin. No.: 00011
Solution File No.: 00421 Soln. Date: 07/29/2011 Soln. No.: 00100
Sequential File No.: 00421 File Date: 07/29/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0361

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:51D		
Control 1 EC	0.100%	15:52D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:52D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:53D		
Control 2 EC	0.100%	15:53D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:53D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:54D		
Control 3 EC	0.100%	15:55D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:55D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 07/29/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00392 Calib. Date: 01/03/2011 Calib. No.: 00012
Certification File No.: 00393 Cert. Date: 01/03/2011 Cert. No.: 00009
Linearity File No.: 00394 Lin. Date: 01/03/2011 Lin. No.: 00010
Solution File No.: 00412 Soln. Date: 06/19/2011 Soln. No.: 00098
Sequential File No.: 00412 File Date: 06/19/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0369

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:50D		
Control 1 EC	0.099%	03:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	03:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:51D		
Control 2 EC	0.098%	03:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:53D		
Control 3 EC	0.098%	03:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	03:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 06/19/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00392	Calib. Date:	01/03/2011
Certification File No.:	00393	Cert. Date:	01/03/2011
Linearity File No.:	00394	Lin. Date:	01/03/2011
Solution File No.:	00410	Soln. Date:	05/23/2011
Sequential File No.:	00410	File Date:	05/23/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0116
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0368

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:04D		
Control 1 EC	0.100%	15:05D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:05D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:05D		
Control 2 EC	0.099%	15:06D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:06D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:07D		
Control 3 EC	0.099%	15:07D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:07D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDSFP2 - 0433₀₀

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH


MI: S

Signature: _____

Tpr I [Signature] # 6027

Badge No.: 6027

Date: 05/23/2011



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDUJS3-0116

Certification Date

4-25-11

Technician

MM

Re-Certification Due Date

4-25-12

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDSEF2-0433

Certification date:

4-25-11

Next Certification due:

4-25-12

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

MM

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00392	Calib. Date:	01/03/2011
Certification File No.:	00393	Cert. No.:	00012
Linearity File No.:	00394	Cert. Date:	01/03/2011
Solution File No.:	00408	Lin. No.:	00010
Sequential File No.:	00408	Soln. Date:	05/09/2011
		Soln. No.:	00096
		File Date:	05/09/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0374

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:49D		
Control 1 EC	0.101%	12:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:51D		
Control 2 EC	0.100%	12:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:52D		
Control 3 EC	0.100%	12:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:54D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LANDELL

First Name: PHILIP

MI: M

Signature: 

Badge No.: 421

Date: 05/09/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00392 Calib. Date: 01/03/2011 Calib. No.: 00012
Certification File No.: 00393 Cert. Date: 01/03/2011 Cert. No.: 00009
Linearity File No.: 00394 Lin. Date: 01/03/2011 Lin. No.: 00010
Solution File No.: 00407 Soln. Date: 05/02/2011 Soln. No.: 00095
Sequential File No.: 00407 File Date: 05/02/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 370 Bottle No.: 1400

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:07D		
Control 1 EC	0.100%	22:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:09D		
Control 2 EC	0.099%	22:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:10D		
Control 3 EC	0.099%	22:11D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:12D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 05/02/2011



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 2/11/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11A085

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1201 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 20, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 15th day of February, 2011.

Handwritten signature of Linda L. Desantis
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00392	Calib. Date: 01/03/2011
Certification File No.:	00393	Calib. No.: 00012
Linearity File No.:	00394	Cert. Date: 01/03/2011
Solution File No.:	00405	Cert. No.: 00009
Sequential File No.:	00405	Lin. Date: 01/03/2011
		Lin. No.: 00010
		Soln. Date: 04/05/2011
		Soln. No.: 00094
		File Date: 04/05/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0375

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:47D		
Control 1 EC	0.100%	08:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49D		
Control 2 EC	0.098%	08:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50D		
Control 3 EC	0.099%	08:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 04/05/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00392	Calib. Date: 01/03/2011
Certification File No.:	00393	Calib. No.: 00012
Linearity File No.:	00394	Cert. Date: 01/03/2011
Solution File No.:	00402	Cert. No.: 00009
Sequential File No.:	00402	Lin. Date: 01/03/2011
		Lin. No.: 00010
		Soln. Date: 03/03/2011
		Soln. No.: 00093
		File Date: 03/03/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0355

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:52S		
Control 1 EC	0.100%	20:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:54S		
Control 2 EC	0.099%	20:54S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:55S		
Control 3 EC	0.099%	20:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 03/03/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00392	Calib. Date:	01/03/2011
Certification File No.:	00393	Cert. No.:	00012
Linearity File No.:	00394	Cert. Date:	01/03/2011
Solution File No.:	00399	Lin. Date:	01/03/2011
Sequential File No.:	00399	Soln. Date:	02/02/2011
		File Date:	02/02/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0364

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:34S		
Control 1 EC	0.102%	19:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:35S		
Control 2 EC	0.099%	19:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:37S		
Control 3 EC	0.099%	19:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	19:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 02/02/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00392	Calib. Date:	01/03/2011
Certification File No.:	00393	Cert. Date:	01/03/2011
Linearity File No.:	00394	Lin. Date:	01/03/2011
Solution File No.:	00399	Soln. Date:	02/02/2011
Sequential File No.:	00399	File Date:	02/02/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	10C077	Expires:	03/10/2012
		Bottle No.:	0364

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:34S		
Control 1 EC	0.102%	19:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:35S		
Control 2 EC	0.099%	19:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:37S		
Control 3 EC	0.099%	19:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	19:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 02/02/2011

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00392	Calib. Date:	01/03/2011
Certification File No.:	00393	Cert. Date:	01/03/2011
Linearity File No.:	00394	Lin. Date:	01/03/2011
Solution File No.:	00396	Soln. Date:	01/06/2011
Sequential File No.:	00396	File Date:	01/06/2011

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUJ S3-0117
Control Solution %:	0.100%			Expires:	03/10/2012
Solution Control Lot:	10C077			Bottle No.:	0359

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:21S		
Control 1 EC	0.102%	00:21S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	00:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:22S		
Control 2 EC	0.099%	00:23S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:23S		
Control 3 EC	0.101%	00:24S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:25S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: 

Badge No.: 2730

Date: 01/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00392	Calib. Date: 01/03/2011
Certification File No.:	00393	Calib. No.: 00012
Linearity File No.:	00394	Cert. Date: 01/03/2011
Solution File No.:	00395	Cert. No.: 00009
Sequential File No.:	00395	Lin. Date: 01/03/2011
		Lin. No.: 00010
		Soln. Date: 01/03/2011
		Soln. No.: 00090
		File Date: 01/03/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0117
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 0354

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:13S		
Control 1 EC	0.101%	12:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15S		
Control 2 EC	0.099%	12:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16S		
Control 3 EC	0.099%	12:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWAP2-116,000

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: _____

Tr. II J. Dellanoce # 6027

Badge No.: 6027

Date: 01/03/2011

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00356	Calib. Date:	07/08/2010
Certification File No.:	00357	Cert. No.:	00011
Linearity File No.:	00358	Cert. Date:	07/08/2010
Solution File No.:	00389	Lin. No.:	00008
Sequential File No.:	00389	Lin. Date:	07/08/2010
		Soln. No.:	00009
		Soln. Date:	12/08/2010
		File Date:	12/08/2010

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUJ S3-0117
Control Solution %:	0.100%			Expires:	03/10/2012
Solution Control Lot:	360			Bottle No.:	1400

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:05S		
Control 1 EC	0.103%	17:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	17:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07S		
Control 2 EC	0.101%	17:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	17:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:08S		
Control 3 EC	0.101%	17:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	17:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

M1: P

Signature: _____



Badge No.: 2730

Date: 12/08/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00356	Calib. Date: 07/08/2010
Certification File No.:	00357	Calib. No.: 00011
Linearity File No.:	00358	Cert. Date: 07/08/2010
Solution File No.:	00383	Cert. No.: 00008
Sequential File No.:	00383	Lin. Date: 07/08/2010
		Lin. No.: 00009
		Soln. Date: 11/10/2010
		Soln. No.: 00088
		File Date: 11/10/2010

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUJ S3-0117
Control Solution %:	0.100%		Expires: 03/10/2012
Solution Control Lot:	10C077		Bottle No.: 0365

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:46S		
Control 1 EC	0.101%	21:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	21:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:48S		
Control 2 EC	0.099%	21:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:49S		
Control 3 EC	0.100%	21:50S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 11/10/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00356	Calib. Date:	07/08/2010
Certification File No.:	00357	Cert. Date:	07/08/2010
Linearity File No.:	00358	Lin. Date:	07/08/2010
Solution File No.:	00379	Soln. Date:	10/13/2010
Sequential File No.:	00379	File Date:	10/13/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	08L061	Expires:	12/01/2010
		Bottle No.:	1147

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:14D		
Control 1 EC	0.101%	20:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:15D		
Control 2 EC	0.100%	20:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:16D		
Control 3 EC	0.100%	20:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 10/13/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE	Calib. Date:	07/08/2010
Calibration File No.:	00356	Calib. No.:	00011
Certification File No.:	00357	Cert. Date:	07/08/2010
Linearity File No.:	00358	Lin. Date:	07/08/2010
Solution File No.:	00378	Soln. Date:	09/14/2010
Sequential File No.:	00378	File Date:	09/14/2010

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUJ S3-0117
Control Solution %:	0.100%			Expires:	12/01/2010
Solution Control Lot:	08L061			Bottle No.:	1150

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:47D		
Control 1 EC	0.101%	09:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48D		
Control 2 EC	0.099%	09:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49D		
Control 3 EC	0.100%	09:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: PRINCIOTTA

First Name: WILLIAM

MI: J

Signature: _____

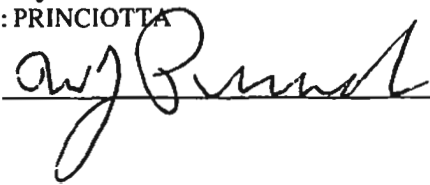

Badge No.: 424

Date: 09/14/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00356 Calib. Date: 07/08/2010 Calib. No.: 00011
Certification File No.: 00357 Cert. Date: 07/08/2010 Cert. No.: 00008
Linearity File No.: 00358 Lin. Date: 07/08/2010 Lin. No.: 00009
Solution File No.: 00373 Soln. Date: 08/27/2010 Soln. No.: 00085
Sequential File No.: 00373 File Date: 08/27/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117
Control Solution %: 0.100% Expires: 12/01/2010
Solution Control Lot: 08L061 Bottle No.: 1136

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:38D		
Control 1 EC	0.098%	16:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:40D		
Control 2 EC	0.097%	16:41D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:41D		
Control 3 EC	0.097%	16:42D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: 

Badge No.: 2730

Date: 08/27/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00356	Calib. Date:	07/08/2010
Certification File No.:	00357	Cert. Date:	07/08/2010
Linearity File No.:	00358	Lin. Date:	07/08/2010
Solution File No.:	00363	Soln. Date:	08/09/2010
Sequential File No.:	00363	File Date:	08/09/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	08L061	Expires:	12/01/2010
		Bottle No.:	1141

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:16D		
Control 1 EC	0.099%	08:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:17D		
Control 2 EC	0.099%	08:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19D		
Control 3 EC	0.099%	08:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: Sgt. Stephen ENT

Badge No.: 2730

Date: 08/09/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00321	Calib. Date: 01/26/2010
Certification File No.:	00322	Calib. No.: 00010
Linearity File No.:	00323	Cert. Date: 01/26/2010
Solution File No.:	00352	Cert. No.: 00007
Sequential File No.:	00352	Lin. Date: 01/26/2010
		Lin. No.: 00008
		Soln. Date: 06/20/2010
		Soln. No.: 00082
		File Date: 06/20/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	08L061	Expires: 12/01/2010
		Bottle No.: 1144

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:03D		
Control 1 EC	0.099%	03:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:04D		
Control 2 EC	0.099%	03:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:06D		
Control 3 EC	0.099%	03:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 06/20/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00321 Calib. Date: 01/26/2010 Calib. No.: 00010
Certification File No.: 00322 Cert. Date: 01/26/2010 Cert. No.: 00007
Linearity File No.: 00323 Lin. Date: 01/26/2010 Lin. No.: 00008
Solution File No.: 00345 Soln. Date: 05/21/2010 Soln. No.: 00080
Sequential File No.: 00345 File Date: 05/21/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0116
Control Solution %: 0.100% Expires: 12/10/2010
Solution Control Lot: 08L061 Bottle No.: 1130

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:47D		
Control 1 EC	0.100%	20:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:48D		
Control 2 EC	0.099%	20:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:50D		
Control 3 EC	0.100%	20:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 05/21/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00321	Calib. Date: 01/26/2010
Certification File No.:	00322	Calib. No.: 00010
Linearity File No.:	00323	Cert. Date: 01/26/2010
Solution File No.:	00338	Cert. No.: 00007
Sequential File No.:	00338	Lin. Date: 01/26/2010
		Lin. No.: 00008
		Soln. Date: 04/22/2010
		Soln. No.: 00079
		File Date: 04/22/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	08L061	Expires: 12/10/2010
		Bottle No.: 1142

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:34D		
Control 1 EC	0.101%	04:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:35D		
Control 2 EC	0.099%	04:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:36D		
Control 3 EC	0.100%	04:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 04/22/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00321	Calib. Date:	01/26/2010
Certification File No.:	00322	Cert. Date:	01/26/2010
Linearity File No.:	00323	Lin. Date:	01/26/2010
Solution File No.:	00334	Soln. Date:	03/24/2010
Sequential File No.:	00334	File Date:	03/24/2010

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUJ S3-0116
Control Solution %:	0.100%			Expires:	12/01/2010
Solution Control Lot:	08L061			Bottle No.:	1140

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:39S		
Control 1 EC	0.101%	10:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 2 EC	0.101%	10:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42S		
Control 3 EC	0.100%	10:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: PRINCIOTTA

First Name: WILLIAM

MI: J

Signature: _____



424

Badge No.: 424

Date: 03/24/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00321	Calib. Date: 01/26/2010
Certification File No.:	00322	Calib. No.: 00010
Linearity File No.:	00323	Cert. Date: 01/26/2010
Solution File No.:	00332	Cert. No.: 00007
Sequential File No.:	00332	Lin. Date: 01/26/2010
		Lin. No.: 00008
		Soln. Date: 03/22/2010
		Soln. No.: 00076
		File Date: 03/22/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUJ S3-0116
Solution Control Lot:	08L061	Expires: 12/10/2010
		Bottle No.: 1139

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:43S		
Control 1 EC	-.---%	18:44S	23.4°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	18:44S	23.4°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____

Sgt. Stephen

Badge No.: 2730

Date: 03/22/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0025
Location: WESTAMPTON POLICE
Calibration File No.: 00321 **Calib. Date:** 01/26/2010 **Calib. No.:** 00010
Certification File No.: 00322 **Cert. Date:** 01/26/2010 **Cert. No.:** 00007
Linearity File No.: 00323 **Lin. Date:** 01/26/2010 **Lin. No.:** 00008
Solution File No.: 00325 **Soln. Date:** 02/22/2010 **Soln. No.:** 00075
Sequential File No.: 00325 **File Date:** 02/22/2010

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUJ S3-0116
Control Solution %: 0.100% **Expires:** 12/01/2010
Solution Control Lot: 08L061 **Bottle No.:** 1131

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:09S		
Control 1 EC	0.100%	09:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:10S		
Control 2 EC	0.099%	09:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:12S		
Control 3 EC	0.099%	09:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 02/22/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0025
Location:	WESTAMPTON POLICE	
Calibration File No.:	00291	Calib. Date: 07/30/2009
Certification File No.:	00292	Calib. No.: 00009
Linearity File No.:	00294	Cert. Date: 07/30/2009
Solution File No.:	00316	Cert. No.: 00006
Sequential File No.:	00316	Lin. Date: 07/30/2009
		Lin. No.: 00007
		Soln. Date: 01/05/2010
		Soln. No.: 00073
		File Date: 01/05/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUJ S3-0116
Control Solution %: 0.100%		Expires: 12/01/2010
Solution Control Lot: 08L061		Bottle No.: 1146

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:39S		
Control 1 EC	0.103%	21:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	21:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:40S		
Control 2 EC	0.103%	21:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	21:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:41S		
Control 3 EC	0.102%	21:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: STEPHEN

MI: P

Signature: _____



Badge No.: 2730

Date: 01/05/2010