

ALCOTEST CHECKLIST

Municipality: WILLINGBORO Alcotest Ser. #: ARWC-0060
County: BURLINGTON Date of Calibration: 01-07-2019

- ☒ 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- ☒ 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDWE 53-0189
- ☒ 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDUN P2-293
- ☒ 4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 170 428 363
- ☒ 5. ☒ A. Alcotest 7110 Calibration Record
☒ B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
☒ C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
☒ D. **Alcotest Card** of operator/coordinator who performed tests.
☒ E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDXK P2-390
- ☒ 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
- | | | |
|--|-----------------|--------------|
| <input checked="" type="checkbox"/> A. | 0.04% Solution. | <u>17240</u> |
| <input checked="" type="checkbox"/> B. | 0.08% Solution. | <u>17250</u> |
| <input checked="" type="checkbox"/> C. | 0.10% Solution. | <u>17230</u> |
| <input checked="" type="checkbox"/> D. | 0.16% Solution. | <u>17260</u> |
- ☒ 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
- | | | |
|--|--|------------------|
| <input checked="" type="checkbox"/> A. | 0.04% used in Calibration/Linearity Testing. | <u>DDCB-0001</u> |
| <input checked="" type="checkbox"/> B. | 0.08% used in Calibration/Linearity Testing. | <u>DDCB-0002</u> |
| <input checked="" type="checkbox"/> C. | 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.] | |
| <input checked="" type="checkbox"/> D. | 0.16% used in Calibration/Linearity Testing. | <u>DDBN-0007</u> |
- ☒ 8. ☒ A. New Standard Solution Report following Calibration.
☒ B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
☒ C. Certificate of Analysis 0.10% solution for same.
Lot #: 17360
☒ D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

2-10-14

SERIAL NUMBER:

ARWC-0060

Dräger Safety Diagnostics, Inc.

BC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- ☒ Model: ALCOTEST CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDUES 3-0189

Certification Date:

6-15-18

Technician:

BS

Re-Certification Due Date:

6-15-19

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDUN P2- 293

Certification Date:

6-18-18

Next Certification Due:

6-18-19

Probe Value:

101

Draeger, Inc.

BS



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-8609163

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 170428363 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5267	12/06/17	B6B30059
Temperature Calibration Bath TC-191	A42238		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5202	12/19/17	B6B30058-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Probe	5356	1/10/18	B7104024
Readout, Digital Thermometer	B5C344	3/12/18	B7314035
Temperature Calibration Bath TC-275	B16388		
Thermistor Probe	5357	1/06/18	B7104023
Readout, Digital Thermometer	B5C344	3/12/18	B7314035

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 6/08/17 Due Date: 6/08/19
Test Conditions: 23.5°C 50.0 %RH 1014 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	0.001	Y	-0.048	0.052	0.010	>4:1
°C		N.A.		25.003	25.001	Y	24.953	25.053	0.010	>4:1
°C		N.A.		50.002	50.001	Y	49.952	50.052	0.010	>4:1
°C		N.A.		100.001	100.003	Y	99.951	100.051	0.010	>4:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: WILLINGBORO TWP POLICE
Serial No.: ARWC-0060
Calibration File No.: 00632
Calib. Date: 01/07/2019
Calib. No.: 00037
Certification File No.: 00621
Cert. Date: 07/12/2018
Cert. No.: 00029
Linearity File No.: 00622
Lin. Date: 07/12/2018
Lin. No.: 00029
Solution File No.: 00631
Soln. Date: 12/10/2018
Soln. No.: 00194
Sequential File No.: 00632
File Date: 01/07/2019


Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 17230
Model No.: CU-34
Serial No.: DDWE S3-0189
Expires: 08/07/2019
Bottle No.: 0829

Coordinator

Last Name: GAMBONE
First Name: BRIAN
MI: M
Signature: TPR. I B. M. #7029
Badge No.: 7029
Date: 01/07/2019

*Black Key Temperature Probe Serial.....# DDX KP2-390 (BMG)

*Digital NIST Temperature Measuring System Serial.....# 170428363 (BMG)

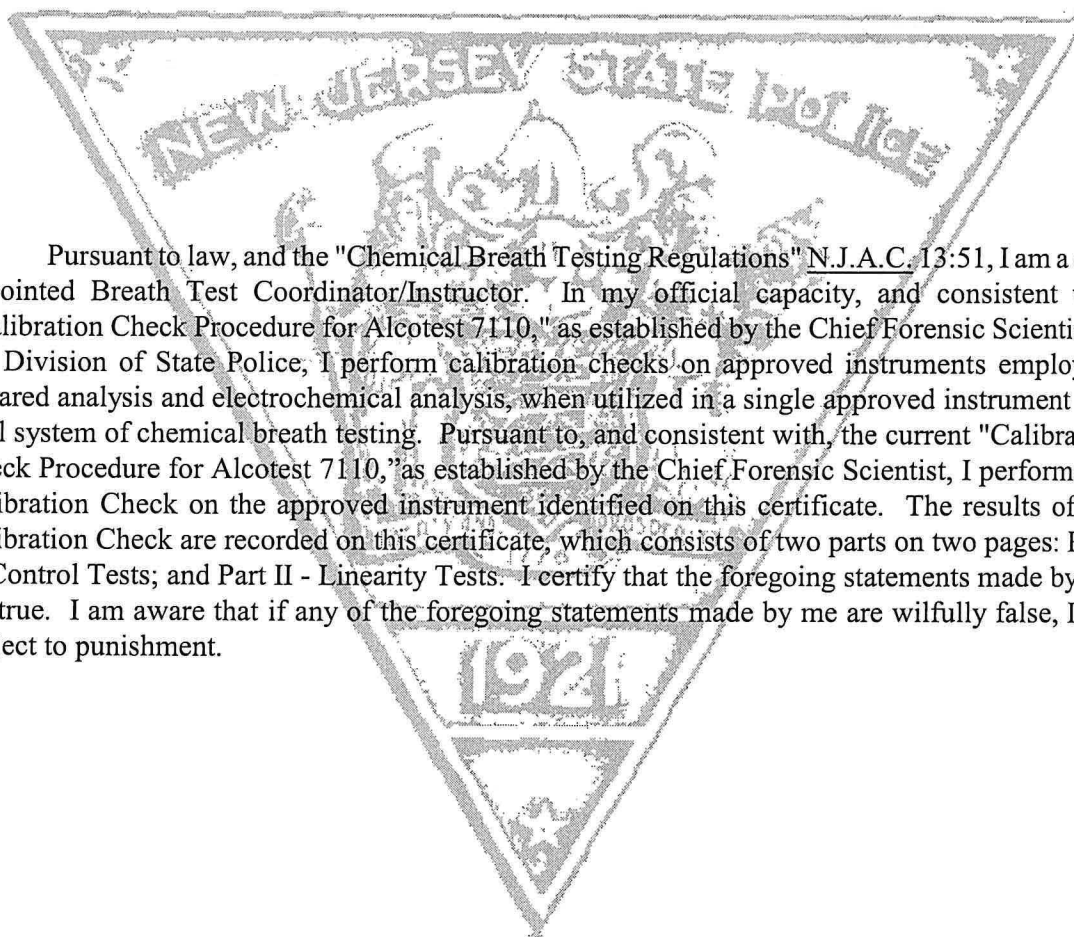

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: WILLINGBORO TWP POLICE
Serial No.: ARWC-0060
Calibration File No.: 00632 Calib. Date: 01/07/2019 Calib. No.: 00037
Certification File No.: 00633 Cert. Date: 01/07/2019 Cert. No.: 00030
Linearity File No.: 00622 Lin. Date: 07/12/2018 Lin. No.: 00029
Solution File No.: 00631 Soln. Date: 12/10/2018 Soln. No.: 00194
Sequential File No.: 00633 File Date: 01/07/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0189
Control Solution %: 0.100% Expires: 08/07/2019
Solution Control Lot: 17230 Bottle No.: 0829

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:50S		
Control 1 EC	0.099%	13:50S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	13:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51S		
Control 2 EC	0.096%	13:52S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:52S		
Control 3 EC	0.097%	13:53S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54S		

All tests within acceptable tolerance.

Coordinator

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature: TPA I B M

Badge No.: 7029

Date: 01/07/2019

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0060
Location:	WILLINGBORO TWP POLICE	
Calibration File No.:	00632	Calib. Date: 01/07/2019
Certification File No.:	00633	Cert. No.: 00037
Linearity File No.:	00634	Cert. Date: 01/07/2019
Solution File No.:	00631	Lin. No.: 00030
Sequential File No.:	00634	Lin. Date: 01/07/2019
		Soln. No.: 00194
		Soln. Date: 12/10/2018
		File Date: 01/07/2019

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDCB-0001
Control Solution %: 0.040%		Expires: 08/10/2019
Solution Control Lot: 17240		Bottle No.: 0741

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDCB-0002
Control Solution %: 0.080%		Expires: 08/15/2019
Solution Control Lot: 17250		Bottle No.: 0812

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDBN-0007
Control Solution %: 0.160%		Expires: 08/21/2019
Solution Control Lot: 17260		Bottle No.: 0508

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:11S		
Control 1 EC	0.042%	14:12S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	14:12S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13S		
Control 2 EC	0.040%	14:14S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.039%	14:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:16S		
Control 3 EC	0.080%	14:16S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	14:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:18S		
Control 4 EC	0.079%	14:19S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	14:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:20S		
Control 5 EC	0.160%	14:21S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.157%	14:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:22S		
Control 6 EC	0.157%	14:23S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.156%	14:23S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:25S		

All tests within acceptable tolerance.

Coordinator

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature:

Brian Gambone # 7029

Badge No.: 7029

Date: 01/07/2019

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Brian M. Gambone
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL TESTS AND IS PERSONNEL TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE BLOOD ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 9th DAY OF October

TWO THOUSAND AND Nineteen

[Signature]
CHIEF
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
11/19/18	GCFA	Adam Stender
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2538 (Rev. 8/1/18)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Brian M. Gambone
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL TESTS AND IS PERSONNEL TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
A METHOD TO DETERMINE BLOOD ALCOHOL
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 15th DAY OF July

TWO THOUSAND AND Tea

[Signature]
CHIEF
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1/8/17	GCFA	Wm Horn
11/4/14	GCFA	Adam Stender
6/4/16	CMFA	Adam Stender
11/19/18	GCFA	Adam Stender
6.		
7.		
8.		
9.		

S.P. 2538 (Rev. 03/16)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS **0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/29/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 10, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30th day of August, 2017.

Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190

NOTARY PUBLIC

STATE OF NEW JERSEY

My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS **0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 09/07/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0963 to 0.0973 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 15, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11 day of September, 2017.

Notary

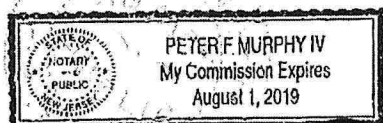

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS **0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/24/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17230


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1216 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 07, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 24 day of August, 2017.

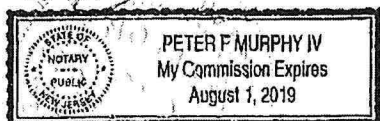Notary

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS 0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/12/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1937 to 0.1957 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 13 day of September, 2017.

Notary

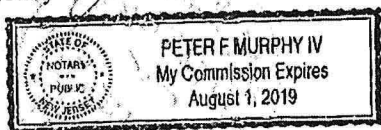

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- ☒ Model: ALCOTEST CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDCB-0001

Certification Date:

8-23-18

Technician:

BS

Re-Certification Due Date:

8-23-19



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- ☒ Model: ALCOTEST CU34
☐ Model: MARK IIA
☐ Other: _____

Serial Number:

DDCB-0002

Certification Date:

8-23-18

Technician:

BS

Re-Certification Due Date:

8-23-19

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ Other: _____

Serial Number:

DDBN-0007

Certification Date:

9-12-18

Technician:

BS

Re-Certification Due Date:

9-12-19

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2-390

Certification Date:

8-23-18

Next Certification Due:

8-23-19

Probe Value:

104

Dräger, Inc.

BS

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWC-0060
Location: WILLINGBORO TWP POLICE
Calibration File No.: 00632 Calib. Date: 01/07/2019 Calib. No.: 00037
Certification File No.: 00633 Cert. Date: 01/07/2019 Cert. No.: 00030
Linearity File No.: 00634 Lin. Date: 01/07/2019 Lin. No.: 00030
Solution File No.: 00635 Soln. Date: 01/07/2019 Soln. No.: 00195
Sequential File No.: 00635 File Date: 01/07/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0189
Control Solution %: 0.100% Expires: 10/17/2019
Solution Control Lot: 17360 Bottle No.: 1125

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:30S		
Control 1 EC	0.099%	15:31S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:32S		
Control 2 EC	0.098%	15:32S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:33S		
Control 3 EC	0.098%	15:34S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUN P2-293 (BMG)

Changed By:

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature: TPR. I Brian A. #7029

Badge No.: 7029

Date: 01/07/2019



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL PATRICK J. CALLAHAN
Acting Superintendent

CERTIFICATION OF ANALYSIS **0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/01/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1197 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 17, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 2nd day of November, 2017.

Mary E. McLaughlin
Notary
MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

