

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00514	Calib. Date:	07/17/2015
Certification File No.:	00515	Cert. No.:	00029
Linearity File No.:	00516	Cert. Date:	07/17/2015
Solution File No.:	00519	Lin. No.:	00022
Sequential File No.:	00519	Soln. Date:	09/23/2015
		Soln. No.:	00141
		File Date:	09/23/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE S3-0189
Solution Control Lot:	15F139	Expires:	06/13/2017
		Bottle No.:	1249

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:17D		
Control 1 EC	0.098%	00:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:18D		
Control 2 EC	0.098%	00:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	00:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:20D		
Control 3 EC	0.097%	00:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	00:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: \_\_\_\_\_



Badge No.: 16187

Date: 09/23/2015

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWC-0060  
**Location:** WILLINGBORO TWP POLICE  
**Calibration File No.:** 00514 **Calib. Date:** 07/17/2015 **Calib. No.:** 00029  
**Certification File No.:** 00515 **Cert. Date:** 07/17/2015 **Cert. No.:** 00022  
**Linearity File No.:** 00516 **Lin. Date:** 07/17/2015 **Lin. No.:** 00022  
**Solution File No.:** 00518 **Soln. Date:** 08/25/2015 **Soln. No.:** 00140  
**Sequential File No.:** 00518 **File Date:** 08/25/2015

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0189  
**Control Solution %:** 0.100% **Expires:** 06/13/2017  
**Solution Control Lot:** 15F139 **Bottle No.:** 1247

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:51D		
Control 1 EC	0.098%	00:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	00:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:53D		
Control 2 EC	0.097%	00:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	00:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:54D		
Control 3 EC	0.098%	00:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	00:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: \_\_\_\_\_

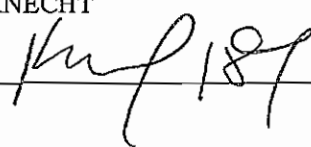

Badge No.: 16187

Date: 08/25/2015

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWC-0060  
 Location: WILLINGBORO TWP POLICE  
 Calibration File No.: 00514 Calib. Date: 07/17/2015 Calib. No.: 00029  
 Certification File No.: 00515 Cert. Date: 07/17/2015 Cert. No.: 00022  
 Linearity File No.: 00516 Lin. Date: 07/17/2015 Lin. No.: 00022  
 Solution File No.: 00517 Soln. Date: 07/17/2015 Soln. No.: 00139  
 Sequential File No.: 00517 File Date: 07/17/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0189  
 Control Solution %: 0.100% Expires: 12/31/2016  
 Solution Control Lot: 14L135 Bottle No.: 0325

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:09D		
Control 1 EC	0.101%	14:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:10D		
Control 2 EC	0.101%	14:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:12D		
Control 3 EC	0.100%	14:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: \_\_\_\_\_

Badge No.: 6040

Date: 07/17/2015

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
<b>Location:</b>	WILLINGBORO TWP POLICE		
<b>Calibration File No.:</b>	00501	<b>Calib. Date:</b>	01/22/2015
<b>Certification File No.:</b>	00502	<b>Cert. No.:</b>	00021
<b>Linearity File No.:</b>	00503	<b>Lin. Date:</b>	01/22/2015
<b>Solution File No.:</b>	00509	<b>Lin. No.:</b>	00021
<b>Sequential File No.:</b>	00509	<b>Soln. Date:</b>	04/25/2015
		<b>Soln. No.:</b>	00137
		<b>File Date:</b>	04/25/2015
<b>Calibrating Unit:</b>	WBT	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDWE S3-0189
<b>Solution Control Lot:</b>	13G115	<b>Expires:</b>	07/18/2015
		<b>Bottle No.:</b>	0326

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:52D		
Control 1 EC	0.098%	04:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:53D		
Control 2 EC	0.098%	04:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:54D		
Control 3 EC	0.099%	04:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: \_\_\_\_\_



Badge No.: 16187

Date: 04/25/2015

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0060
<b>Location:</b>	WILLINGBORO TWP POLICE	
<b>Calibration File No.:</b>	00501	Calib. Date: 01/22/2015
<b>Certification File No.:</b>	00502	Calib. No.: 00028
<b>Linearity File No.:</b>	00503	Cert. Date: 01/22/2015
<b>Solution File No.:</b>	00507	Cert. No.: 00021
<b>Sequential File No.:</b>	00507	Lin. Date: 01/22/2015
		Lin. No.: 00021
		Soln. Date: 03/25/2015
		Soln. No.: 00136
		File Date: 03/25/2015
<b>Calibrating Unit:</b>	WET	Model No.: CU-34
<b>Control Solution %:</b>	0.100%	Serial No.: DDWE S3-0189
<b>Solution Control Lot:</b>	13G115	Expires: 07/18/2015
		Bottle No.: 0329

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:07S		
Control 1 EC	0.099%	04:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:09S		
Control 2 EC	0.099%	04:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:10S		
Control 3 EC	0.100%	04:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSI) Chief Forensic Scientist.

**Changed By:**

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: 

Badge No.: 16187

Date: 03/25/2015

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
<b>Location:</b>	WILLINGBORO TWP POLICE		
<b>Calibration File No.:</b>	00501	<b>Calib. Date:</b>	01/22/2015
<b>Certification File No.:</b>	00502	<b>Cert. Date:</b>	01/22/2015
<b>Linearity File No.:</b>	00503	<b>Lin. Date:</b>	01/22/2015
<b>Solution File No.:</b>	00505	<b>Soln. Date:</b>	02/20/2015
<b>Sequential File No.:</b>	00505	<b>File Date:</b>	02/20/2015
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDWE S3-0189
<b>Solution Control Lot:</b>	13G115	<b>Expires:</b>	07/18/2015
		<b>Bottle No.:</b>	0330

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:44S		
Control 1 EC	0.101%	01:44S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	01:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:45S		
Control 2 EC	0.101%	01:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:47S		
Control 3 EC	0.101%	01:47S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: *Jennifer Knacht* / 187

Badge No.: 16187

Date: 02/20/2015

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC 0060
<b>Location:</b>	WILLINGBORO TWP POLICE		
<b>Calibration File No.:</b>	00488	<b>Calib. Date:</b>	07/31/2014
<b>Certification File No.:</b>	00489	<b>Cert. No.:</b>	00027
<b>Linearity File No.:</b>	00490	<b>Cert. Date:</b>	07/31/2014
<b>Solution File No.:</b>	00500	<b>Lin. Date:</b>	07/31/2014
<b>Sequential File No.:</b>	00500	<b>Lin. No.:</b>	00020
		<b>Soln. Date:</b>	01/13/2015
		<b>Soln. No.:</b>	00131
		<b>File Date:</b>	01/13/2015
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDWE S3-0189
<b>Solution Control Lot:</b>	13G115	<b>Expires:</b>	07/18/2015
		<b>Batch No.:</b>	0336

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:18S		
Control 1 EC	0.103%	03:19S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	03:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:20S		
Control 2 EC	0.103%	03:20S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	03:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:21S		
Control 3 EC	0.102%	03:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	03:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: \_\_\_\_\_



Badge No.: 16187

Date: 01/13/2015