

## ALCOTEST 9510 PARAMETER REPORT

### Equipment

Serial No.: ARMJ-0201  
Firmware: 8326739 1.5  
WinCE application: 8326738 2.9  
Configuration: 8326737 3.10

Date: 03/24/2025  
Time: 07:40:37

### Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

**ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)**  
**Longport Borough**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0201  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Wet Adjust Record**

Wet Adjust File No.: 34 Wet Adjust Date: 03/24/2025 Wet Adjust No.: 2  
Wet Adjust Time: 08:32:28

Concentration: 0.100 %  
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARND-0006 Adj. Unit Exp.: 10/03/2025  
Solution Lot No.: 23230 Soln. Bottle No.: 1262 Adjust Soln. Exp.: 06/26/2025

Preadjust Simulator Temp.: 34.00 degree C  
Postadjust Simulator Temp.: 34.00 degree C

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Widener - First Name: William MI: F Badge No.: 7817

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TPR.1 Wm. Widener 7817*

Signed: Date: 03/24/2025 ID: 22

**ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)**  
**Longport Borough**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0201  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Dry Adjust Record**

Dry Adjust File No.: 35 Dry Adjust Date: 03/24/2025 Dry Adjust No.: 2  
Dry Adjust Time: 08:49:53

Concentration: 0.100 %  
Dry Gas Lot No.: 302-402448282 Adjust Gas Exp.: 05/20/2025  
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001273 Barom. Cert. Exp.: 10/18/2025  
Pre-adjust Amb. Pressure: 1012 hPa Post-adjust Amb. Pressure: 1012 hPa

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Widener - First Name: William MI: F Badge No.: 7817

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TPR. J. Wm. Widener 7817*

Signed:

Date: 03/24/2025

ID: 22

**ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)**  
**Longport Borough**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0201  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Linearity Record**

Linearity File No.: 36 Lin. Date: 03/24/2025 Lin. No.: 2

0.040% Dry Gas Lot No.: 302-402755169 Adjust. Gas Exp.: 05/25/2026  
0.080% Dry Gas Lot No.: 302-402477282 Adjust. Gas Exp.: 06/24/2025  
0.160% Dry Gas Lot No.: 302-402486005 Adjust. Gas Exp.: 07/13/2025  
0.300% Dry Gas Lot No.: 302-402759888 Adjust. Gas Exp.: 05/31/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	09:00:42		*TEST PASSED*
Control .04 Test 1 EC	0.038	09:01:18	1011	*TEST PASSED*
Control .04 Test 1 IR	0.039	09:01:18	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:02:23		*TEST PASSED*
Control .04 Test 2 EC	0.039	09:02:36	1011	*TEST PASSED*
Control .04 Test 2 IR	0.040	09:02:36	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:10:33		*TEST PASSED*
Control .08 Test 3 EC	0.078	09:11:08	1011	*TEST PASSED*
Control .08 Test 3 IR	0.079	09:11:08	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:12:18		*TEST PASSED*
Control .08 Test 4 EC	0.080	09:12:30	1011	*TEST PASSED*
Control .08 Test 4 IR	0.080	09:12:30	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:30:20		*TEST PASSED*
Control .16 Test 5 EC	0.155	09:30:55	1011	*TEST PASSED*
Control .16 Test 5 IR	0.158	09:30:55	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:32:09		*TEST PASSED*
Control .16 Test 6 EC	0.157	09:32:21	1011	*TEST PASSED*
Control .16 Test 6 IR	0.159	09:32:21	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:39:28		*TEST PASSED*
Control .30 Test 7 EC	0.296	09:40:07	1011	*TEST PASSED*
Control .30 Test 7 IR	0.303	09:40:07	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:41:31		*TEST PASSED*
Control .30 Test 8 EC	0.302	09:41:47	1011	*TEST PASSED*
Control .30 Test 8 IR	0.306	09:41:47	1011	*TEST PASSED*
Ambient Air Blank	0.000	09:42:23		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Widener - First Name: William MI: F Badge No.: 7817

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

TPR. | Wm Widener 7817

Signed:

Date: 03/24/2025

ID: 22

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1**  
**Longport Borough**  
**SERIAL NUMBER: ARMJ-0201**

**Equipment**

Inst. Model No.: ALCOTEST 9510    Serial No.: ARMJ-0201  
Firmware: 8326739 1.5    Config.: 8326737 3.10    WinCE: 8326738 2.9  
Cyl1 Install File No.: 28    Cyl1 Install Date: 11/20/2024    Cyl1 Install No.: 1

**Control Tests (0.100%)**

Installation Inlet: #1 (Upper)    Post test active Cyl.: #1 (Upper)  
Dry Gas Lot No.: 302-402921458    Dry Gas Lot Exp.: 12/18/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	11:09:46		*TEST PASSED*
Control Test 1			1009	*TEST PASSED*
EC Result	0.098	11:10:33		*TEST PASSED*
IR Result	0.100	11:10:33		*TEST PASSED*
Ambient Air Blank	0.000	11:11:42		*TEST PASSED*
Control Test 2			1008	*TEST PASSED*
EC Result	0.100	11:12:07		*TEST PASSED*
IR Result	0.101	11:12:07		*TEST PASSED*
Ambient Air Blank	0.000	11:13:20		*TEST PASSED*
Control Test 3			1008	*TEST PASSED*
EC Result	0.099	11:13:45		*TEST PASSED*
IR Result	0.101	11:13:45		*TEST PASSED*
Ambient Air Blank	0.000	11:14:16		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Widener -    First Name: William    MI: F    Badge No.: 7817

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TPR.1 WmWidener 7817*

Signed:

Date: 11/20/2024

ID: 22

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2**  
**Longport Borough**  
**SERIAL NUMBER: ARMJ-0201**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0201  
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl2 Install File No.: 29 Cyl2 Install Date: 11/20/2024 Cyl2 Install No.: 1

**Control Tests (0.100%)**

Installation Inlet: #2 (Lower) Post test active Cyl.: #1 (Upper)  
 Dry Gas Lot No.: 302-402997674 Dry Gas Lot Exp.: 03/18/2027

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	11:22:02		*TEST PASSED*
Control Test 1			1008	*TEST PASSED*
EC Result	0.098	11:22:49		*TEST PASSED*
IR Result	0.100	11:22:49		*TEST PASSED*
Ambient Air Blank	0.000	11:24:00		*TEST PASSED*
Control Test 2			1008	*TEST PASSED*
EC Result	0.099	11:24:25		*TEST PASSED*
IR Result	0.101	11:24:25		*TEST PASSED*
Ambient Air Blank	0.000	11:25:37		*TEST PASSED*
Control Test 3			1008	*TEST PASSED*
EC Result	0.099	11:26:01		*TEST PASSED*
IR Result	0.101	11:26:01		*TEST PASSED*
Ambient Air Blank	0.000	11:26:32		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Widener - First Name: William MI: F Badge No.: 7817

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*TPR. 1 Wm Widener 7817*

Signed:

Date: 11/20/2024

ID: 22



# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036  
DRAEGER MEDICAL SYSTEMS INC

Sales order: 1127619703  
Date: February 08, 2024

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402921458  
ETHANOL IN NITROGEN

Product Expiration: December 18, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	263.7	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: December 18, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Algas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251



**Dräger**

**Alcotest 9510**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

2024-10-28

ARMJ-0201

DMSI, \_\_\_\_\_





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 09/12/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of September, 2023.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



**Customer:** DRAEGER INC

7256 S SAM HOUSTON PKWY W

STE 100

HOUSTON, TX 77085

**PO Number:** S1O4303440829



## Certificate/SO Number: 5-F2R00-160-1 Revision 0

**Manufacturer:** Dräger Safety AG & Co. KGaA

**Model Number:** X-Cal 2000

**Description:** Breath Alcohol Simulator

**Serial Number:** ARND-0006

**ID:** NONE

**As-Found:** In Tolerance

**As-Left:** In Tolerance

**Issue Date:** Oct 04, 2024

**Calibration Date:** Oct 03, 2024

**Due Date:** Oct 03, 2025

**Calibrated To:** Customer Specification

**Calibration Procedure:** 1-AC103519-1

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/INCSSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/INCSSL Z540.3-2006 (R2013) are also covered.


Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104303440829

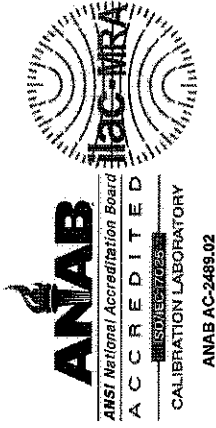

## Certificate/SO Number: 5-F2R00-160-1 Revision 0

### As Found/As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	Cal Process		Measurement Uncertainty (k=2; ±)	Units	TUR
						O	T			
<b>Function Checks</b>										
Bubble Check			P	P	P					
Seal Check			P	P	P					
<b>Temperature Source: Accuracy Test</b>										
Accuracy Test	34.00°C	±(0.02 °C)	33.98	34.02	33.99 °C		1.5e-002	1.6e-002	°C	1.3 : 1
<b>Temperature Source: Stability Test</b>										
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C		5.0e-003	7.6e-003	°C	4.0 : 1

Field not applicable.

### Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
05H1466	Fluke	5628	Secondary Standard PRT	31-Aug-24	31-Aug-25	4500048240	AF/AL
HP927312	Hart Scientific/Fluke	1575	Super Thermometer	10-Jul-24	31-Jan-26	5-S&HP927312-9-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

### Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
70.91°F / 21.62°C	53.30%	DewK8	G	Temperature

### Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone

Customer: DRAEGER INC

7256 S SAM HOUSTON PKWY W

STE 100

HOUSTON, TX 77085


PO Number: S104303440829



**Certificate/SO Number: 5-F2R00-160-1 Revision 0**

are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S104303440829

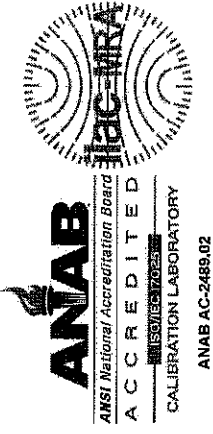

**Certificate/SO Number: 5-F2R00-160-1 Revision 0**

**Legend**

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

Customer: DRAEGER INC  
7296 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S1O4303440829



Certificate/SO Number: 5-F2R00-160-1 Revision 0

Calibrated At:  
16115 Park Row  
Houston, TX 77084

Facility Responsible:  
16115 Park Row  
Houston, TX 77084  
800-828-1470

Unit Barcode:   
09008498612

Date Received: October 01, 2024  
Service Level: R9


Calibrated By:

  
Jose Martinez  
Calibration Technician

Electronically Signed By:

Oct 03, 2024 22:29:20 -04:00

Reviewed By:

  
Josh Soileau  
Lab Manager

Electronically Signed By:

Oct 04, 2024 09:44:59 -04:00

**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S1O4303440829



## Certificate/SO Number: 5-F2R00-340-1 Revision 0

**Manufacturer:** Wika Instr/Mensor Corp/Trend  
**Model Number:** CPG2300  
**Description:** Portable Barometer  
**Serial Number:** 41001273  
**ID:** NONE

**As-Found:** In Tolerance  
**As-Left:** In Tolerance  
**Issue Date:** Oct 18, 2024  
**Calibration Date:** Oct 18, 2024  
**Due Date:** Oct 18, 2025

**Calibrated To:** Manufacturer Specification

**Calibration Procedure:** 1-AC107288-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO /IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements. ISO 9001:2015, ANSI/NCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS:16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/NCSL Z540.3-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor k=2, providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers ( OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

**Notes:**

One or more test points are close to the tolerance limit, however no adjustment was made due to the impact on other test points.



Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104303440829




## Certificate/SO Number: 5-F2R00-340-1 Revision 0

### As Found/As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	O		Cal Process Uncertainty (k=2; ±)	Measurement Uncertainty (k=2; ±)	Units	TUR
						O	T				
<b>Pressure Measure: 552 to 1172 mbara Range</b>											
	550.08mbara	±(0.015% FS)	549.91	550.27	550.20 mbara			1.7e+001	2.0e+001	PPM	19.2 : 1
	610.03mbara	±(0.015% FS)	609.85	610.21	610.10 mbara			1.7e+001	1.9e+001	PPM	17.4 : 1
	680.38mbara	±(0.015% FS)	680.20	680.56	680.50 mbara			1.7e+001	1.9e+001	PPM	15.6 : 1
	734.29mbara	±(0.015% FS)	734.11	734.47	734.40 mbara			1.7e+001	1.9e+001	PPM	14.4 : 1
	804.65mbara	±(0.015% FS)	804.47	804.83	804.70 mbara			1.7e+001	1.8e+001	PPM	13.2 : 1
	864.93mbara	±(0.015% FS)	864.75	865.11	865.00 mbara			1.7e+001	1.8e+001	PPM	12.2 : 1
	924.98mbara	±(0.015% FS)	924.75	925.11	925.10 mbara			1.7e+001	1.8e+001	PPM	11.4 : 1
	985.23mbara	±(0.015% FS)	985.05	985.41	985.30 mbara			1.7e+001	1.8e+001	PPM	10.7 : 1
	1043.9mbara	±(0.015% FS)	1043.7	1044.1	1044.0 mbara			1.7e+001	5.8e+001	PPM	11.3 : 1
	1114.2mbara	±(0.015% FS)	1114.0	1114.4	1114.3 mbara			1.7e+001	5.5e+001	PPM	10.6 : 1
	1174.6mbara	±(0.015% FS)	1174.4	1174.8	1174.7 mbara			1.7e+001	5.2e+001	PPM	10.0 : 1
	924.92mbara	±(0.015% FS)	924.74	925.10	925.00 mbara			1.7e+001	1.8e+001	PPM	11.4 : 1
	864.92mbara	±(0.015% FS)	864.74	865.10	865.10 mbara			1.7e+001	1.9e+001	PPM	12.2 : 1
	804.65mbara	±(0.015% FS)	804.47	804.83	804.80 mbara			1.7e+001	1.8e+001	PPM	13.2 : 1

Field not applicable.

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104303440829

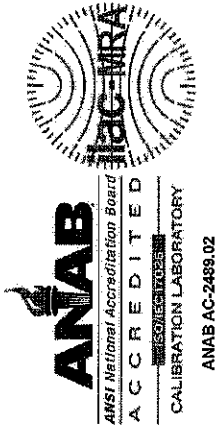

## Certificate/SO Number: 5-F2R00-340-1 Revision 0

### Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
DW11BA	Fluke/DH Instruments	PG7601	Piston Gauge	9-Jul-24	31-Jul-25	5-&DWH1BA-17-1	AF/AL
DW11CA	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	4-Jul-24	31-Oct-24	5-&DWH1CA-33-1	AF/AL
DW11LOW	Fluke/DH Instruments	PC-7100/7600-10-TC	Gas Piston-Cylinder Module	8-Apr-22	30-Apr-27	5-&DWH1LOW-3-1	AF/AL
DW11MASS	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	2-Feb-24	28-Feb-25	5-&DWH1MASS-10-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.


### Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
69.36°F / 20.76°C	43.40%	DewK8	B	GP Pressure

### Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S1O4303440829

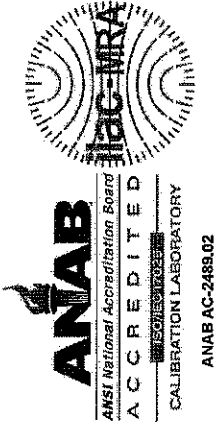


**Certificate/SO Number: 5-F2R00-340-1 Revision 0**

**Legend**

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Seipoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S1O4303440829

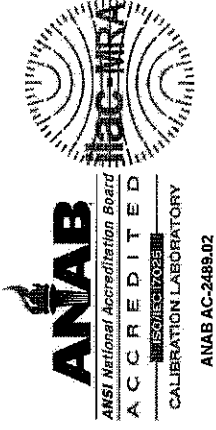


Certificate/SO Number: 5-F2R00-340-1 Revision 0

**Calibrated At:**  
16115 Park Row  
Houston, TX 77084

**Facility Responsible:**  
16115 Park Row  
Houston, TX 77084  
800-828-1470

**Unit Barcode:**  
  
0800B498603

**Date Received:** October 01, 2024  
**Service Level:** R9

**Calibrated By:**  
  
Evan Copeland  
Calibration Technician

Oct 16, 2024  
16:02:22 -04:00

**Reviewed By:**  
  
Daniel Beigits for

Oct 16, 2024  
17:05:43 -04:00

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111663404  
Date: July 05, 2022

**NJSP DEPT OF LAW AND PUBLIC SAFETY**

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402448282  
ETHANOL IN NITROGEN

Product Expiration: May 20, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>	<b>PPM</b>	<b>( BrAC )</b>
ETHANOL	263.3	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 20, 2022

APPROVED BY: \_\_\_\_\_

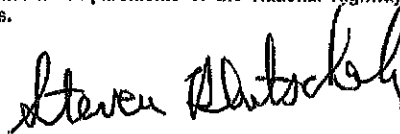

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DRAEGER MEDICAL SYSTEMS INC.;

Sales order: 1121156486

Date: June 12, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402755169  
ETHANOL IN NITROGEN

Product Expiration: May 25, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	104.2PPM	(0.040)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	107.2	(0.041)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 25, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111713599  
Date: July 05, 2022

**NJSP DEPT OF LAW AND PUBLIC SAFETY**

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402477282  
ETHANOL IN NITROGEN

Product Expiration: June 24, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	208.4PPM	(0.080)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>	<b>PPM</b>	<b>( BrAC )</b>
ETHANOL	212.2	(0.081)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: June 24, 2022

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1111788955

Date: July 14, 2022

NJSP

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402486005  
ETHANOL IN NITROGEN

Product Expiration: July 13, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	416.8PPM	(0.160)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	420.0	(0.161)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 263192, dated 6th January 2022 or calibration test 292029, 292030 or 292031, dated 26th March 2022 applies

##### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: July 13, 2022

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251



# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401041NJ  
**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1123022087  
 Date: August 18, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
 ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
 CALGAZ LOT#: 302-402759888  
 ETHANOL IN NITROGEN

Product Expiration: May 31, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	781.5PPM	(0.300)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	793.1	(0.304)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.


Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 31, 2023

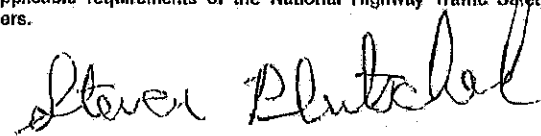APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request"

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**William F. Widener**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE STATUTES 9510 A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF January

TWO THOUSAND AND Twenty Three

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 10/22)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**William F. Widener**  
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE STATUTES 9510 A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 16th DAY OF May

TWO THOUSAND AND Twenty Three

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 10/22)