

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01279	Calib. Date: 08/06/2024
Certification File No.:	01280	Cert. No.: 00053
Linearity File No.:	01281	Cert. Date: 08/06/2024
Solution File No.:	01295	Lin. Date: 08/06/2024
Sequential File No.:	01295	Lin. No.: 00044
		Soln. Date: 12/07/2024
		Soln. No.: 00311
		File Date: 12/07/2024
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	24020	Expires: 01/09/2026
		Bottle No.: 0990

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:52S		
Control 1 EC	0.097%	04:52S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	04:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:53S		
Control 2 EC	0.096%	04:54S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:55S		
Control 3 EC	0.097%	04:55S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 12/07/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01279 Calib. Date: 08/06/2024 Calib. No.: 00053
Certification File No.: 01280 Cert. Date: 08/06/2024 Cert. No.: 00045
Linearity File No.: 01281 Lin. Date: 08/06/2024 Lin. No.: 00044
Solution File No.: 01291 Soln. Date: 11/14/2024 Soln. No.: 00310
Sequential File No.: 01291 File Date: 11/14/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 0838

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:54S		
Control 1 EC	0.096%	01:54S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:55S		
Control 2 EC	0.096%	01:56S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:56S		
Control 3 EC	0.096%	01:57S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	01:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:58S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPOLSKI

First Name: CODY

MI: E

Signature: 

Badge No.: 4066

Date: 11/14/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01279 Calib. Date: 08/06/2024 Calib. No.: 00053
Certification File No.: 01280 Cert. Date: 08/06/2024 Cert. No.: 00045
Linearity File No.: 01281 Lin. Date: 08/06/2024 Lin. No.: 00044
Solution File No.: 01290 Soln. Date: 10/08/2024 Soln. No.: 00309
Sequential File No.: 01290 File Date: 10/08/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 0849

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:59D		
Control 1 EC	0.099%	03:59D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:00D		
Control 2 EC	0.097%	04:01D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:01D		
Control 3 EC	0.098%	04:02D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 10/08/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01279 Calib. Date: 08/06/2024 Calib. No.: 00053
Certification File No.: 01280 Cert. Date: 08/06/2024 Cert. No.: 00045
Linearity File No.: 01281 Lin. Date: 08/06/2024 Lin. No.: 00044
Solution File No.: 01285 Soln. Date: 09/09/2024 Soln. No.: 00308
Sequential File No.: 01285 File Date: 09/09/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 1118

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:24D		
Control 1 EC	0.099%	05:25D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:25D		
Control 2 EC	0.097%	05:26D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:27D		
Control 3 EC	0.098%	05:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TOMPKINS

First Name: NATHAN

MI: A

Signature: 

Badge No.: 4046

Date: 09/09/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01261	Calib. Date: 02/14/2024
Certification File No.:	01262	Calib. No.: 00052
Linearity File No.:	01263	Cert. Date: 02/14/2024
Solution File No.:	01277	Cert. No.: 00044
Sequential File No.:	01277	Lin. Date: 02/14/2024
		Lin. No.: 00043
		Soln. Date: 07/30/2024
		Soln. No.: 00306
		File Date: 07/30/2024
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	24020	Expires: 01/09/2026
		Bottle No.: 1010

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:55D		
Control 1 EC	0.100%	05:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:56D		
Control 2 EC	0.098%	05:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:58D		
Control 3 EC	0.099%	05:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 07/30/2024

Calibrating Unit New Standard Solution Report


Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01279 Calib. Date: 08/06/2024 Calib. No.: 00053
Certification File No.: 01280 Cert. Date: 08/06/2024 Cert. No.: 00045
Linearity File No.: 01281 Lin. Date: 08/06/2024 Lin. No.: 00044
Solution File No.: 01282 Soln. Date: 08/06/2024 Soln. No.: 00307
Sequential File No.: 01282 File Date: 08/06/2024

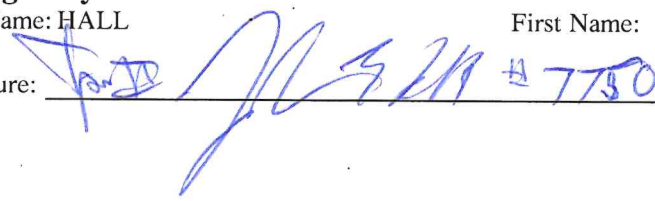
Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 0848

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:49D		
Control 1 EC	0.100%	10:49D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50D		
Control 2 EC	0.098%	10:51D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:51D		
Control 3 EC	0.099%	10:52D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJ P2-293 

Changed By:
Last Name: HALL First Name: JOSHUA MI: B
Signature:  # 7750
Badge No.: 7750
Date: 08/06/2024

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01261	Calib. Date: 02/14/2024
Certification File No.:	01262	Calib. No.: 00052
Linearity File No.:	01263	Cert. Date: 02/14/2024
Solution File No.:	01274	Cert. No.: 00044
Sequential File No.:	01274	Lin. Date: 02/14/2024
		Lin. No.: 00043
		Soln. Date: 07/01/2024
		Soln. No.: 00305
		File Date: 07/01/2024
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	24020	Expires: 01/09/2026
		Bottle No.: 0842

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:23D		
Control 1 EC	0.100%	01:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:24D		
Control 2 EC	0.099%	01:24D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:25D		
Control 3 EC	0.099%	01:26D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:26D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPOLSKI

First Name: CODY

MI: E

Signature: _____

Badge No.: 4066

Date: 07/01/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01261 Calib. Date: 02/14/2024 Calib. No.: 00052
Certification File No.: 01262 Cert. Date: 02/14/2024 Cert. No.: 00044
Linearity File No.: 01263 Lin. Date: 02/14/2024 Lin. No.: 00043
Solution File No.: 01271 Soln. Date: 05/30/2024 Soln. No.: 00304
Sequential File No.: 01271 File Date: 05/30/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 0949

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:55D		
Control 1 EC	0.103%	00:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:57D		
Control 2 EC	0.102%	00:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	00:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:58D		
Control 3 EC	0.102%	00:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPOLSKI

First Name: CODY

MI: E

Signature:



Badge No.: 4066

Date: 05/30/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01261 Calib. Date: 02/14/2024 Calib. No.: 00052
Certification File No.: 01262 Cert. Date: 02/14/2024 Cert. No.: 00044
Linearity File No.: 01263 Lin. Date: 02/14/2024 Lin. No.: 00043
Solution File No.: 01269 Soln. Date: 04/22/2024 Soln. No.: 00303
Sequential File No.: 01269 File Date: 04/22/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 1012

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:22D		
Control 1 EC	0.100%	00:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:23D		
Control 2 EC	0.099%	00:24D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:25D		
Control 3 EC	0.100%	00:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:26D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILK

First Name: JASON

MI: J

Signature: _____



Badge No.: 4049

Date: 04/22/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01261 Calib. Date: 02/14/2024 Calib. No.: 00052
Certification File No.: 01262 Cert. Date: 02/14/2024 Cert. No.: 00044
Linearity File No.: 01263 Lin. Date: 02/14/2024 Lin. No.: 00043
Solution File No.: 01267 Soln. Date: 03/23/2024 Soln. No.: 00302
Sequential File No.: 01267 File Date: 03/23/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 01/09/2026
Solution Control Lot: 24020 Bottle No.: 1160

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:14S		
Control 1 EC	0.100%	00:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:15S		
Control 2 EC	0.099%	00:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:17S		
Control 3 EC	0.099%	00:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

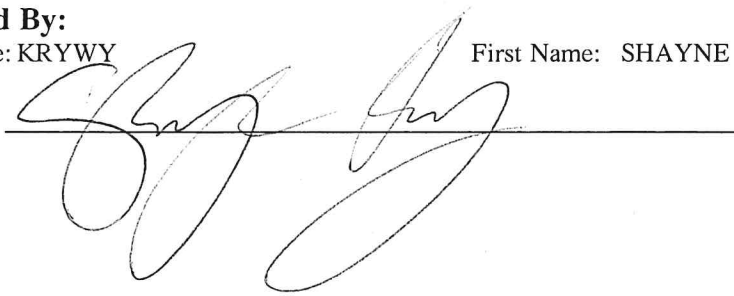
Changed By:

Last Name: KRYWY

First Name: SHAYNE

MI: C

Signature: _____



Badge No.: 4060

Date: 03/23/2024



PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 01/22/2024

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 24020

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1194 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 9, 2026.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 25 day of January, 2024.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01261 Calib. Date: 02/14/2024 Calib. No.: 00052
Certification File No.: 01262 Cert. Date: 02/14/2024 Cert. No.: 00044
Linearity File No.: 01263 Lin. Date: 02/14/2024 Lin. No.: 00043
Solution File No.: 01265 Soln. Date: 02/19/2024 Soln. No.: 00301
Sequential File No.: 01265 File Date: 02/19/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 04/04/2024
Solution Control Lot: 22110 Bottle No.: 1111

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:05S		
Control 1 EC	0.100%	01:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:07S		
Control 2 EC	0.099%	01:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:08S		
Control 3 EC	0.100%	01:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	01:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:10S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPOLSKI

First Name: CODY

MI: E

Signature: 

Badge No.: 4066

Date: 02/19/2024

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C	Serial No.: ARTN-0053	
Location: FLORENCE TOWNSHIP P.D.		
Calibration File No.: 01261	Calib. Date: 02/14/2024	Calib. No.: 00052
Certification File No.: 01262	Cert. Date: 02/14/2024	Cert. No.: 00044
Linearity File No.: 01263	Lin. Date: 02/14/2024	Lin. No.: 00043
Solution File No.: 01264	Soln. Date: 02/14/2024	Soln. No.: 00300
Sequential File No.: 01264	File Date: 02/14/2024	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUM S3-0225
Control Solution %: 0.100%		Expires: 04/04/2024
Solution Control Lot: 22110		Bottle No.: 1446

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:51S		
Control 1 EC	0.102%	10:51S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:52S		
Control 2 EC	0.101%	10:53S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:54S		
Control 3 EC	0.101%	10:54S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:55S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJ P2 - 144 5811

Changed By:

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: _____

[Handwritten Signature] # 7750

Badge No.: 7750

Date: 02/14/2024

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: FLORENCE TOWNSHIP P.D.
Serial No.: ARTN-0053
Calibration File No.: 01246 Calib. Date: 09/26/2023 Calib. No.: 00051
Certification File No.: 01247 Cert. Date: 09/26/2023 Cert. No.: 00043
Linearity File No.: 01248 Lin. Date: 09/26/2023 Lin. No.: 00042
Solution File No.: 01259 Soln. Date: 01/19/2024 Soln. No.: 00299
Sequential File No.: 01259 File Date: 01/19/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 04/04/2024
Solution Control Lot: 22110 Bottle No.: 0826

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:47S		
Control 1 EC	0.100%	04:47S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:47S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:48S		
Control 2 EC	0.098%	04:49S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:50S		
Control 3 EC	0.099%	04:50S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SADAR

First Name: TIMOTHY

MI: J

Signature: _____



Badge No.: 4035

Date: 01/19/2024