

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01316 Calib. Date: 04/30/2025 Calib. No.: 00055
Certification File No.: 01317 Cert. Date: 04/30/2025 Cert. No.: 00047
Linearity File No.: 01318 Lin. Date: 04/30/2025 Lin. No.: 00046
Solution File No.: 01323 Soln. Date: 05/30/2025 Soln. No.: 00317
Sequential File No.: 01323 File Date: 05/30/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 07/23/2026
Solution Control Lot: 24260 Bottle No.: 0098

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:48D		
Control 1 EC	0.100%	06:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:50D		
Control 2 EC	0.100%	06:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:51D		
Control 3 EC	0.099%	06:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	06:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____

Badge No.: 4047

Date: 05/30/2025

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01316 **Calib. Date:** 04/30/2025 **Calib. No.:** 00055
Certification File No.: 01317 **Cert. Date:** 04/30/2025 **Cert. No.:** 00047
Linearity File No.: 01318 **Lin. Date:** 04/30/2025 **Lin. No.:** 00046
Solution File No.: 01319 **Soln. Date:** 04/30/2025 **Soln. No.:** 00316
Sequential File No.: 01319 **File Date:** 04/30/2025

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 01/09/2026
Solution Control Lot: 24020 **Bottle No.:** 0993

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:52D		
Control 1 EC	0.100%	10:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:53D		
Control 2 EC	0.099%	10:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:54D		
Control 3 EC	0.099%	10:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

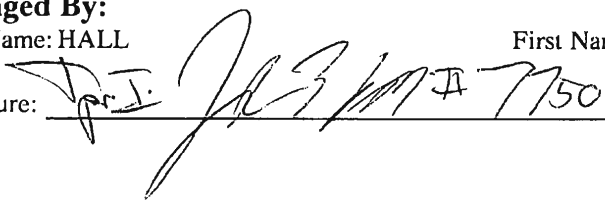
Temperature Probe Serial Number: DDW5 P2-144 

Changed By:

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 04/30/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01298	Calib. Date:	12/30/2024
Certification File No.:	01299	Cert. Date:	12/30/2024
Linearity File No.:	01300	Lin. Date:	12/30/2024
Solution File No.:	01315	Soln. Date:	04/03/2025
Sequential File No.:	01315	File Date:	04/03/2025
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	24260	Expires:	07/23/2026
		Bottle No.:	0152

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:39S		
Control 1 EC	0.099%	05:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:41S		
Control 2 EC	0.098%	05:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:42S		
Control 3 EC	0.098%	05:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:43S		

All tests within acceptable tolerance.

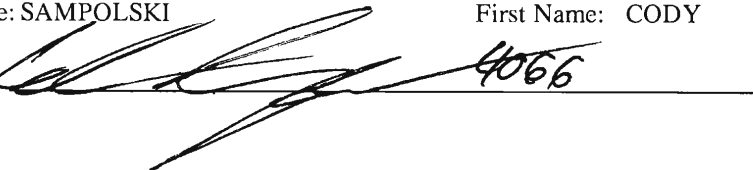
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPOLSKI

First Name: CODY

MI: E

Signature: 

Badge No.: 4066

Date: 04/03/2025

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01298 Calib. Date: 12/30/2024 Calib. No.: 00054
Certification File No.: 01299 Cert. Date: 12/30/2024 Cert. No.: 00046
Linearity File No.: 01300 Lin. Date: 12/30/2024 Lin. No.: 00045
Solution File No.: 01310 Soln. Date: 03/02/2025 Soln. No.: 00314
Sequential File No.: 01310 File Date: 03/02/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 07/23/2026
Solution Control Lot: 24260 Bottle No.: 0581

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:15S		
Control 1 EC	0.098%	04:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:16S		
Control 2 EC	0.098%	04:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:18S		
Control 3 EC	0.099%	04:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:19S		

All tests within acceptable tolerance.

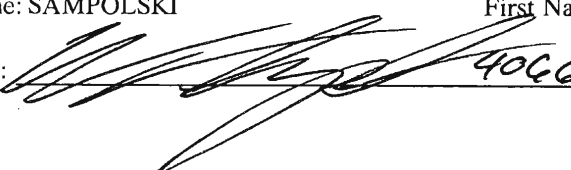
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPOLSKI

First Name: CODY

MI: E

Signature: 

Badge No.: 4066

Date: 03/02/2025

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01298	Calib. Date:	12/30/2024
Certification File No.:	01299	Cert. Date:	12/30/2024
Linearity File No.:	01300	Lin. Date:	12/30/2024
Solution File No.:	01306	Soln. Date:	01/28/2025
Sequential File No.:	01306	File Date:	01/28/2025
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	24260	Expires:	07/23/2026
		Bottle No.:	0034

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:26S		
Control 1 EC	0.099%	04:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:27S		
Control 2 EC	0.098%	04:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:29S		
Control 3 EC	0.099%	04:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 01/28/2025