

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
Location: FRANKLIN TOWNSHIP P.D.  
Calibration File No.: 00641 Calib. Date: 09/04/2024 Calib. No.: 00044  
Certification File No.: 00642 Cert. Date: 09/04/2024 Cert. No.: 00037  
Linearity File No.: 00643 Lin. Date: 09/04/2024 Lin. No.: 00037  
Solution File No.: 00656 Soln. Date: 12/08/2024 Soln. No.: 00208  
Sequential File No.: 00656 File Date: 12/08/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0286  
Control Solution %: 0.100% Expires: 01/09/2026  
Solution Control Lot: 24020 Bottle No.: 1069

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 16:26S |                |                     |
| Control 1 EC      | 0.099% | 16:26S | 33.9°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.100% | 16:26S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:27S |                |                     |
| Control 2 EC      | 0.098% | 16:28S | 33.9°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.098% | 16:28S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:28S |                |                     |
| Control 3 EC      | 0.097% | 16:29S | 33.9°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.099% | 16:29S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:30S |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: KRAUSS

First Name: SCOTT

MI: J

Signature:  #1164

Badge No.: 1164

Date: 12/08/2024

Buena

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
**Location:** FRANKLIN TOWNSHIP P.D.  
**Calibration File No.:** 00641 **Calib. Date:** 09/04/2024 **Calib. No.:** 00044  
**Certification File No.:** 00642 **Cert. Date:** 09/04/2024 **Cert. No.:** 00037  
**Linearity File No.:** 00643 **Lin. Date:** 09/04/2024 **Lin. No.:** 00037  
**Solution File No.:** 00652 **Soln. Date:** 11/13/2024 **Soln. No.:** 00207  
**Sequential File No.:** 00652 **File Date:** 11/13/2024

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDWH S3-0286  
**Control Solution %:** 0.100% **Expires:** 01/09/2026  
**Solution Control Lot:** 24020 **Bottle No.:** 0399

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 11:17S        |                               |                           |
| Control 1 EC      | 0.097%         | 11:17S        | 33.9°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.098%         | 11:17S        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 11:18S        |                               |                           |
| Control 2 EC      | 0.097%         | 11:19S        | 33.9°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.099%         | 11:19S        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 11:20S        |                               |                           |
| Control 3 EC      | 0.097%         | 11:20S        | 33.9°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.099%         | 11:20S        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 11:21S        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_

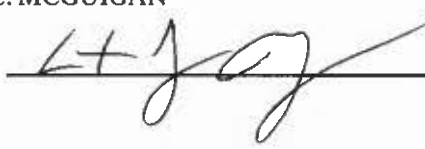

Badge No.: 1143

Date: 11/13/2024

# Calibrating Unit

## New Standard Solution Report

|                         |                        |                          |
|-------------------------|------------------------|--------------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.: ARXB-0074    |
| Location:               | FRANKLIN TOWNSHIP P.D. |                          |
| Calibration File No.:   | 00641                  | Calib. Date: 09/04/2024  |
| Certification File No.: | 00642                  | Calib. No.: 00044        |
| Linearity File No.:     | 00643                  | Cert. Date: 09/04/2024   |
| Solution File No.:      | 00651                  | Cert. No.: 00037         |
| Sequential File No.:    | 00651                  | Lin. Date: 09/04/2024    |
|                         |                        | Lin. No.: 00037          |
|                         |                        | Soln. Date: 10/14/2024   |
|                         |                        | Soln. No.: 00206         |
|                         |                        | File Date: 10/14/2024    |
| <br>                    |                        |                          |
| Calibrating Unit:       | WET                    | Model No.: CU-34         |
| Control Solution %:     | 0.100%                 | Serial No.: DDWH S3-0286 |
| Solution Control Lot:   | 24020                  | Expires: 01/09/2026      |
|                         |                        | Bottle No.: 0409         |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 04:52D |                |                     |
| Control 1 EC      | 0.100% | 04:53D | 33.9°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.099% | 04:53D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 04:54D |                |                     |
| Control 2 EC      | 0.099% | 04:54D | 33.9°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.100% | 04:54D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 04:55D |                |                     |
| Control 3 EC      | 0.099% | 04:55D | 33.9°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.100% | 04:55D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 04:56D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: HEIMERL

First Name: CHARLES

MI: A

Signature: \_\_\_\_\_



Badge No.: 11102

Date: 10/14/2024

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
Location: FRANKLIN TOWNSHIP P.D.  
Calibration File No.: 00622 Calib. Date: 04/01/2024 Calib. No.: 00043  
Certification File No.: 00623 Cert. Date: 04/01/2024 Cert. No.: 00036  
Linearity File No.: 00624 Lin. Date: 04/01/2024 Lin. No.: 00036  
Solution File No.: 00638 Soln. Date: 08/11/2024 Soln. No.: 00204  
Sequential File No.: 00638 File Date: 08/11/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0286  
Control Solution %: 0.100% Expires: 01/09/2026  
Solution Control Lot: 24020 Bottle No.: 0904

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 22:25D |                |                     |
| Control 1 EC      | 0.098% | 22:25D | 33.9°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.099% | 22:25D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:26D |                |                     |
| Control 2 EC      | 0.098% | 22:26D | 33.9°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.100% | 22:26D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:27D |                |                     |
| Control 3 EC      | 0.098% | 22:28D | 33.9°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.099% | 22:28D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:28D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: NEHER

First Name: MICHAEL

MI: E

Signature: \_\_\_\_\_

*Off. Michael Neher #1155*

Badge No.: 1155

Date: 08/11/2024

# Calibrating Unit

## New Standard Solution Report

|                         |                        |                          |
|-------------------------|------------------------|--------------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.: ARXB-0074    |
| Location:               | FRANKLIN TOWNSHIP P.D. |                          |
| Calibration File No.:   | 00622                  | Calib. Date: 04/01/2024  |
| Certification File No.: | 00623                  | Calib. No.: 00043        |
| Linearity File No.:     | 00624                  | Cert. Date: 04/01/2024   |
| Solution File No.:      | 00636                  | Cert. No.: 00036         |
| Sequential File No.:    | 00636                  | Lin. Date: 04/01/2024    |
|                         |                        | Lin. No.: 00036          |
|                         |                        | Soln. Date: 07/16/2024   |
|                         |                        | Soln. No.: 00203         |
|                         |                        | File Date: 07/16/2024    |
| <br>                    |                        |                          |
| Calibrating Unit:       | WET                    | Model No.: CU-34         |
| Control Solution %:     | 0.100%                 | Serial No.: DDWH S3-0286 |
| Solution Control Lot:   | 24020                  | Expires: 01/09/2026      |
|                         |                        | Bottle No.: 1473         |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 05:55D        |                               |                           |
| Control 1 EC      | 0.100%         | 05:56D        | 33.9°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.099%         | 05:56D        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 05:57D        |                               |                           |
| Control 2 EC      | 0.099%         | 05:57D        | 33.9°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.099%         | 05:57D        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 05:58D        |                               |                           |
| Control 3 EC      | 0.099%         | 05:59D        | 33.9°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.099%         | 05:59D        | 33.9°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 05:59D        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HEIMERL

First Name: CHARLES

MI: A

Signature: \_\_\_\_\_

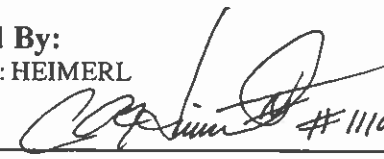

#11102

Badge No.: 11102

Date: 07/16/2024

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
Location: FRANKLIN TOWNSHIP P.D.  
Calibration File No.: 00622 Calib. Date: 04/01/2024 Calib. No.: 00043  
Certification File No.: 00623 Cert. Date: 04/01/2024 Cert. No.: 00036  
Linearity File No.: 00624 Lin. Date: 04/01/2024 Lin. No.: 00036  
Solution File No.: 00635 Soln. Date: 06/13/2024 Soln. No.: 00202  
Sequential File No.: 00635 File Date: 06/13/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWH S3-0286  
Control Solution %: 0.100% Expires: 01/09/2026  
Solution Control Lot: 24020 Bottle No.: 0014

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 12:45D |                |                     |
| Control 1 EC      | 0.100% | 12:46D | 33.9°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.099% | 12:46D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:46D |                |                     |
| Control 2 EC      | 0.099% | 12:47D | 33.9°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 12:47D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:48D |                |                     |
| Control 3 EC      | 0.099% | 12:48D | 33.9°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.100% | 12:48D | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:49D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-018 (WFW)

**Changed By:**

Last Name: WIDENER

First Name: WILLIAM

MI: F

Signature: TOP Wm. F. Widener #7817

Badge No.: 7817

Date: 06/13/2024

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDWHS3-0286

Certification Date:

4-23-24

Technician:

DH/JP

Re-Certification Due Date:

4-23-25

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWAP2-018

Certification Date:

4-23-24

Next Certification Due:

4-23-25

Probe Value:

104

Draeger, Inc.

DH/JP



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 01/22/2024

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 24020

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1194 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 9, 2026.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 25 day of January, 2024.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**William F. Widener III**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 142 OF  
THE LAWS OF 1966 IN THE OPERATION OF THE  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 19th DAY OF August

TWO THOUSAND AND

Sixteen

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

| DATE              | Refresher Course<br>PLACE | INSTRUCTOR              |
|-------------------|---------------------------|-------------------------|
| 1. <u>12/3/18</u> | <u>GUES</u>               | <u>Adam [Signature]</u> |
| 2. <u>9-8-20</u>  | <u>ACCP</u>               | <u>Wm [Signature]</u>   |
| 3. <u>2-7-22</u>  | <u>ACCP</u>               | <u>[Signature]</u>      |
| 4. _____          | _____                     | _____                   |
| 5. _____          | _____                     | _____                   |
| 6. _____          | _____                     | _____                   |
| 7. _____          | _____                     | _____                   |
| 8. _____          | _____                     | _____                   |
| 9. _____          | _____                     | _____                   |

G.P. 2508 (Rev. 03/16)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**William F. Widener**

**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSIS PURSUANT TO CHAPTER 142 OF  
THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 1st DAY OF March

TWO THOUSAND AND Twenty Three

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE     | Refresher Course<br>PLACE | INSTRUCTOR |
|----------|---------------------------|------------|
| 1. _____ | _____                     | _____      |
| 2. _____ | _____                     | _____      |
| 3. _____ | _____                     | _____      |
| 4. _____ | _____                     | _____      |
| 5. _____ | _____                     | _____      |
| 6. _____ | _____                     | _____      |
| 7. _____ | _____                     | _____      |
| 8. _____ | _____                     | _____      |
| 9. _____ | _____                     | _____      |

G.P. 2508 (Rev. 10/22)

# Calibrating Unit

## New Standard Solution Report

|                         |                        |                       |
|-------------------------|------------------------|-----------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.: ARXB-0074 |
| Location:               | FRANKLIN TOWNSHIP P.D. |                       |
| Calibration File No.:   | 00622                  | Calib. No.: 00043     |
| Certification File No.: | 00623                  | Cert. No.: 00036      |
| Linearity File No.:     | 00624                  | Lin. No.: 00036       |
| Solution File No.:      | 00634                  | Soln. No.: 00201      |
| Sequential File No.:    | 00634                  | File Date: 05/26/2024 |
| <br>                    |                        |                       |
| Calibrating Unit:       | WET                    | Model No.: CU-34      |
| Control Solution %:     | 0.100%                 | Serial No.: DDBJ-0006 |
| Solution Control Lot:   | 24020                  | Expires: 01/09/2026   |
|                         |                        | Bottle No.: 0541      |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 15:43D        |                               |                           |
| Control 1 EC      | 0.098%         | 15:44D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.098%         | 15:44D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 15:45D        |                               |                           |
| Control 2 EC      | 0.098%         | 15:45D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.099%         | 15:45D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 15:46D        |                               |                           |
| Control 3 EC      | 0.098%         | 15:47D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.098%         | 15:47D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 15:47D        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: ELLIOTT

First Name: CODY

MI: J

Signature: \_\_\_\_\_



Badge No.: 11113

Date: 05/26/2024

# Calibrating Unit

## New Standard Solution Report

|                         |                        |              |            |
|-------------------------|------------------------|--------------|------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.:  | ARXB-0074  |
| Location:               | FRANKLIN TOWNSHIP P.D. |              |            |
| Calibration File No.:   | 00622                  | Calib. Date: | 04/01/2024 |
| Certification File No.: | 00623                  | Cert. Date:  | 04/01/2024 |
| Linearity File No.:     | 00624                  | Lin. Date:   | 04/01/2024 |
| Solution File No.:      | 00633                  | Soln. Date:  | 05/26/2024 |
| Sequential File No.:    | 00633                  | File Date:   | 05/26/2024 |
| Calibrating Unit:       | WET                    | Model No.:   | CU-34      |
| Control Solution %:     | 0.100%                 | Serial No.:  | DDBJ-0006  |
| Solution Control Lot:   | 24020                  | Expires:     | 01/09/2026 |
|                         |                        | Bottle No.:  | 0406       |

| Function          | Result | Time   | Temperature    | Comment(s)            |
|-------------------|--------|--------|----------------|-----------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)           |
| Ambient Air Blank | 0.000% | 02:11D |                |                       |
| Control 1 EC      | 0.097% | 02:12D | 33.9°C         | AMBIENT AIR CHECK ERR |
| Control 1 IR      | -.---% | 02:12D | 33.9°C         | AMBIENT AIR CHECK ERR |
| Ambient Air Blank | 0.046% | 02:12D |                |                       |
| Control 2 EC      | -.---% | --:--  | N/A            |                       |
| Control 2 IR      | -.---% | --:--  | N/A            |                       |
| Ambient Air Blank | -.---% | --:--  |                |                       |
| Control 3 EC      | -.---% | --:--  | N/A            |                       |
| Control 3 IR      | -.---% | --:--  | N/A            |                       |
| Ambient Air Blank | -.---% | --:--  |                |                       |

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: HEIMERL

First Name: CHARLES

MI: A

Signature: \_\_\_\_\_

 #11102

Badge No.: 11102

Date: 05/26/2024

# Calibrating Unit

## New Standard Solution Report

|                         |                        |                         |
|-------------------------|------------------------|-------------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.: ARXB-0074   |
| Location:               | FRANKLIN TOWNSHIP P.D. |                         |
| Calibration File No.:   | 00622                  | Calib. Date: 04/01/2024 |
| Certification File No.: | 00623                  | Calib. No.: 00043       |
| Linearity File No.:     | 00624                  | Cert. Date: 04/01/2024  |
| Solution File No.:      | 00629                  | Cert. No.: 00036        |
| Sequential File No.:    | 00629                  | Lin. Date: 04/01/2024   |
|                         |                        | Lin. No.: 00036         |
|                         |                        | Soln. Date: 05/10/2024  |
|                         |                        | Soln. No.: 00199        |
|                         |                        | File Date: 05/10/2024   |
| <br>                    |                        |                         |
| Calibrating Unit:       | WET                    | Model No.: CU-34        |
| Control Solution %:     | 0.100%                 | Serial No.: DDBJ-0006   |
| Solution Control Lot:   | 24020                  | Expires: 01/09/2026     |
|                         |                        | Bottle No.: 0135        |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 12:00D |                |                     |
| Control 1 EC      | 0.100% | 12:00D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.099% | 12:00D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:01D |                |                     |
| Control 2 EC      | 0.099% | 12:02D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 12:02D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:02D |                |                     |
| Control 3 EC      | 0.099% | 12:03D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.099% | 12:03D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:04D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HEIMERL

First Name: CHARLES

MI: A

Signature: \_\_\_\_\_



Badge No.: 11102

Date: 05/10/2024

# Calibrating Unit

Buena

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
Location: FRANKLIN TOWNSHIP P.D.  
Calibration File No.: 00605 Calib. Date: 11/06/2023 Calib. No.: 00042  
Certification File No.: 00606 Cert. Date: 11/06/2023 Cert. No.: 00035  
Linearity File No.: 00607 Lin. Date: 11/06/2023 Lin. No.: 00035  
Solution File No.: 00617 Soln. Date: 02/23/2024 Soln. No.: 00197  
Sequential File No.: 00617 File Date: 02/23/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBJ-0006  
Control Solution %: 0.100% Expires: 02/01/2025  
Solution Control Lot: 23040 Bottle No.: 0033

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 13:10S        |                               |                           |
| Control 1 EC      | 0.101%         | 13:10S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.101%         | 13:10S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 13:11S        |                               |                           |
| Control 2 EC      | 0.100%         | 13:12S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.101%         | 13:12S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 13:12S        |                               |                           |
| Control 3 EC      | 0.101%         | 13:13S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.101%         | 13:13S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 13:14S        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: MCGUIGAN

First Name: JEFFREY

MI: M

Signature: \_\_\_\_\_



Badge No.: 1143

Date: 02/23/2024

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
Location: FRANKLIN TOWNSHIP P.D.  
Calibration File No.: 00605 Calib. Date: 11/06/2023 Calib. No.: 00042  
Certification File No.: 00606 Cert. Date: 11/06/2023 Cert. No.: 00035  
Linearity File No.: 00607 Lin. Date: 11/06/2023 Lin. No.: 00035  
Solution File No.: 00613 Soln. Date: 01/20/2024 Soln. No.: 00196  
Sequential File No.: 00613 File Date: 01/20/2024

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDBJ-0006  
Control Solution %: 0.100% Expires: 02/01/2025  
Solution Control Lot: 23040 Bottle No.: 0718

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 14:35S |                |                     |
| Control 1 EC      | 0.099% | 14:35S | 33.9°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.100% | 14:35S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:36S |                |                     |
| Control 2 EC      | 0.098% | 14:37S | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.100% | 14:37S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:37S |                |                     |
| Control 3 EC      | 0.099% | 14:38S | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.100% | 14:38S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:39S |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: MURRAY

First Name: JOSEPH

MI: T

Signature: \_\_\_\_\_



Badge No.: 1154

Date: 01/20/2024