

ALCOTEST CHECKLIST

Municipality: FRANKLIN TWP. Alcotest Ser.#: ARXB-0074

County: GLOUCESTER Date of Calibration: 02-17-2025

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDBJ - 0006

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWJ P2-088

4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 240 418 745

5. **NIST - Traceable Digital Thermometer Readings.**

6. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDL B P3-0178

7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/>	A.	0.04% Solution.	<u>23210</u>
<input checked="" type="checkbox"/>	B.	0.08% Solution.	<u>23290</u>
<input checked="" type="checkbox"/>	C.	0.10% Solution.	<u>23230</u>
<input checked="" type="checkbox"/>	D.	0.16% Solution.	<u>23250</u>

8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

A. 0.04% used in Calibration/Linearity Testing DDRF S3-0008
 B. 0.08% used in Calibration/Linearity Testing DDRK S3-0011
 C. 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.]
 D. 0.16% used in Calibration/Linearity Testing DDRK S3-0022

9. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 24260
 D. Alcotest card of operator/coordinator who completed change.


Dräger**Alcotest 7110****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

3/16/21ARXB-0074

Dräger, Inc..

GR

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDBJ-0006

Certification Date:

9-16-24

Technician:

DH / CR

Re-Certification Due Date:

9-16-25

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWJ P2-048

Certification Date:

9-17-24

Next Certification Due:

9-17-25

Probe Value:

107

Draeger, Inc.

DH / CR



Calibration complies with ISO/IEC 17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-15138511

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 240418745 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	08 Aug 2024	1000494698
Temperature Probe	3039	03 Aug 2024	15-E5O3Q-20-1
Temperature Probe	5401	28 Jul 2024	4500031366
Temperature Probe	5357	28 Jul 2024	4500031372
Thermistor Module	B5C344	10 Jul 2024	1000493579
Temperature Calibration Bath	B5C478		
Temperature Calibration Bath	B93537		
Temperature Calibration Bath	B96546		
Temperature Probe	5407	10 Jan 2025	4500038066
Thermistor Module	8A070	28 Aug 2024	1000495892

Certificate Information:

Technician: 420 Procedure: CAL-06 Cal Date: 21 May 2024 Cal Due Date: 21 May 2026

Test Conditions: 64.01%RH 24.08°C 1009mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.001	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.001	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		99.997	100.002	Y	99.947	100.047	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement : (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-15138511

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 21 May 2024

**CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com**

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Trpr. I Joshua B. Hill
Name

7750
Badge No.

Location:

Franklin Township P. D.
Agency

ARXB-0074
Alcotest Serial No.

Equipment:

240 418 745
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDRF S3-0008	07:53 S	08:55 S	34.0°C
0.08%	DDRK S3-0011	07:53 S	08:56 S	34.0°C
0.10%	DDBT-0006	07:53 S	08:57 S	34.0°C
0.16%	DDRK S3-0022	07:53 S	08:58 S	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Joshua B. Hill #7750
Coordinator's Signature

02/17/2025
Date

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
FRANKLIN TOWNSHIP P.D.
Serial No.: ARXB-0074

Calibration File No.:	00663	Calib. Date:	02/17/2025	Calib. No.:	00045
Certification File No.:	00642	Cert. Date:	09/04/2024	Cert. No.:	00037
Linearity File No.:	00643	Lin. Date:	09/04/2024	Lin. No.:	00037
Solution File No.:	00658	Soln. Date:	01/18/2025	Soln. No.:	00209
Sequential File No.:	00663	File Date:	02/17/2025		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDBJ-0006
Control Solution %:	0.100%			Expires:	06/26/2025
Solution Control Lot:	23230			Bottle No.:	0288


Coordinator

Last Name: HALL
First Name: JOSHUA
MI: B
Badge No.: 7750
Date: 02/17/2025

Signature:  # 7750

*Black Key Temperature Probe Serial.....# DDL B P3-0178 (TB)

*Digital NIST Temperature Measuring System Serial.....# 240 418 745 (TB)

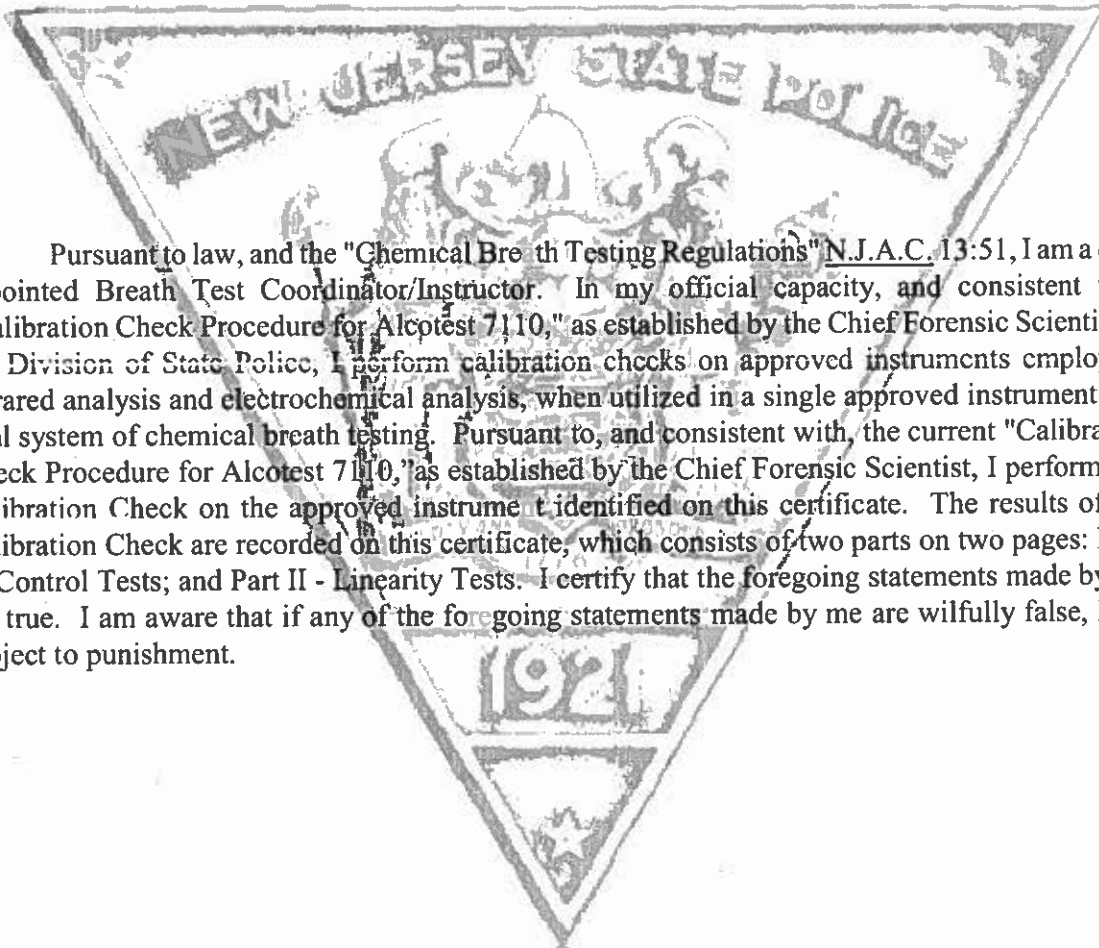

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
FRANKLIN TOWNSHIP P.D.
Serial No.: ARXB-0074

Calibration File No.:	00663	Calib. Date:	02/17/2025	Calib. No.:	00045
Certification File No.:	00664	Cert. Date:	02/17/2025	Cert. No.:	00038
Linearity File No.:	00643	Lin. Date:	09/04/2024	Lin. No.:	00037
Solution File No.:	00658	Soln. Date:	01/18/2025	Soln. No.:	00209
Sequential File No.:	00664	File Date:	02/17/2025		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDBJ-0006
Control Solution %:	0.100%			Expires:	06/26/2025
Solution Control Lot:	23230			Bottle No.:	0288

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:11S		
Control 1 EC	0.099%	09:11S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:12S		
Control 2 EC	0.099%	09:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13S		
Control 3 EC	0.099%	09:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15S		

All tests within acceptable tolerance.

Coordinator

Last Name: HALL First Name: JOSHUA MI: B

Signature:  Badge No.: 7750 Date: 02/17/2025

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXB-0074
Location: FRANKLIN TOWNSHIP P.D.
Calibration File No.: 00663 Calib. Date: 02/17/2025 Calib. No.: 00045
Certification File No.: 00664 Cert. Date: 02/17/2025 Cert. No.: 00038
Linearity File No.: 00665 Lin. Date: 02/17/2025 Lin. No.: 00038
Solution File No.: 00658 Soln. Date: 01/18/2025 Soln. No.: 00209
Sequential File No.: 00665 File Date: 02/17/2025

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRF S3-0008
Control Solution %: 0.040% Expires: 06/12/2025
Solution Control Lot: 23210 Bottle No.: 0147

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0011
Control Solution %: 0.080% Expires: 08/03/2025
Solution Control Lot: 23290 Bottle No.: 0087

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0022
Control Solution %: 0.160% Expires: 07/05/2025
Solution Control Lot: 23250 Bottle No.: 1296

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:32S		
Control 1 EC	0.041%	09:33S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34S		
Control 2 EC	0.041%	09:35S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:36S		
Control 3 EC	0.081%	09:37S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:37S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:39S		
Control 4 EC	0.080%	09:39S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41S		
Control 5 EC	0.159%	09:42S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	09:42S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		
Control 6 EC	0.158%	09:44S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.160%	09:44S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45S		

All tests within acceptable tolerance.

Coordinator

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 02/17/2025

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Joshua B. Hall

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND Twenty Two

D. J. Cole
COLONEL
NEW JERSEY STATE POLICE

W. J. A.
ACTING ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 02/22)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Joshua B. Hall

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1964 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 21st DAY OF December

TWO THOUSAND AND Seventeen

D. J. Cole
ACTING SUPERINTENDENT
NEW JERSEY STATE POLICE

W. J. A.
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>8/22/19</u>	<u>N.J.S.P. Galloway</u>	<u>B. A.</u>
2. <u>1/12/21</u>	<u>ACCC</u>	<u>B. M.</u>
3. <u>10-3-23</u>	<u>ACCC</u>	<u>B. M.</u>
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 11/17)



NEW JERSEY STATE POLICE
Alcohol Drug Testing Unit

Tpr. II Joshua B. Hall #7750

Hamilton Technology Complex
Suite #400
1200 Negron Drive
Hamilton, NJ 08691

Tel#: (609) 584-5051 ext 5608
Email: Joshua.Hall@njsp.gov
Cell# (609) 947-3179



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

CERTIFICATION OF ANALYSIS 0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/10/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23210

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0486 to 0.0490 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 12, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11 day of August, 2023.

Karen E. Stahl
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110622
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 09/14/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0958 to 0.0971 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 03, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of September, 2023.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 09/12/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of September, 2023.

Notary signature

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 6/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

CERTIFICATION OF ANALYSIS 0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 09/14/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1923 to 0.1953 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 05, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of September 2023.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDRF53-0008

Certification Date:

Technician:

Re-Certification Due Date:

12-16-24 DH / QR

12-16-25

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDRK53-0011

Certification Date:

Technician:

Re-Certification Due Date:

12-19-24 DH / QR

12-19-25

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDRK53-0022

Certification Date:

Technician:

Re-Certification Due Date:

12-16-24

DH / QR

12-16-25

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDLBP3-0178

12-19-24

12-19-25

Probe Value:

103

Dräger, Inc.

DH / QR



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TANIESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/08/2024

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 24260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2026.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Michael Kennedy

Michael Kennedy
Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of August, 2024.

Handwritten signature of Notary Karen E. Stahl

Notary

KAREN E. STAHL
Notary Public, State of New Jersey
Comm. # 50110522
My Commission Expires 8/13/2029



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

