

# ALCOTEST CHECKLIST

Municipality: WILLINGBORO Alcotest Ser. #: ARWC - 0060

County: BURLINGTON Date of Calibration: 01-22-2015

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.  
Ser. #: DDWE 53 - 0189

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.  
Ser. #: DDUN P2 - 293

4. **Digital Temperature Measuring System Report of Calibration.**  
Ser. #: 130602271

5.  A. Alcotest 7110 Calibration Record  
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**  
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**  
 D. **Alcotest Card** of operator/coordinator who performed tests.  
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].  
Ser. #: DDUN P2 - 231

6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>13</u>	<u>I</u>	<u>120</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>13</u>	<u>I</u>	<u>121</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>13</u>	<u>I</u>	<u>122</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>14</u>	<u>H</u>	<u>131</u>

7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

A. 0.04% used in Calibration/Linearity Testing. DDMK 53 - 0003  
 B. 0.08% used in Calibration/Linearity Testing. DDAE - 0022  
 C. 0.10% used in Calibration/Linearity Testing.  
[Same as CU34 unit on instrument.]  
 D. 0.16% used in Calibration/Linearity Testing. DDCN - 0052

8.  A. New Standard Solution Report following Calibration.  
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].  
 C. Certificate of Analysis 0.10% solution for same.  
Lot #: 13 G 115  
 D. Alcotest card of operator/coordinator who completed change.

02-24-2015

**Dräger**

**Alcotest® 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

2-10-14

SERIAL NUMBER:

ARWC-0060

Dräger Safety Diagnostics, Inc.

BC



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Dräger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWE S3-0189

Certification Date

Technician

Re-Certification Due Date

10-8-14

BC

10-8-15

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUN Pa-293

10-6-14

10-6-15

Probe Value

104

**Dräger Safety Diagnostics, Inc.**  
Technical Service Department

BC



Calibration  
Certificate No. 1750.01

Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-5427014

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087  
**Instrument Identification:**

Model: 61220-601 S/N: 130602271 Manufacturer: Control Company

**Standards/Equipment:**

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-178	A45240		
Thermistor Module	A17118	2/13/14	1000332071
Temperature Probe	128	2/20/14	6-B48Z9-30-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A17118	2/13/14	1000332071
Temperature Probe	3039	2/20/14	6-B48Z9-1-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Module	A27129	11/09/13	1000327261
Temperature Probe	5202	11/30/14	15-B15PW-1-1
Temperature Calibration Bath TC-275	B16388		
Digital Thermometer	B16815	8/12/14	1000341967
PRT Temperature Probe	02022	8/14/15	83812004

**Certificate Information:**

Technician: 88 Procedure: CAL-08 Cal Date: 10/08/13 Cal Due: 10/08/15  
Test Conditions: 24.0°C 37.0 %RH 1017 mBar

**Calibration Data: (New Instrument)**

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.001	0.000	Y	-0.051	0.049	0.013	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.023	2.2:1
°C		N.A.		50.003	50.001	Y	49.953	50.053	0.014	3.6:1
°C		N.A.		100.001	99.994	Y	99.951	100.051	0.018	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

*Nicol Rodriguez*  
Nicol Rodriguez, Quality Manager

*Arnon Justice*  
Arnon Justice, Technical Manager

**Maintaining Accuracy:**

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA  
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-RvA.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

# Alcotest 7110 Calibration Record

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWC-0060  
Location: WILLINGBORO TWP POLICE  
Calibration File No.: 00501 Calib. Date: 01/22/2015 Calib. No.: 00028  
Certification File No.: 00489 Cert. Date: 07/31/2014 Cert. No.: 00020  
Linearity File No.: 00490 Lin. Date: 07/31/2014 Lin. No.: 00020  
Solution File No.: 00500 Soln. Date: 01/13/2015 Soln. No.: 00133  
Sequential File No.: 00501 File Date: 01/22/2015


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0189  
Control Solution %: 0.100% Expires: 09/17/2015  
Solution Control Lot: 13I122 Bottle No.: 1208

## Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L  
Signature: Sgt. Michelle Goncalves #6040 Badge No.: 6040  
Date: 01/22/2015

\*Black Key Temperature Probe Serial.....# DDUNPA-231 (MA)

\*Digital NIST Temperature Measuring System Serial.....# 130602271 (MA)

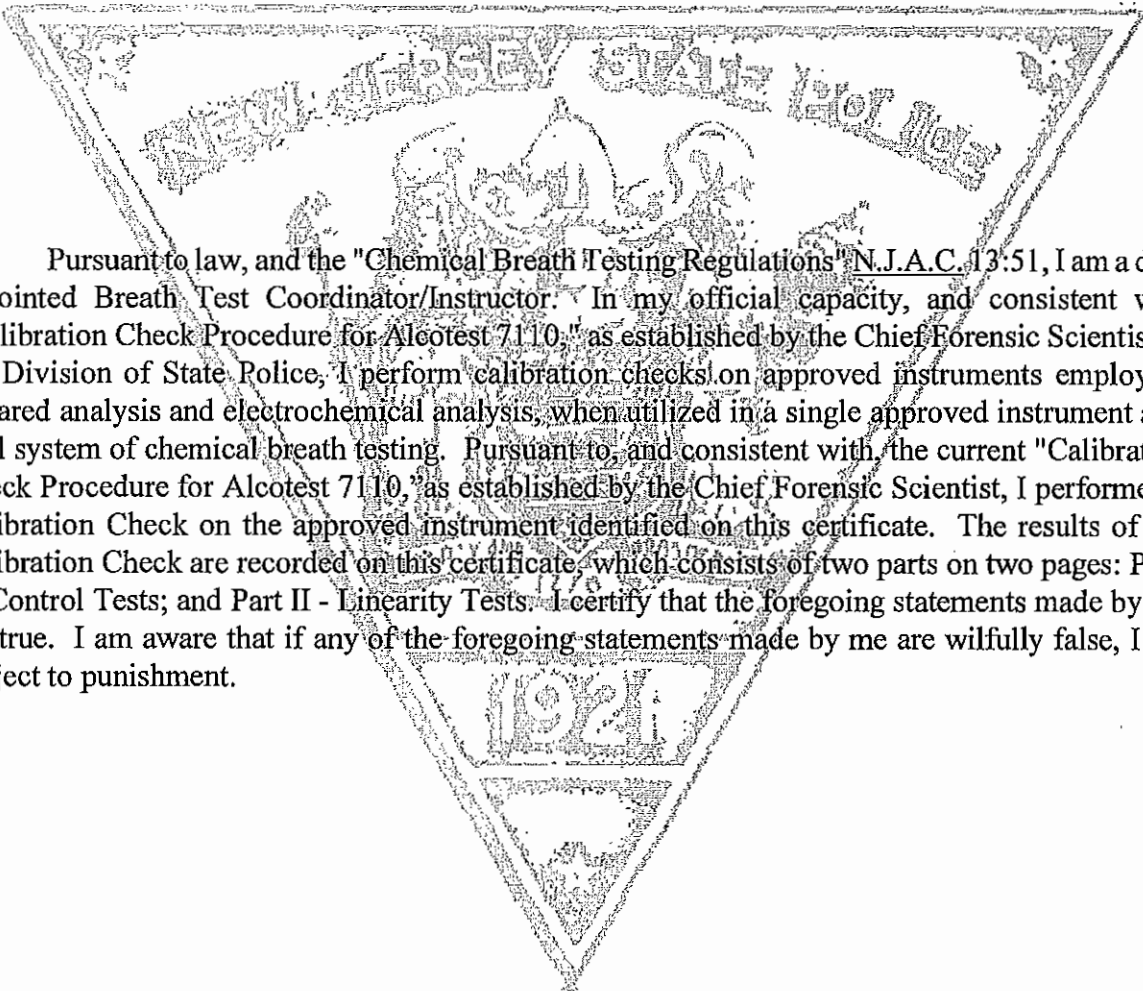

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

### Equipment

Alcotest 7110 MKIII-C  
Location: WILLINGBORO TWP POLICE  
Serial No.: ARWC-0060  
Calibration File No.: 00501 Calib. Date: 01/22/2015 Calib. No.: 00028  
Certification File No.: 00502 Cert. Date: 01/22/2015 Cert. No.: 00021  
Linearity File No.: 00490 Lin. Date: 07/31/2014 Lin. No.: 00020  
Solution File No.: 00500 Soln. Date: 01/13/2015 Soln. No.: 00133  
Sequential File No.: 00502 File Date: 01/22/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0189  
Control Solution %: 0.100% Expires: 09/17/2015  
Solution Control Lot: 13I122 Bottle No.: 1208

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:03S		
Control 1 EC	0.099%	10:03S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04S		
Control 2 EC	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05S		
Control 3 EC	0.100%	10:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L  
Signature:  Badge No.: 6040  
Date: 01/22/2015

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWC-0060  
Location: WILLINGBORO TWP POLICE  
Calibration File No.: 00501 Calib. Date: 01/22/2015 Calib. No.: 00028  
Certification File No.: 00502 Cert. Date: 01/22/2015 Cert. No.: 00021  
Linearity File No.: 00503 Lin. Date: 01/22/2015 Lin. No.: 00021  
Solution File No.: 00500 Soln. Date: 01/13/2015 Soln. No.: 00133  
Sequential File No.: 00503 File Date: 01/22/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0003  
Control Solution %: 0.040% Expires: 09/13/2015  
Solution Control Lot: 13I120 Bottle No.: 1134

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0022  
Control Solution %: 0.080% Expires: 09/16/2015  
Solution Control Lot: 13I121 Bottle No.: 0128

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCN-0052  
Control Solution %: 0.160% Expires: 08/05/2016  
Solution Control Lot: 14H131 Bottle No.: 1062

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:18S		
Control 1 EC	0.041%	10:19S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	10:19S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20S		
Control 2 EC	0.041%	10:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.038%	10:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:23S		
Control 3 EC	0.081%	10:23S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	10:23S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:25S		
Control 4 EC	0.081%	10:25S	33.9°C	*** TEST PASSED ***
Control 4 IR	0.079%	10:25S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:27S		
Control 5 EC	0.160%	10:27S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	10:27S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:29S		
Control 6 EC	0.159%	10:30S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.159%	10:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:31S		


All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: 

Badge No.: 6040

Date: 01/22/2015

DEPARTMENT OF  
**Traffic and Public Safety**  
*It is to be certified that*

**Michelle L. Goncalves**  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT THE COURSE...  
 THE LAWS OF THE STATE OF NEW JERSEY...  
 A SECTION TO BE DESIGNATED...  
 CITY OF...  
 15th DAY OF December

*[Signature]*  
 SUPERVISOR  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12-3-13	CCPA	Wm Lora
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2008 (Rev. 05/10)

DEPARTMENT OF  
**Traffic and Public Safety**  
*It is to be certified that*

**Michelle Goncalves**  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT THE COURSE...  
 THE LAWS OF THE STATE OF NEW JERSEY...  
 A SECTION TO BE DESIGNATED...  
 CITY OF...  
 23rd DAY OF March

*[Signature]*  
 SUPERVISOR  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2008 (Rev. 05/10)





CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lieutenant Governor

*State of New Jersey*  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF CRIMINAL JUSTICE  
PO BOX 085  
TRENTON, NJ 08625-0085  
TELEPHONE: (609) 984-6300

JEFFREY S. CHIESA  
Attorney General

STEPHEN J. TAYLOR  
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent  
Division of State Police  
Division Headquarters  
P.O. Box 7068  
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -  
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:


Pursuant to the provisions of *N.J.A.C. 13:51-2.1* (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A. 39:4-50.3*, *39:3-10.25* and *12:7-56*, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa  
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police  
DSFC Patrick Guilfooy, Unit Head, Alcohol/Drug Test Unit, Division of State Police ✓



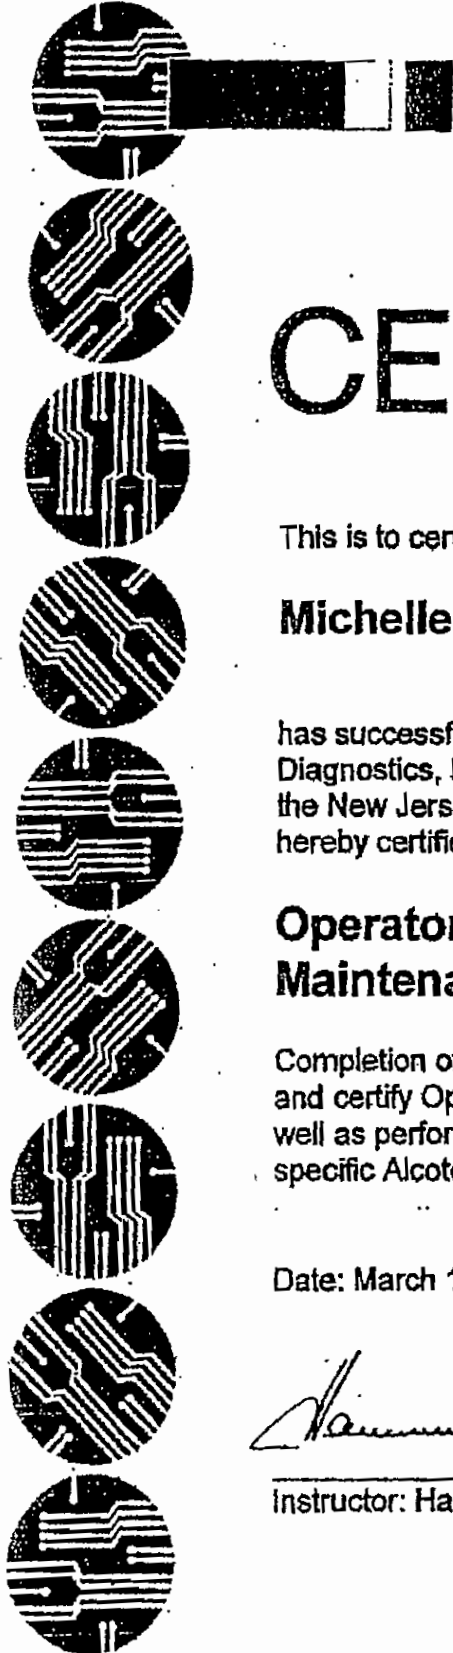

# CERTIFICATE

This is to certify that


**Michelle Goncalves**

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and  
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012

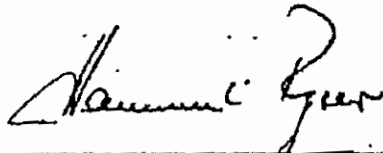  
Instructor: Hansueli Ryser

**Dräger**



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/25/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 13J120

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 13, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


[Handwritten signature of Ali M. Alaoui]

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of October, 2013.

[Handwritten signature of Notary]

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE

Governor

KIM GUADAGNO

Lt. Governor

JOHN J. HOFFMAN

Acting Attorney General

COLONEL JOSEPH R. FUENTES

Superintendent

CERTIFICATION OF ANALYSIS  
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/31/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 131121

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0959 to 0.0971 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 16, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of November, 2013.

Notary

MARY ELIZABETH MCLAUGHLIN  
NOTARY PUBLIC OF NEW JERSEY  
MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

JOHN J. HOFFMAN  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/23/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 131122

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1222 grams per 100 milliliters of solution,


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 17, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.  
 Research Scientist  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28<sup>th</sup> day of October, 2013.

Linda L. DePanti  
 Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

JOHN J. HOFFMAN  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 8/14/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14H131


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1925 to 0.1944 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 5, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

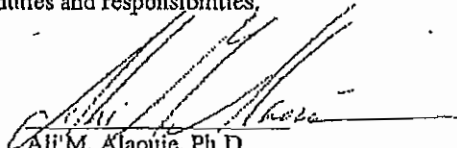  
 Ali M. Alaoui, Ph.D.  
 Research Scientist  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15<sup>th</sup> day of August, 2014.

  
 Notary  
**MARY ELIZABETH MCLAUGHLIN**  
 ID # 2052190  
 NOTARY PUBLIC  
 STATE OF NEW JERSEY  
 My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"  
 New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Dräger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDMK53-0003

Certification Date

Technician

Re-Certification Due Date

9-19-14

BC

9-19-15



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Dräger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDCN-0052

Certification Date

Technician

Re-Certification Due Date

9-22-14

BC

9-22-15



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDAE-0022

Certification Date

8-28-14

Technician

BC

Re-Certification Due Date

8-28-15

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe, within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDUNP2-231

Certification date:

9-19-14

Next Certification due:

9-19-15

Probe Value

107

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

BC



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0060
Location:	WILLINGBORO TWP POLICE	
Calibration File No.:	00501	Calib. Date: 01/22/2015
Certification File No.:	00502	Calib. No.: 00028
Linearity File No.:	00503	Cert. Date: 01/22/2015
Solution File No.:	00504	Cert. No.: 00021
Sequential File No.:	00504	Lin. Date: 01/22/2015
		Lin. No.: 00021
		SoIn. No.: 00134
		File Date: 01/22/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0189
Solution Control Lot:	13G115	Expires: 07/18/2015
		Bottle No.: 0333

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:39S		
Control 1 EC	0.100%	11:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:40S		
Control 2 EC	0.100%	11:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:41S		
Control 3 EC	0.099%	11:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUNP2-293 ME

**Changed By:**

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt. Michelle Goncalves #6040

Badge No.: 6040

Date: 01/22/2015



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lt. Governor

JOHN J. HOFFMAN  
Acting Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.

**ANALYSIS DATE:** 7/29/2013

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 13G115

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1213 to 0.1220 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 18, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 7<sup>th</sup> day of August, 2013.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable

