

ALCOTEST CHECKLIST

Municipality: BURLINGTON TWP. Alcotest Ser.#: ARTL-0024

County: BURLINGTON Calibration Date: 03-15-2010

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used
Ser. #: DDUL S3-0167
3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent
Ser. #: DDXA P2-011
4. **Digital Temperature Measuring System Report of Calibration**
5. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests**
 D. **Alcotest Card** of operator/coordinator who performed tests
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator]
Ser. #: DDWA P2-016
6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
- | | | | | |
|--|----------------|-----------|----------|------------|
| <input checked="" type="checkbox"/> A. | 0.04% Solution | <u>08</u> | <u>F</u> | <u>054</u> |
| <input checked="" type="checkbox"/> B. | 0.08% Solution | <u>08</u> | <u>F</u> | <u>055</u> |
| <input checked="" type="checkbox"/> C. | 0.10% Solution | <u>09</u> | <u>D</u> | <u>065</u> |
| <input checked="" type="checkbox"/> D. | 0.16% Solution | <u>08</u> | <u>G</u> | <u>057</u> |
7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
- A. 0.04% Calibration/Linearity Testing DDWE S3-0196
- B. 0.08% Calibration/Linearity Testing DDWE S3-0203
- C. 0.10% Calibration/Linearity Testing DDUL S3-0167
[Same as instrument's CU34 unit]
- D. 0.16% Calibration/Linearity Testing DDWE S3-0205
8. A. New Standard Solution Report - following Calibration
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument]
 C. Certificate of Analysis 0.10% solution for same
Lot #: _____
 D. Alcotest card of operator/coordinator who completed change

RJP

Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

03/04/200

ARTL-0024

Draeger Safety Diagnostics, Inc.

_____ *JS*



Draegersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDULS3-0167

Certification Date

Technician

Re-Certification Due Date

1/28/10

am

1/28/11

Draegersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXAP2-011

1/28/10

1/28/11

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

am



Calibration
Certificate No. 1750.01

Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NCSL Z540-1



Cert. No.: 4000-2035927

Traceable® Certificate of Calibration for Digital Thermometer

Instrument Identification:

Model: 61220-601 S/N: 80637585 Manufacturer: Control Company

Standards/Equipment:

| Description | Serial Number | Due Date | NIST Traceable Reference |
|--|---------------|----------|--------------------------|
| Temperature Probe Thermistor Module | 149 | 3/06/09 | A82225037-3 |
| Temperature Calibration Bath TC218 | A27129 | 8/22/09 | 1000248949 |
| Temperature Calibration Bath TC155 | A73332 | | |
| Thermistor Module | 93139 | | |
| Temperature Probe | A27129 | 8/22/09 | 1000248949 |
| | 157 | 5/28/09 | A8519038-4 |

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 11/18/08 Cal Due: 11/18/10
Test Conditions: 25.0°C 34.0 %RH 1031 mBar

Calibration Data: (New Instrument)

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min | Max | ±uc | TUR |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|-------|-------|
| °C | | N.A. | | 0.001 | -0.002 | Y | -0.049 | 0.051 | 0.013 | 3.8:1 |
| °C | | N.A. | | 25.001 | 25.003 | Y | 24.951 | 25.051 | 0.013 | 3.8:1 |
| °C | | N.A. | | 60.001 | 59.998 | Y | 59.951 | 60.051 | 0.018 | 2.8:1 |
| °C | | N.A. | | 100.001 | 100.001 | Y | 99.951 | 100.051 | 0.013 | 3.8:1 |

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Date=MM/DD/YY.

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2000 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-AQ-HOU.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

| | | | | | |
|-------------------------|------------------------|--------------|------------|-------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARTL-0024 | | |
| Location: | BURLINGTON TOWNSHIP PD | | | | |
| Calibration File No.: | 00490 | Calib. Date: | 03/15/2010 | Calib. No.: | 00013 |
| Certification File No.: | 00418 | Cert. Date: | 08/25/2009 | Cert. No.: | 00007 |
| Linearity File No.: | 00419 | Lin. Date: | 08/25/2009 | Lin. No.: | 00007 |
| Solution File No.: | 00488 | Soln. Date: | 03/04/2010 | Soln. No.: | 00078 |
| Sequential File No.: | 00490 | File Date: | 03/15/2010 | | |
| Calibrating Unit: | WET | Model No.: | CÜ-34 | Serial No.: | DDUL S3-0167 |
| Control Solution %: | 0.100% | | | Expires: | 04/22/2011 |
| Solution Control Lot: | 09D065 | | | Bottle No.: | 0264 |

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S


Signature: Tpc II J. Dellanoce # 6027

Badge No.: 6027

Date: 03/15/2010

*Black Key Temperature Probe Serial.....# DDWAP2-016 *gro*

*Digital NIST Temperature Measuring System Serial.....# 80637585 *gro*

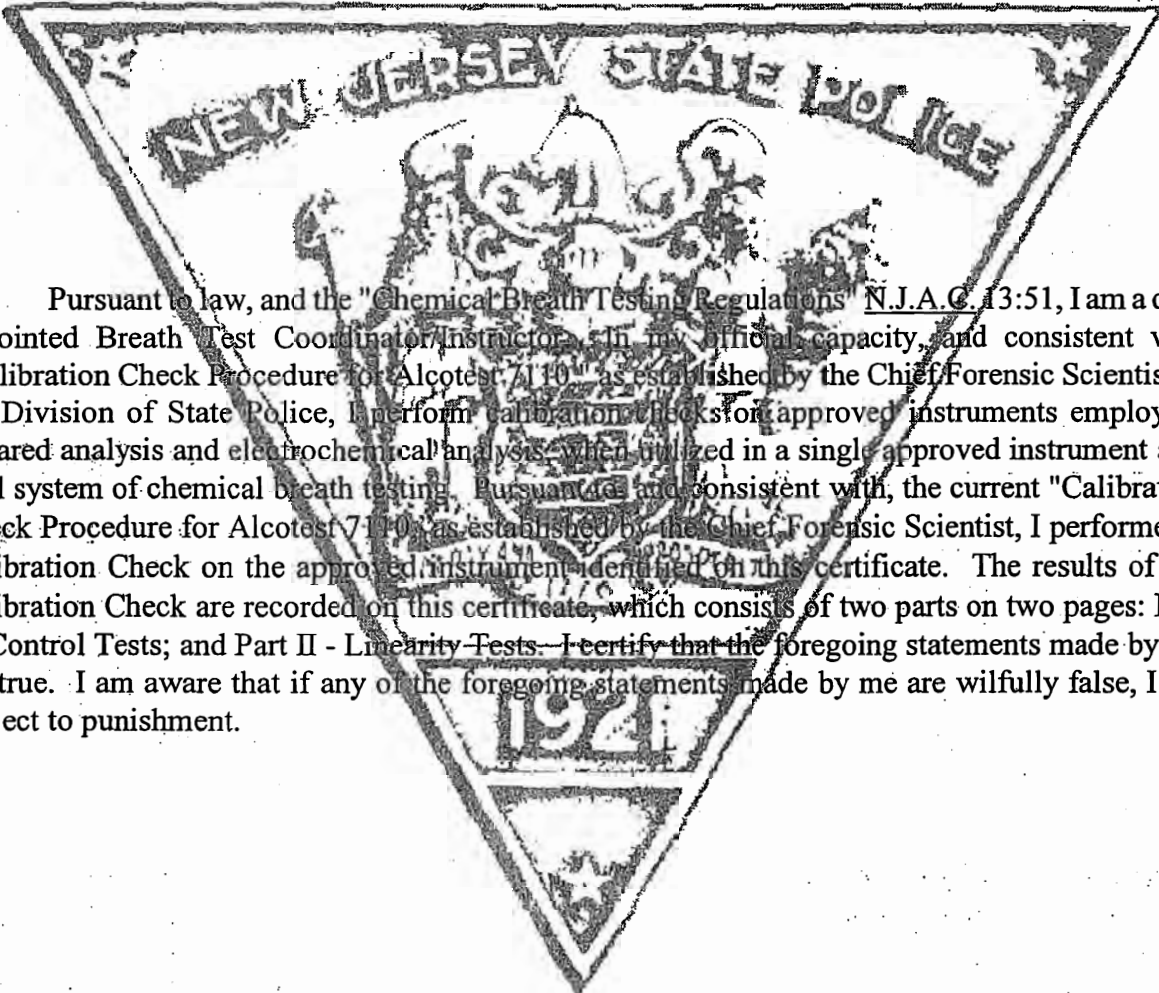

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

| | | |
|-------------------------|------------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARTL-0024 |
| Location: | BURLINGTON TOWNSHIP PD | |
| Calibration File No.: | 00490 | Calib. Date: 03/15/2010 |
| Certification File No.: | 00491 | Calib. No.: 00013 |
| Linearity File No.: | 00419 | Cert. Date: 03/15/2010 |
| Solution File No.: | 00488 | Cert. No.: 00008 |
| Sequential File No.: | 00491 | Lin. Date: 08/25/2009 |
| | | Lin. No.: 00007 |
| | | Soln. Date: 03/04/2010 |
| | | Soln. No.: 00078 |
| | | File Date: 03/15/2010 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUL S3-0167 |
| Solution Control Lot: | 09D065 | Expires: 04/22/2011 |
| | | Bottle No.: 0264 |


| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|-------------------------------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 10:29S 11:29 D _{9.5} | | |
| Control 1 EC | 0.099% | 10:29S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 10:29S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:30S | | |
| Control 2 EC | 0.100% | 10:30S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 10:30S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:31S | | |
| Control 3 EC | 0.100% | 10:31S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 10:31S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:32S 11:32 D _{9.0} | | |

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
 Signature: Tpr. J. Dellanoce #6027 Badge No: 6027 Date: 03/15/2010

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Inspector. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

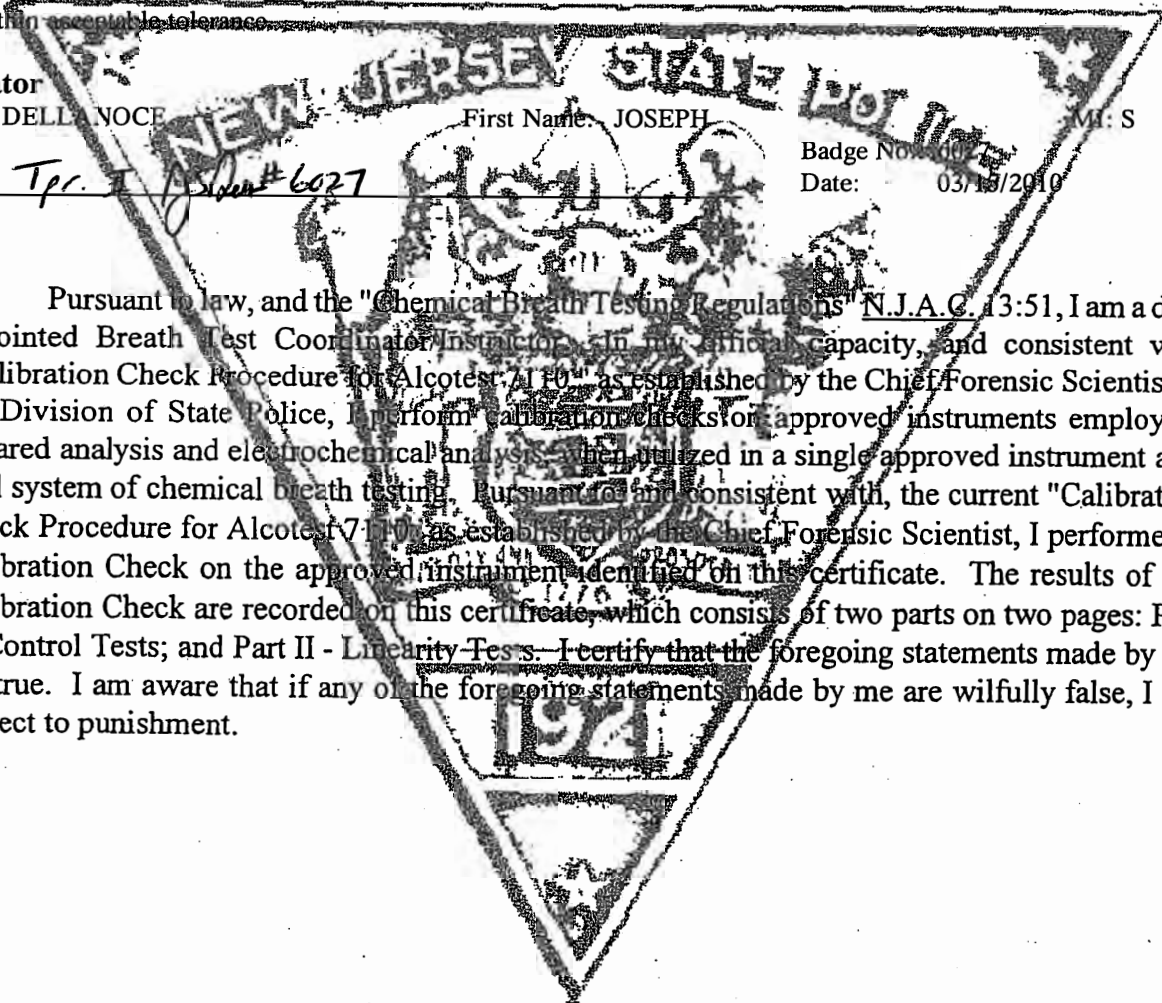

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00490 **Calib. Date:** 03/15/2010 **Calib. No.:** 00013
Certification File No.: 00491 **Cert. Date:** 03/15/2010 **Cert. No.:** 00008
Linearity File No.: 00492 **Lin. Date:** 03/15/2010 **Lin. No.:** 00008
Solution File No.: 00488 **Soln. Date:** 03/04/2010 **Soln. No.:** 00078
Sequential File No.: 00492 **File Date:** 03/15/2010

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0196
Control Solution %: 0.040% **Expires:** 06/26/2010
Solution Control Lot: 08F054 **Bottle No.:** 0092

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0203
Control Solution %: 0.080% **Expires:** 06/28/2010
Solution Control Lot: 08F055 **Bottle No.:** 0770

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0205
Control Solution %: 0.160% **Expires:** 07/07/2010
Solution Control Lot: 08G057 **Bottle No.:** 1213

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 10:48S | 34.0°C | |
| Control 1 EC | 0.041% | 10:49S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.041% | 10:49S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:50S | | |
| Control 2 EC | 0.041% | 10:50S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.041% | 10:50S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:52S | | |
| Control 3 EC | 0.081% | 10:52S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.080% | 10:52S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:53S | | |
| Control 4 EC | 0.081% | 10:54S | 34.0°C | *** TEST PASSED *** |
| Control 4 IR | 0.080% | 10:54S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:55S | | |
| Control 5 EC | 0.162% | 10:56S | 34.0°C | *** TEST PASSED *** |
| Control 5 IR | 0.161% | 10:56S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:57S | | |
| Control 6 EC | 0.162% | 10:58S | 34.0°C | *** TEST PASSED *** |
| Control 6 IR | 0.161% | 10:58S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:59S | | |

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: *Joseph Dellanoce* # 6027

Badge No.: 6027

Date: 03/15/2010

DEPARTMENT OF
Motor and Public Safety
 This is to certify that

Joseph S. Dellanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**
 A METHOD TO DETERMINE INTOXICATION.
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND Five



Joseph S. Dellanoce
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

Joseph S. Dellanoce
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| | DATE | Refresher Course PLACE | INSTRUCTOR |
|----|---------|---------------------------|----------------------|
| 1. | 2-15-07 | GC/PA | C. P. [unclear] |
| 2. | 12-7-09 | OL/PA | William S. [unclear] |
| 3. | | | |
| 4. | | | |
| 5. | | | |
| 6. | | | |
| 7. | | | |
| 8. | | | |
| 9. | | | |

S.P. 293B (Rev. 12/04)

DEPARTMENT OF
Public Safety
 This is to certify that
Joseph Ballanocce
 New Jersey State Police
 IS QUALIFIED AND COMPETENT TO INSTRUCT IN ALL ASPECTS PURSUANT TO CHAPTER
 143 OF THE LAWS OF 1944 IN THE OPERATION OF THE **Breathalyzer**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AND SEAL THIS 13th DAY OF Dec.
 TWO THOUSAND AND 01

 SUPERINTENDENT
 NEW JERSEY STATE POLICE

 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES: 8/30 - 9/3/99

Refresher Course

| | DATE | PLACE | INSTRUCTOR |
|----|----------|----------|------------|
| 1. | 12/12/01 | A.G.P.C. | ROTTOR |
| 2. | 2-9-03 | 66th | C. P. ... |
| 3. | 10-3-03 | ACTE | Ch. ... |
| 4. | | | |
| 5. | | | |
| 6. | | | |
| 7. | | | |
| 8. | | | |
| 9. | | | |

SP-293B (Rev. 4/00)

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-016

Certification date:

2-3-10

Next Certification due:

2-3-11

Probe Value

106

Draeger Safety Diagnostics, Inc.
Technical Service Department

mm



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

JON S. CORZINE
Governor

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/16/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F054

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0487 to 0.0493 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/25/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F055

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0977 to 0.0984 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 5/08/2009

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09D065

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1201 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 22, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of May, 2009.

Notary



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 07/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G057

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1956 to 0.1959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary

JOHN R. LEAVER
 NOTARY PUBLIC STATE OF NEW JERSEY
 MY COMMISSION EXPIRES 12/14/2012



Draeger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0196

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDWES3-0203

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11



Draeger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDWES3-0205

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11

Calibrating Unit

New Standard Solution Report

| | | | |
|-------------------------|------------------------|--------------|------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARTL-0024 |
| Location: | BURLINGTON TOWNSHIP PD | Calib. No.: | 00013 |
| Calibration File No.: | 00490 | Calib. Date: | 03/15/2010 |
| Certification File No.: | 00491 | Cert. Date: | 03/15/2010 |
| Linearity File No.: | 00492 | Lin. Date: | 03/15/2010 |
| Solution File No.: | 00493 | Soln. Date: | 03/15/2010 |
| Sequential File No.: | 00493 | File Date: | 03/15/2010 |

| | | | | | |
|-----------------------|--------|------------|------------|-------------|--------------|
| Calibrating Unit: | WET | Model No.: | CU-34 | Serial No.: | DDUL S3-0167 |
| Control Solution %: | 0.100% | Expires: | 12/31/2011 | Bottle No.: | 0669 |
| Solution Control Lot: | 09L072 | | | | |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|-----------------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 12:07S | 13:07 D ₉₀ | |
| Control 1 EC | 0.102% | 12:07S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 12:07S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:08S | | |
| Control 2 EC | 0.102% | 12:08S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.102% | 12:08S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:09S | | |
| Control 3 EC | 0.102% | 12:09S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.101% | 12:09S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 12:10S | 13:10 D ₉₀ | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDxAP2-011₉₀

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tr. II [Signature] #6027

Badge No.: 6027

Date: 03/15/2010



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 1/15/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09L072

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1203 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 31, 2011.

As the Director of Office of Forensic Sciences, Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Howard J. Baum, Ph.D.
 Director, Office of Forensic Sciences
 Division of State Police

Sworn to and subscribed before me this 21 day of January, 2010.

Notary

JOHN R. LEAVER
 NOTARY PUBLIC STATE OF NEW JERSEY
 MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable

