

ALCOTEST CHECKLIST

Municipality: BURLINGTON Twp. Alcotest Ser.#: ARTL-0024

County: BURLINGTON Date of Calibration: 07-05-2012

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDUL S3-0167

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDXA P2-011

4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 122172176

5. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDMB P1-0002

6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>11</u>	<u>F</u>	<u>090</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>11</u>	<u>F</u>	<u>091</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>10</u>	<u>I</u>	<u>082</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>11</u>	<u>G</u>	<u>092</u>

7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

A. 0.04% used in Calibration/Linearity Testing. DDWF S3-0215
 B. 0.08% used in Calibration/Linearity Testing. DDAE-0022
 C. 0.10% used in Calibration/Linearity Testing DDUL S3-0167 [Same as instrument's CU34 unit].
 D. 0.16% used in Calibration/Linearity Testing. DDWF S3-0241

8. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 11 G 093
 D. Alcotest card of operator/coordinator who completed change.

Dräger safety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48884 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

03/04/2000

ARTL-0024

Dräger Safety Diagnostics, Inc.



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DD4653-0167

Certification Date

Technician

Re-Certification Due Date

11/26/12

ZM

11/26/13

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDKA P2-011

11/26/12

11/26/13

Probe Value

1.03

Dräger Safety Diagnostics, Inc.
Technical Service Department

ZM



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Carl No.: 4000-4269885

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087
Instrument Identification:

Model: 81220-601 S/N: 122172176 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-275	A9A237		
Digital Thermometer	B18815	6/08/12	B1606038
PRT Temperature Probe	01841	6/28/12	B1625045
Temperature Calibration Bath TC-255	B01375		
Thermistor Module	A27129	10/31/12	1000308945
Temperature Probe	157	11/13/12	8-BL72N-1-1
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17116	2/01/13	1000311439
Temperature Probe	128	2/14/13	8-BN9WZ-27-1

Certificate Information:

Technician: 88 Procedure: CAL-06 Cal Date: 3/30/12 Cal Due: 3/30/14
Test Conditions: 23.0°C 44.0 %RH 1012 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.000	-0.001	Y	-0.050	0.050	0.019	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.014	3.8:1
°C		N.A.		80.000	80.000	Y	79.950	80.050	0.016	2.8:1
°C		N.A.		100.001	100.002	Y	99.951	100.051	0.018	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Minimum Standard Reading; As Left-Instrument Reading; In-Tol-In Tolerance; Min/Max-Applicable Range; ±U-Expanded Measurement Uncertainty; TUR-Test Uncertainty Ratio; Accuracy-(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date-MMDDYY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Brown
Wallace Brown, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change due, in any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4454 Rox Road Friendswood, TX 77641 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (ASLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-ANAS.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment

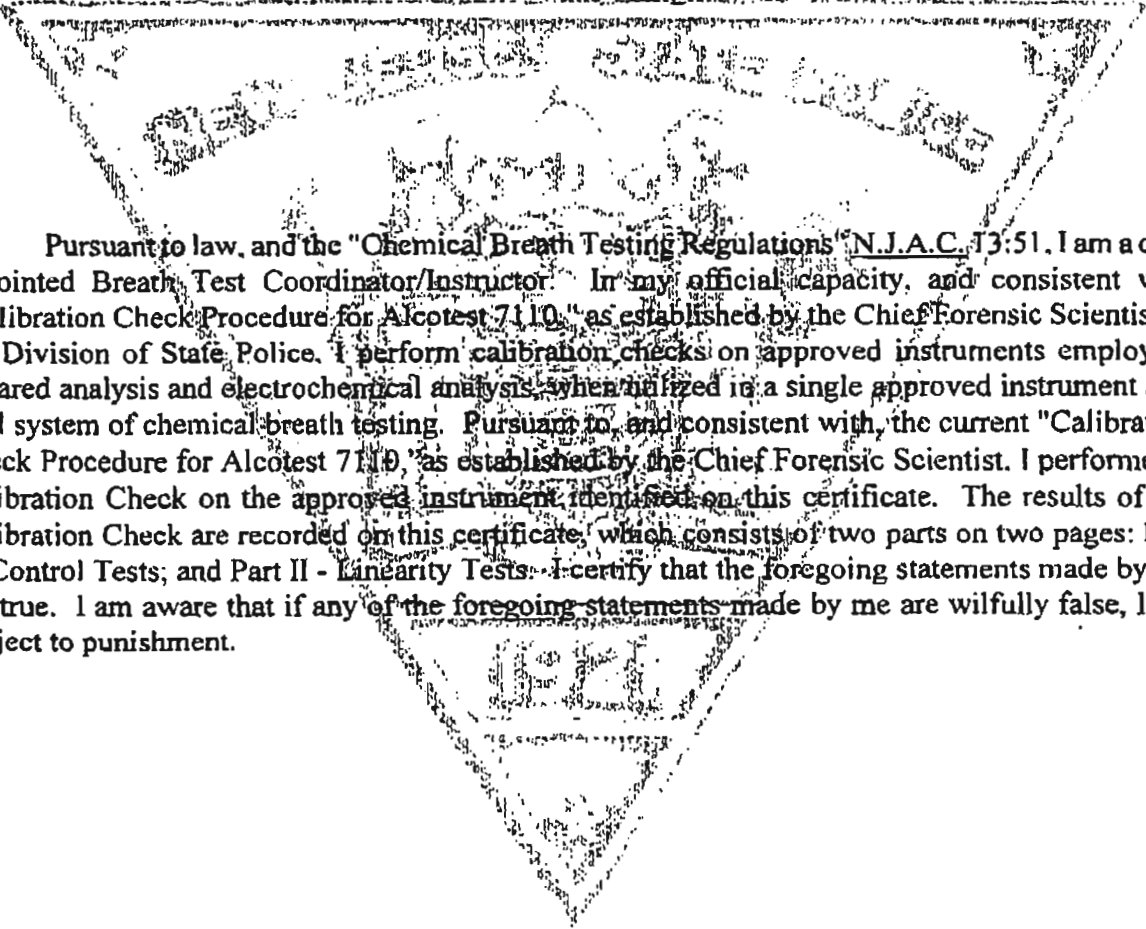
Alcotest 7110 MKIII-C
Location: BURLINGTON TOWNSHIP PD
Serial No.: ARTL-0024
Calibration File No.: 00769
Certification File No.: 00709
Linearity File No.: 00710
Solution File No.: 00765
Sequential File No.: 00769
Calib. Date: 07/05/2012
Cert. Date: 01/18/2012
Lin. Date: 01/18/2012
Soln. Date: 06/24/2012
File Date: 07/05/2012
Calib. No.: 00018
Cert. No.: 00012
Lin. No.: 00012
Soln. No.: 00114

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 101082
Model No.: CU-34
Serial No.: DDUL S3-0167
Expires: 09/09/2012
Bottle No.: 0451

Coordinator

Last Name: GONCALVES
First Name: MICHELLE
MI: L
Signature: Det I. Alves # 6040
Badge No.: 6040
Date: 07/05/2012

*Black Key Temperature Probe Serial.....# DDMB P1 - 0002 (NA)
*Digital NIST Temperature Measuring System Serial.....# 12212176 (NA)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00769 **Calib. Date:** 07/05/2012 **Calib. No.:** 00018
Certification File No.: 00770 **Cert. Date:** 07/05/2012 **Cert. No.:** 00013
Linearity File No.: 00710 **Lin. Date:** 01/18/2012 **Lin. No.:** 00012
Solution File No.: 00765 **Soln. Date:** 06/24/2012 **Soln. No.:** 00114
Sequential File No.: 00770 **File Date:** 07/05/2012

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0167
Control Solution %: 0.100% **Expires:** 09/09/2012
Solution Control Lot: 10I082 **Bottle No.:** 0451

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:30D		
Control 1 EC	0.099%	09:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	09:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31D		
Control 2 EC	0.100%	09:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32D		
Control 3 EC	0.100%	09:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		

All tests within acceptable tolerance.


Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature:



Badge No.: 6040

Date: 07/05/2012

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00769 **Calib. Date:** 07/05/2012 **Calib. No.:** 00018
Certification File No.: 00770 **Cert. Date:** 07/05/2012 **Cert. No.:** 00013
Linearity File No.: 00771 **Lin. Date:** 07/05/2012 **Lin. No.:** 00013
Solution File No.: 00765 **Soln. Date:** 06/24/2012 **Soln. No.:** 00114
Sequential File No.: 00771 **File Date:** 07/05/2012

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0215
Control Solution %: 0.040% **Expires:** 06/27/2013
Solution Control Lot: 11F090 **Bottle No.:** 0059

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDAE-0022
Control Solution %: 0.080% **Expires:** 06/30/2013
Solution Control Lot: 11F091 **Bottle No.:** 0896

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0241
Control Solution %: 0.160% **Expires:** 07/03/2013
Solution Control Lot: 11G092 **Bottle No.:** 0086

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:47D		
Control 1 EC	0.041%	09:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	09:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49D		
Control 2 EC	0.041%	09:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	09:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51D		
Control 3 EC	0.082%	09:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53D		
Control 4 EC	0.082%	09:53D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.081%	09:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55D		
Control 5 EC	0.162%	09:55D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.160%	09:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57D		
Control 6 EC	0.162%	09:57D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.160%	09:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59D		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature:

Det J Goncalves # 6040

Badge No.: 6040

Date: 07/05/2012



CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lieutenant Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF CRIMINAL JUSTICE
PO BOX 085
TRENTON, NJ 08625-0085
TELEPHONE: (609) 984-6300

JEFFREY S. CHIESA
Attorney General

STEPHEN J. TAYLOR
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C.* 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A.* 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police
DSFC Patrick Guilfoy, Unit Head, Alcohol/Drug Test Unit, Division of State Police ✓



DEPARTMENT OF
Traffic and Public Safety
Who is to certify that

Michelle L. McKelvey

IS QUALIFIED AND COMPETENT TO OPERATE A MOTOR VEHICLE IN ACCORDANCE WITH THE PROVISIONS OF CHAPTER 14B OF TITLE 17A OF THE STATUTES OF THE STATE OF NEW JERSEY AS AMENDED BY CHAPTER 110 OF THE STATUTES OF 1997 AND BY CHAPTER 110 OF THE STATUTES OF 2002 AND BY CHAPTER 110 OF THE STATUTES OF 2003 AND BY CHAPTER 110 OF THE STATUTES OF 2004 AND BY CHAPTER 110 OF THE STATUTES OF 2005 AND BY CHAPTER 110 OF THE STATUTES OF 2006 AND BY CHAPTER 110 OF THE STATUTES OF 2007 AND BY CHAPTER 110 OF THE STATUTES OF 2008 AND BY CHAPTER 110 OF THE STATUTES OF 2009 AND BY CHAPTER 110 OF THE STATUTES OF 2010 AND BY CHAPTER 110 OF THE STATUTES OF 2011 AND BY CHAPTER 110 OF THE STATUTES OF 2012 AND BY CHAPTER 110 OF THE STATUTES OF 2013 AND BY CHAPTER 110 OF THE STATUTES OF 2014 AND BY CHAPTER 110 OF THE STATUTES OF 2015 AND BY CHAPTER 110 OF THE STATUTES OF 2016 AND BY CHAPTER 110 OF THE STATUTES OF 2017 AND BY CHAPTER 110 OF THE STATUTES OF 2018 AND BY CHAPTER 110 OF THE STATUTES OF 2019 AND BY CHAPTER 110 OF THE STATUTES OF 2020 AND BY CHAPTER 110 OF THE STATUTES OF 2021 AND BY CHAPTER 110 OF THE STATUTES OF 2022 AND BY CHAPTER 110 OF THE STATUTES OF 2023

16th DAY OF AUGUST

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES Feb. 3-7-2003

Refresher Course

DATE	PLACE	INSTRUCTOR
1. 10/10/07	OCPTA	[Signature]
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2020 (Rev. 05/02)

DEPARTMENT OF
Traffic and Public Safety
Who is to certify that

MICHELLE L. MCKELVEY
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO OPERATE A MOTOR VEHICLE IN ACCORDANCE WITH THE PROVISIONS OF CHAPTER 14B OF TITLE 17A OF THE STATUTES OF THE STATE OF NEW JERSEY AS AMENDED BY CHAPTER 110 OF THE STATUTES OF 1997 AND BY CHAPTER 110 OF THE STATUTES OF 2002 AND BY CHAPTER 110 OF THE STATUTES OF 2003 AND BY CHAPTER 110 OF THE STATUTES OF 2004 AND BY CHAPTER 110 OF THE STATUTES OF 2005 AND BY CHAPTER 110 OF THE STATUTES OF 2006 AND BY CHAPTER 110 OF THE STATUTES OF 2007 AND BY CHAPTER 110 OF THE STATUTES OF 2008 AND BY CHAPTER 110 OF THE STATUTES OF 2009 AND BY CHAPTER 110 OF THE STATUTES OF 2010 AND BY CHAPTER 110 OF THE STATUTES OF 2011 AND BY CHAPTER 110 OF THE STATUTES OF 2012 AND BY CHAPTER 110 OF THE STATUTES OF 2013 AND BY CHAPTER 110 OF THE STATUTES OF 2014 AND BY CHAPTER 110 OF THE STATUTES OF 2015 AND BY CHAPTER 110 OF THE STATUTES OF 2016 AND BY CHAPTER 110 OF THE STATUTES OF 2017 AND BY CHAPTER 110 OF THE STATUTES OF 2018 AND BY CHAPTER 110 OF THE STATUTES OF 2019 AND BY CHAPTER 110 OF THE STATUTES OF 2020 AND BY CHAPTER 110 OF THE STATUTES OF 2021 AND BY CHAPTER 110 OF THE STATUTES OF 2022 AND BY CHAPTER 110 OF THE STATUTES OF 2023

10th DAY OF August

FIVE

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2020 (Rev. 05/02)

DEPARTMENT OF
Traffic and Public Safety
Who is to certify that

Michelle L. Gonçalves
New Jersey State Police

IS QUALIFIED AND COMPETENT TO OPERATE A MOTOR VEHICLE IN ACCORDANCE WITH THE PROVISIONS OF CHAPTER 14B OF TITLE 17A OF THE STATUTES OF THE STATE OF NEW JERSEY AS AMENDED BY CHAPTER 110 OF THE STATUTES OF 1997 AND BY CHAPTER 110 OF THE STATUTES OF 2002 AND BY CHAPTER 110 OF THE STATUTES OF 2003 AND BY CHAPTER 110 OF THE STATUTES OF 2004 AND BY CHAPTER 110 OF THE STATUTES OF 2005 AND BY CHAPTER 110 OF THE STATUTES OF 2006 AND BY CHAPTER 110 OF THE STATUTES OF 2007 AND BY CHAPTER 110 OF THE STATUTES OF 2008 AND BY CHAPTER 110 OF THE STATUTES OF 2009 AND BY CHAPTER 110 OF THE STATUTES OF 2010 AND BY CHAPTER 110 OF THE STATUTES OF 2011 AND BY CHAPTER 110 OF THE STATUTES OF 2012 AND BY CHAPTER 110 OF THE STATUTES OF 2013 AND BY CHAPTER 110 OF THE STATUTES OF 2014 AND BY CHAPTER 110 OF THE STATUTES OF 2015 AND BY CHAPTER 110 OF THE STATUTES OF 2016 AND BY CHAPTER 110 OF THE STATUTES OF 2017 AND BY CHAPTER 110 OF THE STATUTES OF 2018 AND BY CHAPTER 110 OF THE STATUTES OF 2019 AND BY CHAPTER 110 OF THE STATUTES OF 2020 AND BY CHAPTER 110 OF THE STATUTES OF 2021 AND BY CHAPTER 110 OF THE STATUTES OF 2022 AND BY CHAPTER 110 OF THE STATUTES OF 2023

25th DAY OF December

Eleven


[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2020 (Rev. 05/02)



CERTIFICATE

This is to certify that

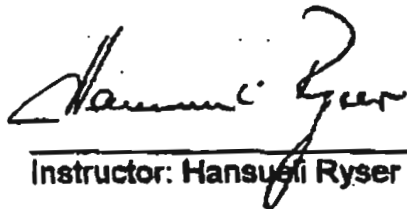
Michelle Goncalves

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012


Instructor: Hansueli Ryser

Dräger



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 West Trenton NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

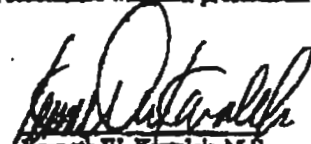
MANUFACTURER: Draeger Safety, Inc. ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11FD90

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Krawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.


 Notary

Linda S. Kellfontis
 Jersey Rules, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 West Trenton NJ 08628-0068
 (609) 883-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Dreyer Safety, Inc. ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11R091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kowalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.

Notary

Linda L. Demerillo
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WRST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

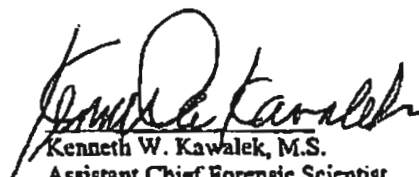
ANALYSIS DATE: 9/23/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 101082


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1190 to 0.1194 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 9, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 28th day of September, 2010.


 Notary

Linda L. Edwards
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7058
 West Trenton NJ 08628-0058
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

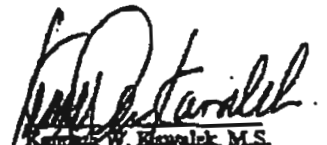
MANUFACTURER: Dynast Safety, Inc. ANALYSIS DATE: 7/25/2011


BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G092

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Howalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.

 Notary.

Linda L. Wharton
 Notary Public, State of New Jersey
 My Commission Expires: 9-11-14



New Jersey is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDAE-0022

Certification Date

Technician

Re-Certification Due Date

6/8/12

2M

6/8/13



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWES3-0215

Certification Date

Technician

Re-Certification Due Date

2/2/12

2M

2/2/13



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK II A

Other: _____

Serial Number:

DDWES3-0241

Certification Date

Technician

Re-Certification Due Date

2/2/12

ZM

2/2/13

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDMBPI-0002

2/3/12

2/3/13

Probe Value

102

Dräger Safety Diagnostics, Inc.
Technical Service Department

ZM

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00769	Calib. Date: 07/05/2012
Certification File No.:	00770	Calib. No.: 00018
Linearity File No.:	00771	Cert. Date: 07/05/2012
Solution File No.:	00772	Cert. No.: 00013
Sequential File No.:	00772	Lin. Date: 07/05/2012
		Lin. No.: 00013
		Soln. Date: 07/05/2012
		Soln. No.: 00115
		File Date: 07/05/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0167
Solution Control Lot:	11G093	Expires: 07/07/2013
		Bottle No.: 0873

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:05D		
Control 1 EC	0.103%	11:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		
Control 2 EC	0.101%	11:07D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		
Control 3 EC	0.101%	11:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number DDXAP2-011 MEL

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Det I Gals # 6040

Badge No.: 6040

Date: 07/05/2012



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE Box 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 7/28/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G093

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1200 to 0.1206 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.

Handwritten signature of Notary

Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

