

ALCOTEST CHECKLIST

Municipality: STRATFORD

Alcotest Ser. #: ARNK-0039

County: CAMDEN

Date of Calibration: 03-14-2023

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDUK S3-0133
3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDLL P1-0015
4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 221 473 067
5. **NIST - Traceable Digital Thermometer Readings.**
6.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDLA P3-0041
7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
 - A. 0.04% Solution. 21250
 - B. 0.08% Solution. 21260
 - C. 0.10% Solution. 21230
 - D. 0.16% Solution. 21290
8. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - A. 0.04% used in Calibration/Linearity Testing. DDAE-0017
 - B. 0.08% used in Calibration/Linearity Testing. DDWF S3-0225
 - C. 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.]
 - D. 0.16% used in Calibration/Linearity Testing. DDWF S3-0228
9.
 - A. New Standard Solution Report following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 22160
 - D. Alcotest card of operator/coordinator who completed change.

Edger

Alcotest® 7110 MKII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKII-C has been tested in accordance with the procedures set forth in the Alcotest 7110 MKII-C Accuracy Manual for a period of 12 months. The Alcotest 7110-C is certified as a "Truck" and "Tractor" unit with 0.05% and 0.10% BAC and 0.10% and 0.15% BAC. The operating parameters during calibration of 200 hours are within 12 hours of the calibration date listed, or within accuracy to your State regulations.

Calibration Date:
L-19-17

SERIAL NUMBER:
ARKK-0099

Edger Safety Diagnostics, Inc.

BC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDWKS3-0133

Certification Date:

11-11-22

Technician:

MB / DH

Re-Certification Due Date:

11-11-23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDLLP1-0015

Certification Date:

11-11-22

Next Certification Due:

11-11-23

Probe Value:

107

Draeger, Inc.

MB / DH



**Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001**



Cert. No.: 4000-13326328

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 221473067 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Temperature Probe	128	09 Jul 2022	15-D4F0Q-40-1
Thermistor Module	A17118	08 Jul 2022	1000469276
Temperature Calibration Bath	A45240		
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Thermistor Module	B96381	18 Aug 2022	1000470702
Temperature Probe	5392	04 Aug 2022	4500006080
Temperature Probe	5398	24 Aug 2022	4500006081
Thermistor Module	B96382	08 Oct 2022	1000472708
Temperature Probe	5410	20 Oct 2022	4500006780

Certificate Information:

Technician: 299 Procedure: CAL-06 Cal Date: 25 Apr 2022 Cal Due Date: 25 Apr 2024
 Test Conditions: 58.46%RH 23.43°C 1017mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	-0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.000	25.001	Y	24.95	25.05	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.001	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		100.001	100.003	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max=As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez
 Nicol Rodriguez, Quality Manager

Marisa Elms
 Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com**

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-ANAB.
 International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-13326328

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 25 Apr 2022

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by ONV GL, Certificate No. CERT-01805-2006-AQ-HOU-AWAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Sgt. Matthew R. Watson
Name

7078
Badge No.

Location:

Stratford Police Dept.
Agency

ARNK-0039
Alcotest Serial No.

Equipment:

221473067
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDAE-0017	11:54 ⁰ (MW)	12:55 ⁰ (MW)	33.9°c
0.08%	DDWF 53-0225	11:54 ⁰ (MW)	12:56 ⁰ (MW)	34.0°c
0.10%	DDUK 53-0133	11:54 ⁰ (MW)	12:58 ⁰ (MW)	33.9°c
0.16%	DDWF 53-0228	11:54 ⁰ (MW)	12:59 ⁰ (MW)	33.9°c

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius ± 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.


Sgt. Matthew R. Watson #7078
Coordinator's Signature

03/14/2023
Date


Alcotest 7110 Calibration Record

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	03107	Calib. Date:	03/14/2023
Certification File No.:	03079	Calib. No.:	00050
Linearity File No.:	03080	Cert. Date:	10/13/2022
Solution File No.:	03104	Cert. No.:	00039
Sequential File No.:	03107	Lin. Date:	10/13/2022
		Lin. No.:	00038
		Soln. Date:	02/14/2023
		Soln. No.:	00369
		File Date:	03/14/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	21230	Expires:	06/23/2023
		Bottle No.:	1370

Coordinator

Last Name: WATSON First Name: MATTHEW MI: R
Signature: Sgt.  #7078 Badge No.: 7078
Date: 03/14/2023

*Black Key Temperature Probe Serial.....# DDLAP3-0041 MRW
*Digital NIST Temperature Measuring System Serial.....# 221473067 MRW

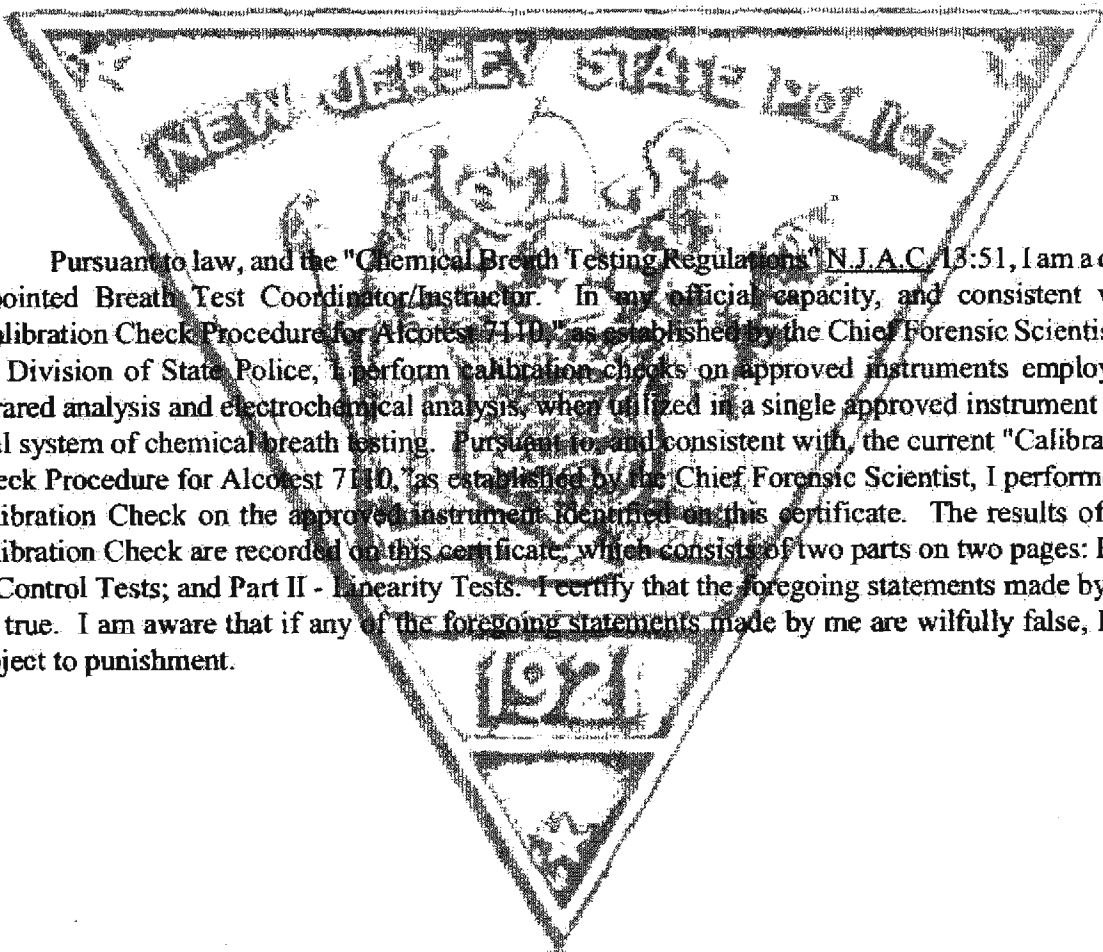

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	03107	Calib. Date: 03/14/2023
Certification File No.:	03108	Calib. No.: 00050
Linearity File No.:	03080	Cert. Date: 03/14/2023
Solution File No.:	03104	Cert. No.: 00040
Sequential File No.:	03108	Lin. Date: 10/13/2022
		Lin. No.: 00038
		Soln. Date: 02/14/2023
		Soln. No.: 00369
		File Date: 03/14/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	21230	Expires: 06/23/2023
		Bottle No.: 1370

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:06S	13:060 MW	
Control 1 EC	0.100%	12:06S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		
Control 2 EC	0.099%	12:08S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:09S		
Control 3 EC	0.099%	12:09S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:09S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:10S	13:100 MW	

All tests within acceptable tolerance.


Coordinator

Last Name: WATSON First Name: MATTHEW MI: R

Signature: Sgt. Matthew Watson

Badge No.: 7078
Date: 03/14/2023

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

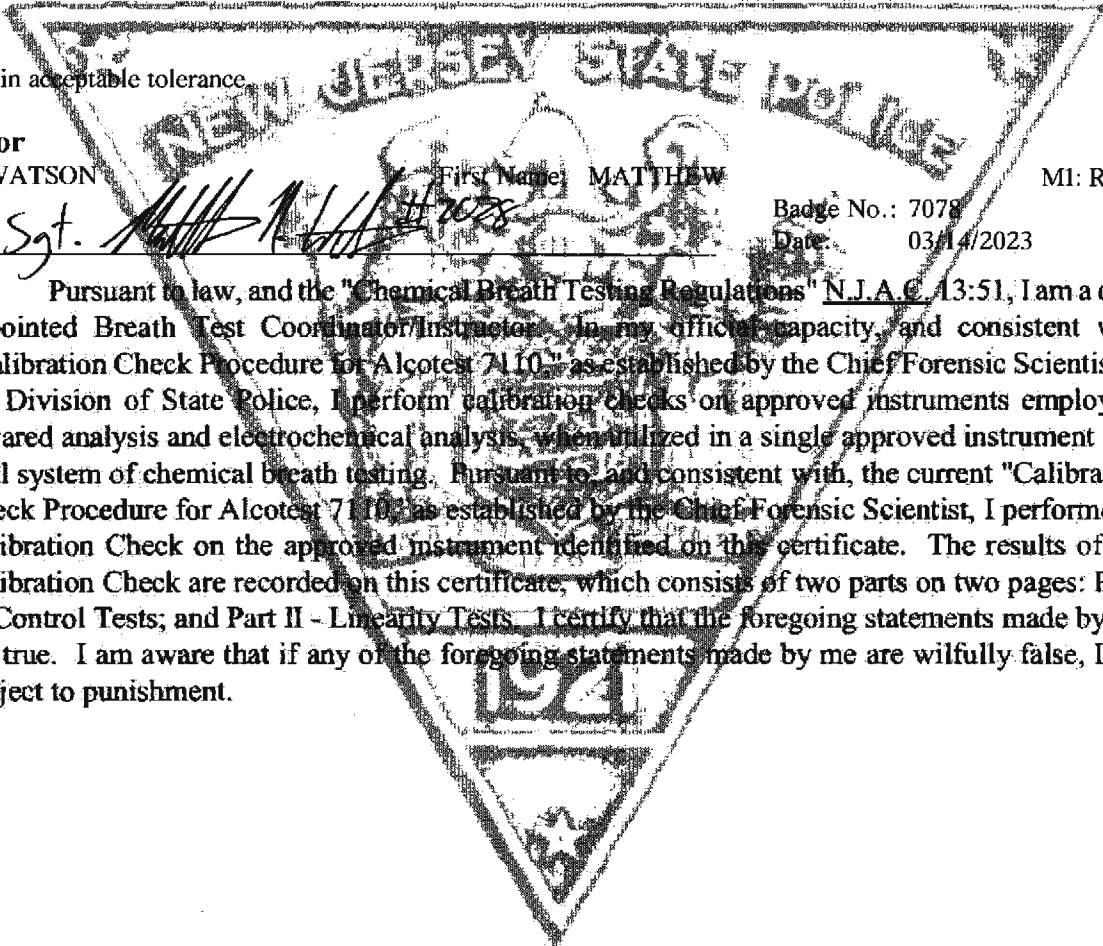

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 03107 Calib. Date: 03/14/2023 Calib. No.: 00050
Certification File No.: 03108 Cert. Date: 03/14/2023 Cert. No.: 00040
Linearity File No.: 03109 Lin. Date: 03/14/2023 Lin. No.: 00039
Solution File No.: 03104 Soln. Date: 02/14/2023 Soln. No.: 00369
Sequential File No.: 03109 File Date: 03/14/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0017
Control Solution %: 0.040% Expires: 07/06/2023
Solution Control Lot: 21250 Bottle No.: 1199

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0225
Control Solution %: 0.080% Expires: 07/19/2023
Solution Control Lot: 21260 Bottle No.: 0342

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0228
Control Solution %: 0.160% Expires: 07/29/2023
Solution Control Lot: 21290 Bottle No.: 0950

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:20S	33.9°C	MW
Control 1 EC	0.041%	12:21S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	12:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22S		
Control 2 EC	0.041%	12:23S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.042%	12:23S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:25S		
Control 3 EC	0.083%	12:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.083%	12:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:27S		
Control 4 EC	0.081%	12:28S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.083%	12:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29S		
Control 5 EC	0.163%	12:30S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.164%	12:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:31S		
Control 6 EC	0.162%	12:32S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.163%	12:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34S	33.9°C	MW


All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: Sgt.  #2078

Badge No.: 7078

Date: 03/14/2023

DEPARTMENT OF
Traffic and Public Safety
State is to certify that

Matthew R. Wilson
New Jersey Police



IS QUALIFIED AND COMPETENT TO INSTRUCT IN THE OPERATION OF A BREATH TEST INSTRUMENT IN ACCORDANCE WITH CHAPTER 100 OF THE LAWS OF 1964 BY THE OPERATOR OF A MOTOR VEHICLE IN THE STATE OF NEW JERSEY IN ACCORDANCE WITH SECTION 7110 MKIII-C

DAY OF August

THE YEAR AND 1982

[Signature]
SUPERVISOR
NEW JERSEY STATE POLICE

[Signature]
ACTING ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-8-12	GCPA	Wm Lass
2. 7/14/15	CAAPA	Adam Gaudin
3. 3/23/17	Lakehurst	Michelle Lincoln
4. 9-20-19	GCPA	Wm Lass
5. 11/09/21	GCPA	Wm Lass
6.		
7.		
8.		
9.		
10.		

S.P. 2000 (Rev. 01/78)

DEPARTMENT OF
Traffic and Public Safety
State is to certify that

Matthew R. Wilson
Breath Test Coordinator/Instructor



IS QUALIFIED AND COMPETENT TO COORDINATE AND INSTRUCT IN THE OPERATION OF A BREATH TEST INSTRUMENT IN ACCORDANCE WITH CHAPTER 100 OF THE LAWS OF 1964 BY THE OPERATOR OF A MOTOR VEHICLE IN THE STATE OF NEW JERSEY IN ACCORDANCE WITH SECTION 7110 MKIII-C

DAY OF June

THE YEAR AND Sixteen

[Signature]
SUPERVISOR
NEW JERSEY STATE POLICE

[Signature]
ACTING ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		
10.		

S.P. 2000 (Rev. 01/78)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 06, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.

Notary 

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110622
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURDIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.


ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0970 to 0.0977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.

Notary 

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110622
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/08/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1200 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 23, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of July, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110822
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor
SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General
PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/11/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1945 to 0.1977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 29, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of August, 2021.

Notary signature

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110622
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDAE-0017

Certification Date:

Technician:

Re-Certification Due Date:

2/10/2023

TM/MB

2/10/2024

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDWFS3-0225

Certification Date:

Technician:

Re-Certification Due Date:

6-15-22

MB

6-15-23

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDWF53-0228

Certification Date:

Technician:

Re-Certification Due Date:

2/17/2023

TM/MB

2/17/2024

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDLAP3-0041

2-24-23

2-24-24

Probe Value:

103

Dräger, Inc.

DH/4

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 03107 Calib. Date: 03/14/2023 Calib. No.: 00050
Certification File No.: 03108 Cert. Date: 03/14/2023 Cert. No.: 00040
Linearity File No.: 03109 Lin. Date: 03/14/2023 Lin. No.: 00039
Solution File No.: 03110 Soln. Date: 03/14/2023 Soln. No.: 00370
Sequential File No.: 03110 File Date: 03/14/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 05/09/2024
Solution Control Lot: 22160 Bottle No.: 1418

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:38S 14:38 ₀	MW	
Control 1 EC	0.101%	13:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:40S		
Control 2 EC	0.100%	13:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41S		
Control 3 EC	0.101%	13:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	13:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:43S 14:43 ₀	MW	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDLLP1-0015 (MRW)

Changed By:

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: Sgt. Matthew R. Watson #7078

Badge No.: 7078

Date: 03/14/2023



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 05/23/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22160

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is May 9, 2024.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 26 day of May, 2022.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

