

# ALCOTEST CHECKLIST

Municipality: STRATFORD

Alcotest Ser.#: ARNK-0039

County: CAMDEN

Date of Calibration: 07-22-2020

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.  
Ser. #: DDUK 53-0133

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.  
Ser. #: DDL PI-0015

4. **Digital Temperature Measuring System Report of Calibration.**  
Ser. #: 191957 498

5. **NIST - Traceable Digital Thermometer Readings.**

6.  A. Alcotest 7110 Calibration Record  
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**  
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**  
 D. **Alcotest Card** of operator/coordinator who performed tests.  
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].  
Ser. #: DDLH PI-0079

7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>19310</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>19320</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>19270</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>19360</u>

8. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

<input checked="" type="checkbox"/> A.	0.04% used in Calibration/Linearity Testing.	<u>DDAE-0016</u>
<input checked="" type="checkbox"/> B.	0.08% used in Calibration/Linearity Testing.	<u>DDMK 53-0003</u>
<input checked="" type="checkbox"/> C.	0.10% used in Calibration/Linearity Testing. [Same as CU34 unit on instrument.]	
<input checked="" type="checkbox"/> D.	0.16% used in Calibration/Linearity Testing.	<u>DDYA 53-0004</u>

9.  A. New Standard Solution Report following Calibration.  
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].  
 C. Certificate of Analysis 0.10% solution for same.  
Lot #: 19150  
 D. Alcotest card of operator/coordinator who completed change.

**Dräger**

**Alcotest® 7110 MKII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKII-C is compliant with "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 50 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

1-19-17

SERIAL NUMBER:

AKISK-0039

Draeger Safety Diagnostics, Inc.

BC

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDUKS3-0133

Certification Date:

3-19-20

Technician:

[Signature]

Re-Certification Due Date:

3-19-21

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.  
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDLL P1-0015

Certification Date:

3-20-20

Next Certification Due:

3-20-21

Probe Value:

105

Dräger, Inc.

[Signature]



Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10176223

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: WVR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Malsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 191957498 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	20 Apr 2019	1000424560
Thermistor Module	A27129	10 Jan 2020	1000436202
Temperature Calibration Bath	A73332		
Temperature Probe	3039	08 May 2019	6-B7F4L-20-1
Temperature Calibration Bath	A79341		
Temperature Probe	5394	29 Jan 2020	B9124038
Temperature Calibration Bath	B16388		
Temperature Probe	5267	28 Jan 2020	B9124036

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 13 Feb 2019 Cal Due Date: 13 Feb 2021  
 Test Conditions: 37.61%RH 23.29°C 1026mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	0.001	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.000	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.001	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.002	99.999	Y	99.952	100.052	0.0087	>4:1

This certificate indicates traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max=As Left Nominal(Rounded) + Tolerance;

*Nicol Rodriguez*

Nicol Rodriguez, Quality Manager

*Adam J. ...*

Adam J. ... Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598  
 Phone 281 482-1714 Fax 281 482-8448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
 Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RuA.  
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10176223

**Traceable® Certificate of Calibration for Digital Thermometer**

---

**CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598**  
**Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com**

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
 Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-RuA.  
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

**Alcotest 7110 MKIII-C Calibration  
NIST-Traceable Digital Thermometer Readings**

**Coordinator:**

TPA-I Brian M. Gambone  
Name

7029  
Badge No.

**Location:**

Stratford Police Dept.  
Agency

ARNK-0039  
Alcotest Serial No.

**Equipment:**

191957498  
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDAE-0016	08:09 D	09:11 D	34.0°C
0.08%	DDMM 53-0003	08:09 D	09:12 D	34.0°C
0.10%	DDMK 53-0133	08:09 D	09:13 D	34.0°C
0.16%	DDYA 53-0004	08:09 D	09:14 D	34.0°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius  $\pm$  0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

TPA-I B M Gambone #7029  
Coordinator's Signature

7/22/2020  
Date

# Alcotest 7110 Calibration Record

## Equipment

Alcotest 7110 MKIII-C  
Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 02839 Calib. Date: 07/22/2020 Calib. No.: 00044  
Certification File No.: 02825 Cert. Date: 03/12/2020 Cert. No.: 00033  
Linearity File No.: 02826 Lin. Date: 03/12/2020 Lin. No.: 00032  
Solution File No.: 02838 Soln. Date: 07/09/2020 Soln. No.: 00328  
Sequential File No.: 02839 File Date: 07/22/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/14/2021  
Solution Control Lot: 19270 Bottle No.: 0288

## Coordinator


Last Name: GAMBONE First Name: BRIAN MI: M

Signature: TPR. I Brian Gambone #7029 Badge No.: 7029  
Date: 07/22/2020

\*Black Key Temperature Probe Serial.....# DDLHPI-0079 **(BMG)**

\*Digital NIST Temperature Measuring System Serial.....# 191957498 **(BMG)**

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

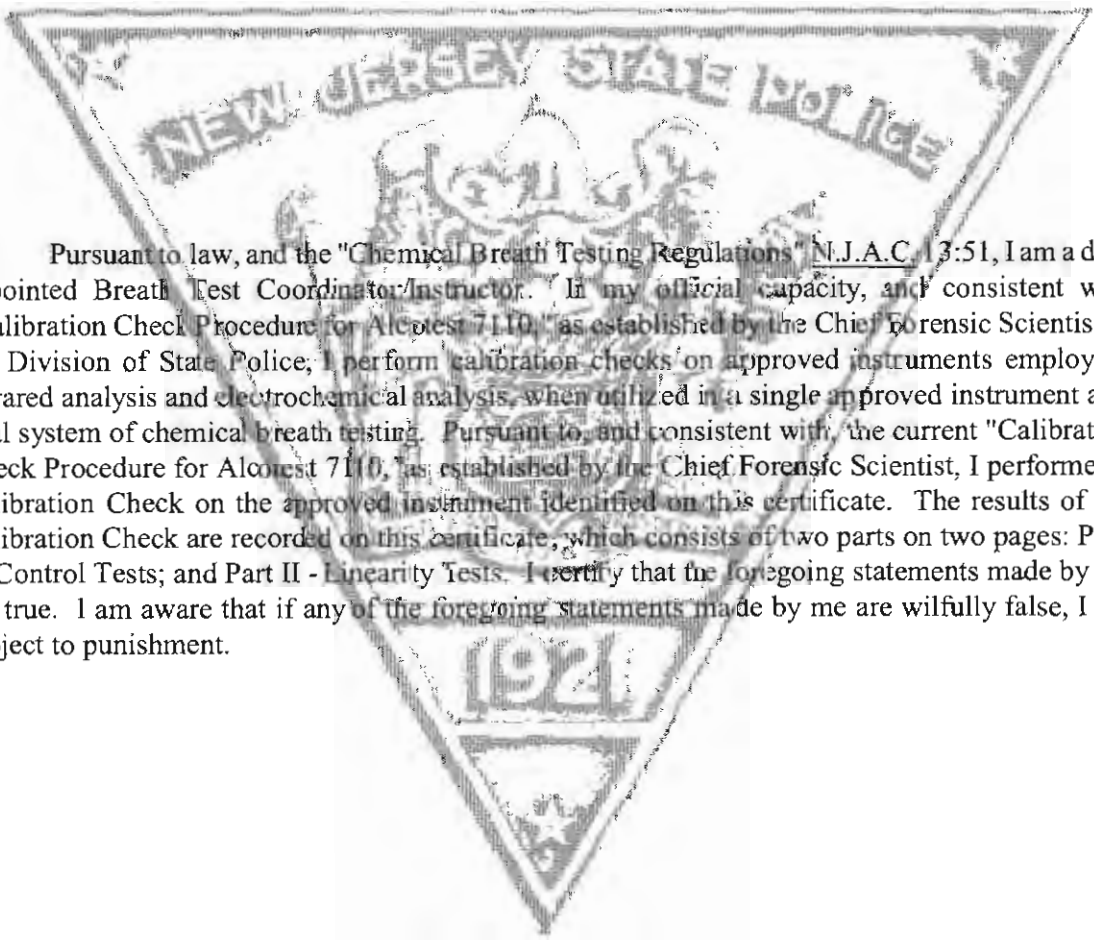

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 02839 Calib. Date: 07/22/2020 Calib. No.: 00044  
Certification File No.: 02840 Cert. Date: 07/22/2020 Cert. No.: 00034  
Linearity File No.: 02826 Lin. Date: 03/12/2020 Lin. No.: 00032  
Solution File No.: 02838 Soln. Date: 07/09/2020 Soln. No.: 00328  
Sequential File No.: 02840 File Date: 07/22/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 10/14/2021  
Solution Control Lot: 19270 Bottle No.: 0288

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:39D		
Control 1 EC	0.100%	09:40D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		
Control 2 EC	0.099%	09:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42D		
Control 3 EC	0.099%	09:43D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		

All tests within acceptable tolerance.

### Coordinator

Last Name: GAMBONE

First Name: BRIAN

MI: M

Badge No.: 7029

Signature: TPR. I BGM

Date: 07/22/2020

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.



# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 02839 Calib. Date: 07/22/2020 Calib. No.: 00044  
Certification File No.: 02840 Cert. Date: 07/22/2020 Cert. No.: 00034  
Linearity File No.: 02841 Lin. Date: 07/22/2020 Lin. No.: 00033  
Solution File No.: 02838 Soln. Date: 07/09/2020 Soln. No.: 00328  
Sequential File No.: 02841 File Date: 07/22/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0016  
Control Solution %: 0.040% Expires: 11/04/2021  
Solution Control Lot: 19310 Bottle No.: 1461

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0003  
Control Solution %: 0.080% Expires: 11/11/2021  
Solution Control Lot: 19320 Bottle No.: 0333

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDYA S3-0004  
Control Solution %: 0.160% Expires: 12/02/2021  
Solution Control Lot: 19360 Bottle No.: 1365

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:07D		
Control 1 EC	0.041%	10:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	10:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09D		
Control 2 EC	0.041%	10:10D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	10:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:11D		
Control 3 EC	0.082%	10:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	10:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13D		
Control 4 EC	0.080%	10:14D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.081%	10:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:15D		
Control 5 EC	0.162%	10:16D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.162%	10:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:18D		
Control 6 EC	0.161%	10:18D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.161%	10:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		

All tests within acceptable tolerance.

### Coordinator

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature:  # 7029

Badge No.: 7029

Date: 07/22/2020

DEPARTMENT OF  
**Traffic and Public Safety**  
Wishes to be certified that

**Brian M. Gambone**  
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL TESTING AND IS THE PURSUANT TO A TRAINING COURSE OF THE LAWS OF THE STATE OF NEW YORK AND IS THE PURSUANT TO A TRAINING COURSE OF THE LAWS OF THE STATE OF NEW YORK.

A METHOD TO DETERMINE BLOOD ALCOHOL CONCENTRATION UNDERSTANDS BY BOARD AT TOWNSHIRE, NEW YORK, THIS 20 DAY OF October

THIS INSTRUMENT AND Exhibits

*[Signature]*  
NEW YORK STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW YORK

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
11/19/18	GCEA	Adam Stender
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 9/14)

DEPARTMENT OF  
**Traffic and Public Safety**  
Wishes to be certified that

**Brian M. Gambone**  
New York State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL TESTING AND IS THE PURSUANT TO A TRAINING COURSE OF THE LAWS OF THE STATE OF NEW YORK AND IS THE PURSUANT TO A TRAINING COURSE OF THE LAWS OF THE STATE OF NEW YORK.

A METHOD TO DETERMINE BLOOD ALCOHOL CONCENTRATION UNDERSTANDS BY BOARD AT TOWNSHIRE, NEW YORK, THIS 15th DAY OF July

THIS INSTRUMENT AND Ten

*[Signature]*  
NEW YORK STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW YORK

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1/27/17	GCPA	Wm Linn
11/4/14	GCPA	Adam Stender
6/4/16	CMPT	Adam Stender
11/19/18	GCEA	Adam Stender
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 03/16)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/14/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19310

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 04, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of November, 2019.

Notary [Signature]

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110622
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor
SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General
PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19320

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0971 to 0.0985 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of November, 2019.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110822
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/21/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1232 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 14, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60140522
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 12/11/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1956 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 02, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of December, 2019.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDAE - 0016

Certification Date:

3.10.20

Technician:

Om

Re-Certification Due Date:

3.10.21

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDMK53-0003

Certification Date:

3.9.20

Technician:

Om

Re-Certification Due Date:

3.9.21

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDYAS3-0004

Certification Date:

3.10.20

Technician:

DA

Re-Certification Due Date:

3.10.21

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDLHP1-0079

Certification Date:

3.11.20

Next Certification Due:

3.11.21

Probe Value:

106

Draeger, Inc.

[Signature]



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02839	Calib. Date: 07/22/2020
Certification File No.:	02840	Cert. No.: 00044
Linearity File No.:	02841	Cert. Date: 07/22/2020
Solution File No.:	02842	Lin. Date: 07/22/2020
Sequential File No.:	02842	Lin. No.: 00033
		Soln. Date: 07/22/2020
		Soln. No.: 00329
		File Date: 07/22/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	19150	Expires: 06/10/2021
		Bottle No.: 0215

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:25D		
Control 1 EC	0.101%	11:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:27D		
Control 2 EC	0.100%	11:27D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:28D		
Control 3 EC	0.100%	11:29D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDLLPI-0015

**BMG**

**Changed By:**

Last Name: GAMBONE

First Name: BRIAN

MI: M

Signature: TPA. I B M #7029

Badge No.: 7029

Date: 07/22/2020



# State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

PHILIP D. MURPHY  
*Governor*

SHEILA Y. OLIVER  
*Lt. Governor*

GURBIR S. GREWAL  
*Attorney General*

PATRICK J. CALLAHAN  
*Colonel*

## CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.

**ANALYSIS DATE:** 06/20/2019


**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 19150

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 10, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Michael Kennedy*  
Michael Kennedy  
Assistant Chief Forensic Scientist  
NJSP Office of Forensic Sciences

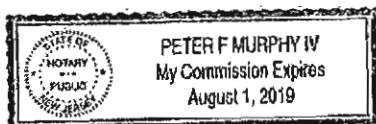

Sworn to and subscribed before me this 26<sup>th</sup> day of June, 2019.

*[Signature]*  
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable

