

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0038
Location:	EASTAMPTON TOWNSHIP		
Calibration File No.:	00377	Calib. Date:	04/11/2013
Certification File No.:	00378	Cert. Date:	04/11/2013
Linearity File No.:	00379	Lin. Date:	04/11/2013
Solution File No.:	00408	Soln. Date:	09/29/2013
Sequential File No.:	00408	File Date:	09/29/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0130
Solution Control Lot:	12A097	Expires:	01/05/2014
		Bottle No.:	0268

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:31D		
Control 1 EC	0.099%	05:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:32D		
Control 2 EC	0.099%	05:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:34D		
Control 3 EC	0.099%	05:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHEPARD

First Name: DENNIS

MI:

Signature: _____



Badge No.: 3436

Date: 09/29/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0038
Location:	EASTAMPTON TOWNSHIP		
Calibration File No.:	00377	Cal No.:	00018
Certification File No.:	00378	Ce No.:	00015
Linearity File No.:	00379	Lir No.:	00015
Solution File No.:	00407	So No.:	00125
Sequential File No.:	00407	File	
Calibrating Unit:	WET	M No.:	DDUK S3-0130
Control Solution %:	0.100%	s:	01/05/2014
Solution Control Lot:	12A097	Bottle No.:	0265

DO NOT
SEND

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:01D		
Control 1 EC	-.---%	01:02D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	01:02D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHEPARD

First Name: DENNIS

MI: E

Signature: 

Badge No.: 3436

Date: 09/29/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0038
Location:	EASTAMPTON TOWNSHIP	
Calibration File No.:	00377	Calib. Date: 04/11/2013
Certification File No.:	00378	Calib. No.: 00018
Linearity File No.:	00379	Cert. Date: 04/11/2013
Solution File No.:	00404	Cert. No.: 00015
Sequential File No.:	00404	Lin. Date: 04/11/2013
		Lin. No.: 00015
		Soln. Date: 09/01/2013
		Soln. No.: 00124
		File Date: 09/01/2013

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0130
Control Solution %:	0.100%		Expires: 01/05/2014
Solution Control Lot:	12A097		Bottle No.: 0269

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:26D		
Control 1 EC	0.095%	20:27D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	20:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:28D		
Control 2 EC	0.096%	20:28D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	20:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:29D		
Control 3 EC	0.096%	20:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	20:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SHEPARD

First Name: DENNIS

MI: E

Signature: _____



Badge No.: 3436

Date: 09/01/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0038
Location:	EASTAMPTON TOWNSHIP	
Calibration File No.:	00377	Calib. Date: 04/11/2013
Certification File No.:	00378	Calib. No.: 00018
Linearity File No.:	00379	Cert. Date: 04/11/2013
Solution File No.:	00397	Cert. No.: 00015
Sequential File No.:	00397	Lin. Date: 04/11/2013
		Lin. No.: 00015
		Soln. Date: 08/03/2013
		Soln. No.: 00123
		File Date: 08/03/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0130
Solution Control Lot:	12A097	Expires: 01/05/2014
		Bottle No.: 0255

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:29D		
Control 1 EC	0.100%	20:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:31D		
Control 2 EC	0.100%	20:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:32D		
Control 3 EC	0.099%	20:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MUSSER

First Name: MICHAEL

MI: D

Signature: _____

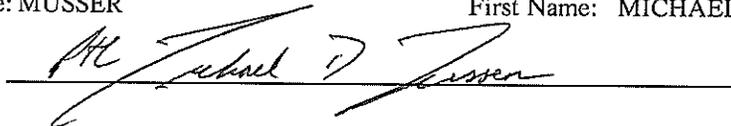

Badge No.: 3409

Date: 08/03/2013

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0038
Location:	EASTAMPTON TOWNSHIP	
Calibration File No.:	00377	Calib. Date: 04/11/2013
Certification File No.:	00378	Cert. Date: 04/11/2013
Linearity File No.:	00379	Lin. Date: 04/11/2013
Solution File No.:	00394	Soln. Date: 07/03/2013
Sequential File No.:	00394	File Date: 07/03/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0130
Solution Control Lot:	12A097	Expires: 01/05/2014
		Bottle No.: 0257

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:40D		
Control 1 EC	0.100%	20:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:42D		
Control 2 EC	0.100%	20:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:43D		
Control 3 EC	0.099%	20:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GRAHAM

First Name: PTL

MI: D

Signature: _____

[Handwritten Signature]
#3416

Badge No.: 3416

Date: 07/03/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0038
Location:	EASTAMPTON TOWNSHIP	
Calibration File No.:	00377	Calib. Date: 04/11/2013
Certification File No.:	00378	Calib. No.: 00018
Linearity File No.:	00379	Cert. Date: 04/11/2013
Solution File No.:	00387	Cert. No.: 00015
Sequential File No.:	00387	Lin. Date: 04/11/2013
		Lin. No.: 00015
		Soln. Date: 06/04/2013
		Soln. No.: 00121
		File Date: 06/04/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0130
Solution Control Lot:	12A097	Expires: 01/05/2014
		Bottle No.: 0272

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:16D		
Control 1 EC	0.099%	17:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	17:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:18D		
Control 2 EC	0.099%	17:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:19D		
Control 3 EC	0.097%	17:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHEPARD

First Name: DENNIS

MI: E

Signature: 

Badge No.: 3412

Date: 06/04/2013

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0038
Location: EASTAMPTON TOWNSHIP
Calibration File No.: 00377 Calib. Date: 04/11/2013 Calib. No.: 00018
Certification File No.: 00378 Cert. Date: 04/11/2013 Cert. No.: 00015
Linearity File No.: 00379 Lin. Date: 04/11/2013 Lin. No.: 00015
Solution File No.: 00385 Soln. Date: 05/10/2013 Soln. No.: 00120
Sequential File No.: 00385 File Date: 05/10/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0130
Control Solution %: 0.100% Expires: 01/05/2014
Solution Control Lot: 12A097 Bottle No.: 0270

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:46D		
Control 1 EC	0.098%	08:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:48D		
Control 2 EC	0.096%	08:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49D		
Control 3 EC	0.096%	08:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHEPARD

First Name: DENNIS

MI: E

Signature: 

Badge No.: 3412

Date: 05/10/2013


Alcotest 7110 Calibration Record

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0038
Location:	EASTAMPTON TOWNSHIP		
Calibration File No.:	00377	Calib. Date:	04/11/2013
Certification File No.:	00360	Cert. Date:	11/15/2012
Linearity File No.:	00361	Lin. Date:	11/15/2012
Solution File No.:	00376	Soln. Date:	04/09/2013
Sequential File No.:	00377	File Date:	04/11/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0130
Solution Control Lot:	12B099	Expires:	02/20/2014
		Bottle No.:	0028

Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L
Signature: *[Handwritten Signature]* # 6040 Badge No.: 6040
Date: 04/11/2013

*Black Key Temperature Probe Serial.....# DDMBP1-0002 (Mea)
*Digital NIST Temperature Measuring System Serial.....# 122172176 (Mea)

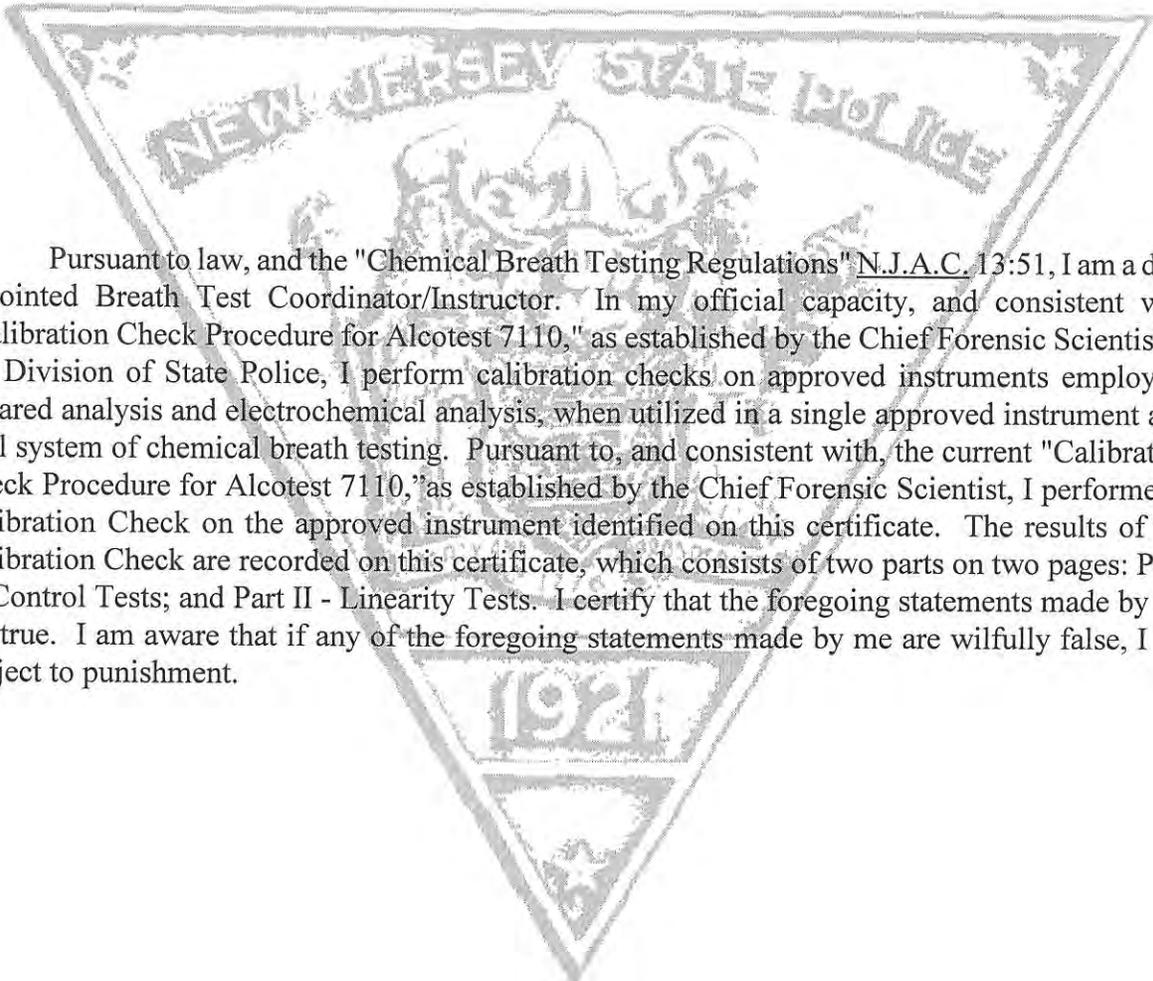

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0038
Location: EASTAMPTON TOWNSHIP
Calibration File No.: 00377 Calib. Date: 04/11/2013 Calib. No.: 00018
Certification File No.: 00378 Cert. Date: 04/11/2013 Cert. No.: 00015
Linearity File No.: 00361 Lin. Date: 11/15/2012 Lin. No.: 00014
Solution File No.: 00376 Soln. Date: 04/09/2013 Soln. No.: 00118
Sequential File No.: 00378 File Date: 04/11/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0130
Control Solution %: 0.100% Expires: 02/20/2014
Solution Control Lot: 12B099 Bottle No.: 0028

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:40D		
Control 1 EC	0.100%	12:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:42D		
Control 2 EC	0.098%	12:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:43D		
Control 3 EC	0.097%	12:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:45D		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: 

Badge No.: 6040

Date: 04/11/2013

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0038
Location: EASTAMPTON TOWNSHIP
Calibration File No.: 00377 Calib. Date: 04/11/2013 Calib. No.: 00018
Certification File No.: 00378 Cert. Date: 04/11/2013 Cert. No.: 00015
Linearity File No.: 00379 Lin. Date: 04/11/2013 Lin. No.: 00015
Solution File No.: 00376 Soln. Date: 04/09/2013 Soln. No.: 00118
Sequential File No.: 00379 File Date: 04/11/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0215
Control Solution %: 0.040% Expires: 06/27/2013
Solution Control Lot: 11F090 Bottle No.: 1321

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0193
Control Solution %: 0.080% Expires: 06/30/2013
Solution Control Lot: 11F091 Bottle No.: 0130

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0241
Control Solution %: 0.160% Expires: 07/03/2013
Solution Control Lot: 11G092 Bottle No.: 0889

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:57D		
Control 1 EC	0.040%	12:58D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	12:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:00D		
Control 2 EC	0.040%	13:00D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.039%	13:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:02D		
Control 3 EC	0.081%	13:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.079%	13:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:04D		
Control 4 EC	0.081%	13:05D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	13:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:06D		
Control 5 EC	0.160%	13:07D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.158%	13:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:09D		
Control 6 EC	0.158%	13:09D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.157%	13:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:11D		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: _____

[Handwritten Signature] #6040

Badge No.: 6040

Date: 04/11/2013

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0038
 Location: EASTAMPTON TOWNSHIP
 Calibration File No.: 00377 Calib. Date: 04/11/2013 Calib. No.: 00018
 Certification File No.: 00378 Cert. Date: 04/11/2013 Cert. No.: 00015
 Linearity File No.: 00379 Lin. Date: 04/11/2013 Lin. No.: 00015
 Solution File No.: 00380 Soln. Date: 04/11/2013 Soln. No.: 00119
 Sequential File No.: 00380 File Date: 04/11/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0130
 Control Solution %: 0.100% Expires: 01/05/2014
 Solution Control Lot: 12A097 Bottle No.: 0274

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:19D		
Control 1 EC	0.101%	14:19D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:19D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:20D		
Control 2 EC	0.099%	14:21D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:21D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:22D		
Control 3 EC	0.099%	14:22D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:22D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number DDJFP2-0438 (M)

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Michelle Goncalves #6040

Badge No.: 6040

Date: 04/11/2013



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDUK 53-0130

Certification Date

3-22-13

Technician

BC

Re-Certification Due Date

3-22-14

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDSF A2-0438

Certification date:

3-22-13

Next Certification due:

3-22-14

Probe Value

104

Draeger Safety Diagnostics, Inc.
Technical Service Department

B/E

Draeger safety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

03-11-08

ARUK-0038

Draeger Safety Diagnostics, Inc.
Durango, CO





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

JEFFREY S. CHIESA
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 2/6/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12A097

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 5, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Monica L. Tramontin
 Forensic Scientist III
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 13th day of February, 2012.

Mary E. McLaughlin
 Notary


MARY ELIZABETH MCLAUGHLIN
 NOTARY PUBLIC OF NEW JERSEY
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable



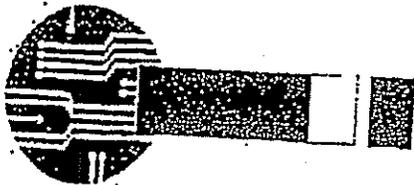

CERTIFICATE

This is to certify that


Michelle Goncalves

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012

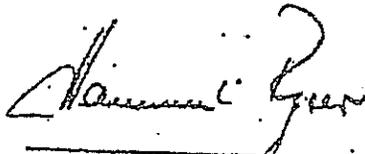

Instructor: Hansueli Ryser

Dräger



CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lieutenant Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF CRIMINAL JUSTICE
PO Box 085
TRENTON, NJ 08625-0085
TELEPHONE: (609) 984-6500

JEFFREY S. CHIESA
Attorney General

STEPHEN J. TAYLOR
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C. 13:51-2.1 (b) and (c)*, as adopted and promulgated under the provisions of *N.J.S.A. 39:4-50.3, 39:3-10.25 and 12:7-56*, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police
DSFC Patrick Guilfooy, Unit Head, Alcohol/Drug Test Unit, Division of State Police



DEPARTMENT OF
Traffic and Public Safety
 What is to be certified that
 MICHELLE L. MCKELVEY
 IS QUALIFIED AND COMPETENT TO CONDUCT COURSE AND INSTRUCTORS PERFORMING TO CHAPTER 147 OF
 THE LAWS OF NEW JERSEY IN THE OPERATION OF THE **DRUG ANALYZER**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY ON 16th DAY OF Aug
 TWO THOUSAND AND 04
 SUPERINTENDENT
 NEW JERSEY STATE POLICE
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES Feb. 3-7-2003
 Refresher Course

DATE	PLACE	INSTRUCTOR
1. <u>10/10/03</u>	<u>OCFA</u>	<u>C. P. [Signature]</u>
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 05/02)

DEPARTMENT OF
Traffic and Public Safety
 What is to be certified that
 MICHELLE L. MCKELVEY
 NEW JERSEY STATE POLICE
 IS QUALIFIED AND COMPETENT TO CONDUCT COURSE AND INSTRUCTORS PERFORMING TO CHAPTER 147 OF
 THE LAWS OF NEW JERSEY IN THE OPERATION OF THE **ALCOHOL TEST 7110 MKII-C**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY ON 10th DAY OF August
 TWO THOUSAND AND FIVE
 SUPERINTENDENT
 NEW JERSEY STATE POLICE
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____
 Refresher Course

DATE	PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 05/02)

DEPARTMENT OF
Traffic and Public Safety
 What is to be certified that
 Michelle L. Goncalves
 New Jersey State Police
 IS QUALIFIED AND COMPETENT TO CONDUCT COURSE AND INSTRUCTORS PERFORMING TO CHAPTER 147 OF
 THE LAWS OF NEW JERSEY IN THE OPERATION OF THE **ALCOHOL TEST 7110 MKII-C**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY ON 15th DAY OF December
 TWO THOUSAND AND Eleven
 SUPERINTENDENT
 NEW JERSEY STATE POLICE
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____
 Refresher Course

DATE	PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 05/02)

DEPARTMENT OF
Traffic and Public Safety
 What is to be certified that
 Michelle Goncalves
 New Jersey State Police
 IS QUALIFIED AND COMPETENT TO CONDUCT COURSE AND INSTRUCTORS PERFORMING TO CHAPTER 147 OF
 THE LAWS OF NEW JERSEY IN THE OPERATION OF THE **High Tech Coordinator/Instructor**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY ON 23rd DAY OF March
 TWO THOUSAND AND Twelve
 SUPERINTENDENT
 NEW JERSEY STATE POLICE
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____
 Refresher Course

DATE	PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 05/02)



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-4289985

Traceable Certificates of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Metronford Road, Radnor, PA 19087
Instrument Identification:

Model: 61220-601 S/N: 122172176 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-275	ABA237		
Digital Thermometer	B16315	6/05/12	B1606038
PRT Temperature Probe	D1541	5/28/12	B1526035
Temperature Calibration Bath TC-258	B01375		
Thermistor Module	A27128	10/31/12	1000306945
Temperature Probe	157	11/13/12	6-BL72N-1-1
Temperature Calibration Bath TC-178	A45240		
Thermistor Module	A17118	2/01/13	1000311439
Temperature Probe	128	2/14/13	6-BN8WZ-27-1

Certificate Information:

Technician: 68 Procedure: CAL-03 Cal Date: 3/30/12 Cal Due: 3/30/14
Test Conditions: 23.0°C 44.0 %RH 1012 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.000	-0.001	Y	-0.050	0.050	0.013	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.014	3.8:1
°C		N.A.		60.650	60.650	Y	60.650	60.650	0.040	2.8:1
°C		N.A.		100.001	100.002	Y	99.951	100.051	0.019	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). This uncertainty represents an expanded uncertainty using a coverage factor $k=2$ to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy= $(\text{Max}-\text{Min})/2$; Min = As Left Nominal (Rounded) - Tolerance; Max = As Left Nominal (Rounded) + Tolerance; Date=YYYYMMDD

Neil Rodriguez
Neil Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:


In our opinion, once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contaminants.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4465 Ross Road, Friendswood, TX 77646 USA
Phone 281 482-1714 Fax 281 482-5468 service@control.com www.control.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CE31-01603-2008-AQ-PCU-ANAS.
International Laboratory Accreditation Cooperation (ILAC) • Multilateral Recognition Arrangement (MRA).



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWF 53-0241

Certification Date


Technician

Re-Certification Due Date

2-6-13

BC

2-6-14



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXD 53-0193

Certification Date

Technician

Re-Certification Due Date

2-5-13

BC

2-5-14

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDMBP1-0002

Certification date:

02/05/13

Next Certification due:

02/05/14

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department

SY



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWF 53-0215

Certification Date

2-6-13

Technician

BC

Re-Certification Due Date

2-6-14



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 West Trenton NJ 08621-0668
 (609) 832-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11R090


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kowalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.


 Notary

Lincoln I. D'Amico
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
West Trenton NJ 08628-0068
(609) 832-2000

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11E091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13-51-3.4, of approved breath test instruments (N.J.A.C. 13-51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kwalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.

Notary

Linda L. DiCorleone
Notary Public, State of New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 West Trenton, NJ 08621-0068
 (609) 821-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

PAULA T. DOW
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Dresser Safety, Inc.

ANALYSIS DATE: 7/15/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G492


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Ronald W. Kowalik, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 1st day of August, 2011.


 Notary



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JEFFREY S. CHIESA
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 3/20/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12B099

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1211 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 20, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Monica L. Tramontin
 Forensic Scientist III
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 22nd day of March, 2012.

Notary

MARY ELIZABETH McLAUGHLIN
 NOTARY PUBLIC OF NEW JERSEY
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"
 New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable

