

Municipality: PENNSVILLE Twp Alcotest Ser.#: ARTN-0044

ALCOTEST CHECKLIST 01-30-2009

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R..
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDUM 53-0238
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R..
Ser. #: DDWA P2-063
- 4. **Digital Temperature Measuring System Report of Calibration.**
- 5.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDWA P2-0001
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
 - A. 0.04% Solution. 08 F 054
 - B. 0.08% Solution. 08 F 055
 - C. 0.10% Solution. 08 G 056
 - D. 0.16% Solution. 08 G 057
- 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - A. 0.04% used in Calibration/Linearity Testing. DDMK 53-0003
 - B. 0.08% used in Calibration/Linearity Testing. DDRK 53-0005
 - C. 0.10% used in Calibration/Linearity Testing DDUM 53-0238 [Same as instrument's CU34 unit].
 - D. 0.16% used in Calibration/Linearity Testing. DDRF 53-0009
- 8.
 - A. New Standard Solution Report - following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 08 A 049
 - D. Alcotest card of operator/coordinator who completed change.

Dräger safety

Alcotest 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

01-15-08

SERIAL NUMBER:

ARTN-0044

Draeger Safety Diagnostics, Inc.



Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-063

Certification date:

01-13-2009


Next Certification due:

01-13-2010

Probe Value

104

Dräger Safety Diagnostics, Inc.
Technical Service Department



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers. (F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWMS3-0239

Certification Date

01-13-2009

Technician



Re-Certification Due Date

01-13-2010

Drägersafety

Ertco-Hart Digital Temperature Measuring System

REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature verification Serial Number: HH41 301316 / HH41 303176 / MERCURY THERMOMETER

Digital Units Serial Number: A71569

Probe Serial Number: 765077

Certification Date: 02-12-2008

Next Certification Due: 02-12-2009

At 34.00 °C digital unit displays 34.05 °C

Draeger Safety Diagnostics, Inc. Technician: 

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: PENNSVILLE P.D. Serial No.: ARTN-0044
Calibration File No.: 00295 Calib. Date: 01/30/2009 Calib. No.: 00009
Certification File No.: 00267 Cert. Date: 08/13/2008 Cert. No.: 00005
Linearity File No.: 00268 Lin. Date: 08/13/2008 Lin. No.: 00005
Solution File No.: 00294 Soln. Date: 01/07/2009 Soln. No.: 00067
Sequential File No.: 00295 File Date: 01/30/2009


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0238
Control Solution %: 0.100% Expires: 07/02/2010
Solution Control Lot: 08G056 Bottle No.: 1352

Coordinator

Last Name: WEYMAN

First Name: HAROLD

MI: -

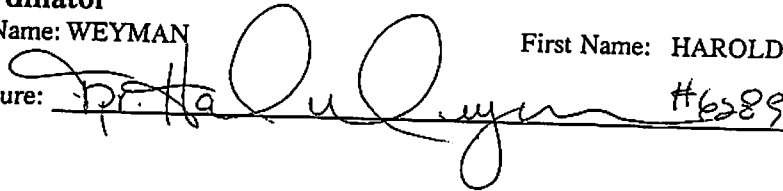Signature: 


#6289

Badge No.: 6289

Date: 01/30/2009

*Black Key Temperature Probe Serial# DDWAP2 - od H.W.

*Ertco-Hart Digital Temperature Measuring System Serial# A71569 H.W.

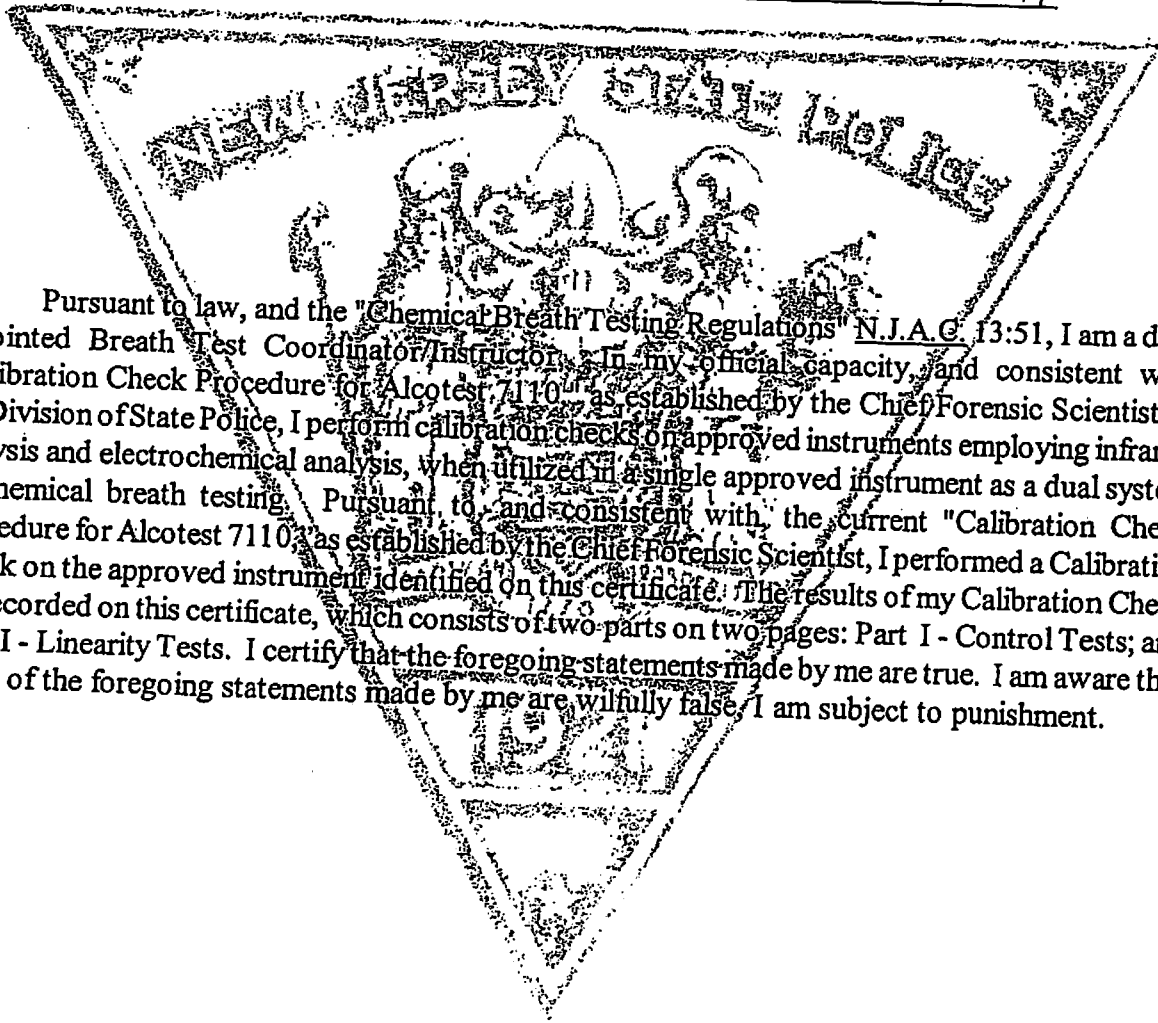

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.


Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0044
Location:	PENNSVILLE P.D.	Calib. No.:	00009
Calibration File No.:	00295	Cert. No.:	00006
Certification File No.:	00296	Lin. No.:	00005
Linearity File No.:	00268	Soln. No.:	00067
Solution File No.:	00294	Calib. Date:	01/30/2009
Sequential File No.:	00296	Cert. Date:	01/30/2009
		Lin. Date:	08/13/2008
		Soln. Date:	01/07/2009
		File Date:	01/30/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0238
Solution Control Lot:	08G056	Expires:	07/02/2010
		Bottle No.:	1352

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:12S		
Control 1 EC	0.100%	10:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13S		
Control 2 EC	0.097%	10:14S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14S		
Control 3 EC	0.098%	10:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16S		

All tests within acceptable tolerance.

Coordinator
 Last Name: WEYMAN First Name: HAROLD MI: -
 Signature:  #6289
 Badge No: 6289 Date: 01/30/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0044
Location:	PENNSVILLE P.D.	
Calibration File No.:	00295	Calib. Date: 01/30/2009
Certification File No.:	00296	Calib. No.: 00009
Linearity File No.:	00297	Cert. Date: 01/30/2009
Solution File No.:	00294	Lin. Date: 01/30/2009
Sequential File No.:	00297	Lin. No.: 00006
		Soln. Date: 01/07/2009
		Soln. No.: 00067
		File Date: 01/30/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDMK S3-0003
Control Solution %:	0.040%		Expires: 06/26/2010
Solution Control Lot:	08F054		Bottle No.: 0282

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDRK S3-0005
Control Solution %:	0.080%		Expires: 06/28/2010
Solution Control Lot:	08F055		Bottle No.: 0941

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDRF S3-0009
Control Solution %:	0.160%		Expires: 07/07/2010
Solution Control Lot:	08G057		Bottle No.: 0727

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:37S		
Control 1 EC	0.042%	10:37S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	10:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39S		
Control 2 EC	0.042%	10:39S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	10:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41S		
Control 3 EC	0.081%	10:41S	33.8°C	*** TEST PASSED ***
Control 3 IR	0.080%	10:41S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		
Control 4 EC	0.081%	10:44S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	10:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45S		
Control 5 EC	0.159%	10:46S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	10:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47S		
Control 6 EC	0.158%	10:48S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.161%	10:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50S		

All tests within acceptable tolerance.

Coordinator

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature: 

Badge No.: 6289

Date: 01/30/2009


DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Harold Weyman
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF
 THE LAWS OF 1966 IN THE OPERATION OF A BREATH TEST COORDINATOR/INSTRUCTOR
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 5th DAY OF November

TWO THOUSAND AND Eight


 SUPERINTENDENT
 NEW JERSEY STATE POLICE


 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	_____	_____	_____
2.	_____	_____	_____
3.	_____	_____	_____
4.	_____	_____	_____
5.	_____	_____	_____
6.	_____	_____	_____
7.	_____	_____	_____
8.	_____	_____	_____
9.	_____	_____	_____

DEPARTMENT OF
Law and Public Safety
 This is to certify that

Harold Weyman
 New Jersey State Police


IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 143 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 30th DAY OF MAY
 TWO THOUSAND AND EIGHT

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	_____	_____	_____
2.	_____	_____	_____
3.	_____	_____	_____
4.	_____	_____	_____
5.	_____	_____	_____
6.	_____	_____	_____
7.	_____	_____	_____
8.	_____	_____	_____
9.	_____	_____	_____

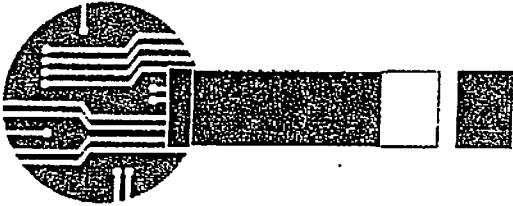

CERTIFICATE

This is to certify that

Harold Weyman
Detective, #6289

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified


**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: September 18, 2008

Instructor: Hansueli Ryser

Dräger

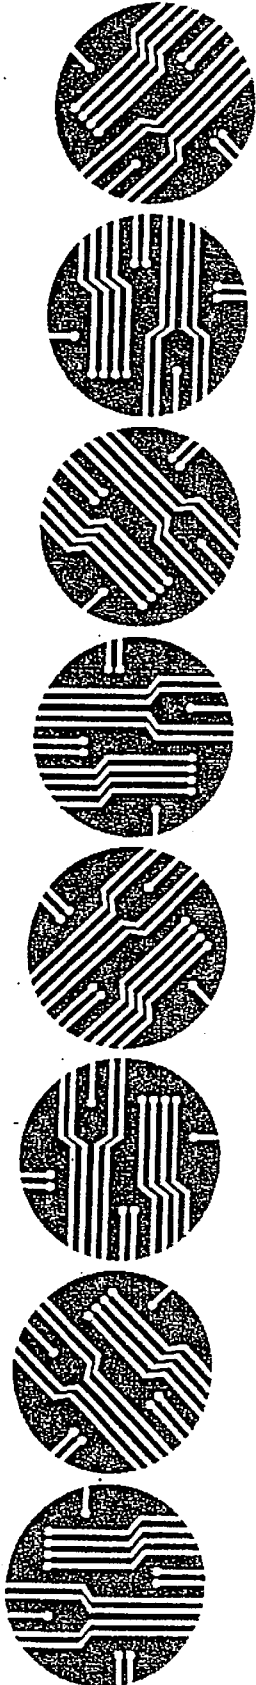

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAPZ-001

Certification date:

02-12-08

Next Certification due:

02-12-09

Probe Value

101

Draeger Safety Diagnostics, Inc.
Technical Service Department





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR PREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 07/16/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F054

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0487 to 0.0493 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary
JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 07/25/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F055

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0977 to 0.0984 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 11th day of August, 2008.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 07/24/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G056

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1227 to 0.1236 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 2, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 13th day of August, 2008.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 07/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G057

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1956 to 0.1959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDMK 53-0003

Certification Date


02-13-08

Technician

YE

Re-Certification Due Date

02-13-09



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDRK53-0005

Certification Date

02-13-08

Technician

Re-Certification Due Date

02-13-09



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDRF53-0009

Certification Date

02-13-08

Technician

[Signature]

Re-Certification Due Date

02-13-09

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0044
Location:	PENNSVILLE P.D.	
Calibration File No.:	00295	Calib. Date: 01/30/2009
Certification File No.:	00296	Calib. No.: 00009
Linearity File No.:	00297	Cert. Date: 01/30/2009
Solution File No.:	00298	Cert. No.: 00006
Sequential File No.:	00298	Lin. Date: 01/30/2009
		Lin. No.: 00006
		Soln. Date: 01/30/2009
		Soln. No.: 00068
		File Date: 01/30/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUM S3-0238
Control Solution %: 0.100%		Expires: 01/09/2010
Solution Control Lot: 08A049		Bottle No.: 0540

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:02S		
Control 1 EC	0.101%	12:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		
Control 2 EC	0.099%	12:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:05S		
Control 3 EC	0.099%	12:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperatur Probe Serial Number: DDXAP2-103 *H.W.*

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature: *H. Weyman* #6289

Badge No.: 6289

Date: 01/30/2009



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 02/08/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08A049

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1220 to 0.1225 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 9, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 16th day of April, 2008.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

