

ALCOTEST CHECKLIST

Municipality: FLORENCE TWP. Alcotest Ser.#: ARTN-0053

County: BURLINGTON Date of Calibration: 03-28-2011

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDUM 53-0222
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWI P2-293
- 4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 101733 534
- 5.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDWA P2-016
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
 - A. 0.04% Solution. 10 A 073
 - B. 0.08% Solution. 10 A 074
 - C. 0.10% Solution. 10 F 080
 - D. 0.16% Solution. 10 A 075
- 7. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - A. 0.04% used in Calibration/Linearity Testing. DDWE 53-0196
 - B. 0.08% used in Calibration/Linearity Testing. DDWE 53-0203
 - C. 0.10% used in Calibration/Linearity Testing DDUM 53-0222
[Same as instrument's CU34 unit].
 - D. 0.16% used in Calibration/Linearity Testing DDWE 53-0205
- 8.
 - A. New Standard Solution Report following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 10 F 079
 - D. Alcotest card of operator/coordinator who completed change.

7-12-2011

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

3/21/2011

ARTN-0053

Dräger Safety Diagnostics, Inc.





NEW JERSEY STATE POLICE
Alcohol/Drug Testing Unit

Trooper Steve Dellanoce #6027
Breath Test Coordinator / Instructor

Hamilton Technology Complex
Suite 400
1200 Negron Drive
Hamilton, NJ 08891

(609) 584-5000 ext. 5808
cell: (609) 947-9211
Fax: (609) 584-8359
email: LPP6027@gw.njsp.org



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDUM53-0222

Certification Date

Technician

Re-Certification Due Date

11-17-10

mm

11-17-11

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWTP2-293

11-17-10

11-17-11

Probe Value

105

Dräger Safety Diagnostics, Inc.
Technical Service Department

mm



Calibration
Certificate No. 1750.01

Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NCSL Z540-1



Cert. No.: 4000-2966289

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, P.O. Box 2158, Secaucus, NJ 07094 U.S.A.

Instrument Identification:

Model: 61220-601

S/N: 101733534

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	11/19/10	A9B21010
Temperature Probe	128	12/10/10	A9B23079
Temperature Calibration Bath TC-231	A78341		
Temperature Probe	3039	12/10/10	A9B23080-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Module	A27129	7/09/10	1000264338
Temperature Probe	5202	3/11/11	B0310050
Temperature Calibration Bath TC-255	B01375		
Temperature Probe	157	7/27/10	A9708011-4

Certificate Information:

Technician: 104

Procedure: CAL-06

Cal Date: 6/08/10

Cal Due: 6/08/12

Test Conditions: 24.0°C 42.0%RH 1015 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	-0.001	Y	-0.048	0.052	0.013	3.8:1
°C		N.A.		24.999	25.000	Y	24.949	25.049	0.013	3.8:1
°C		N.A.		60.001	59.998	Y	59.951	60.051	0.018	2.8:1
°C		N.A.		100.001	100.002	Y	99.951	100.051	0.013	3.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal/Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = Nominal/Rounded - Tolerance; Max = Nominal/Rounded + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change bits, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AD-HOU-ANAB.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00458 Calib. Date: 03/28/2011 Calib. No.: 00017
Certification File No.: 00428 Cert. Date: 01/05/2011 Cert. No.: 00009
Linearity File No.: 00429 Lin. Date: 01/05/2011 Lin. No.: 00009
Solution File No.: 00456 Soln. Date: 03/21/2011 Soln. No.: 00105
Sequential File No.: 00458 File Date: 03/28/2011


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222
Control Solution %: 0.100% Expires: 06/14/2012
Solution Control Lot: 10F080 Bottle No.: 0371

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
Signature: Joe Dellanoce #6027 Badge No.: 6027
Date: 03/28/2011

*Black Key Temperature Probe Serial.....# DDWAP2-016 *js*

*Digital NIST Temperature Measuring System Serial.....# 101733534 *js*

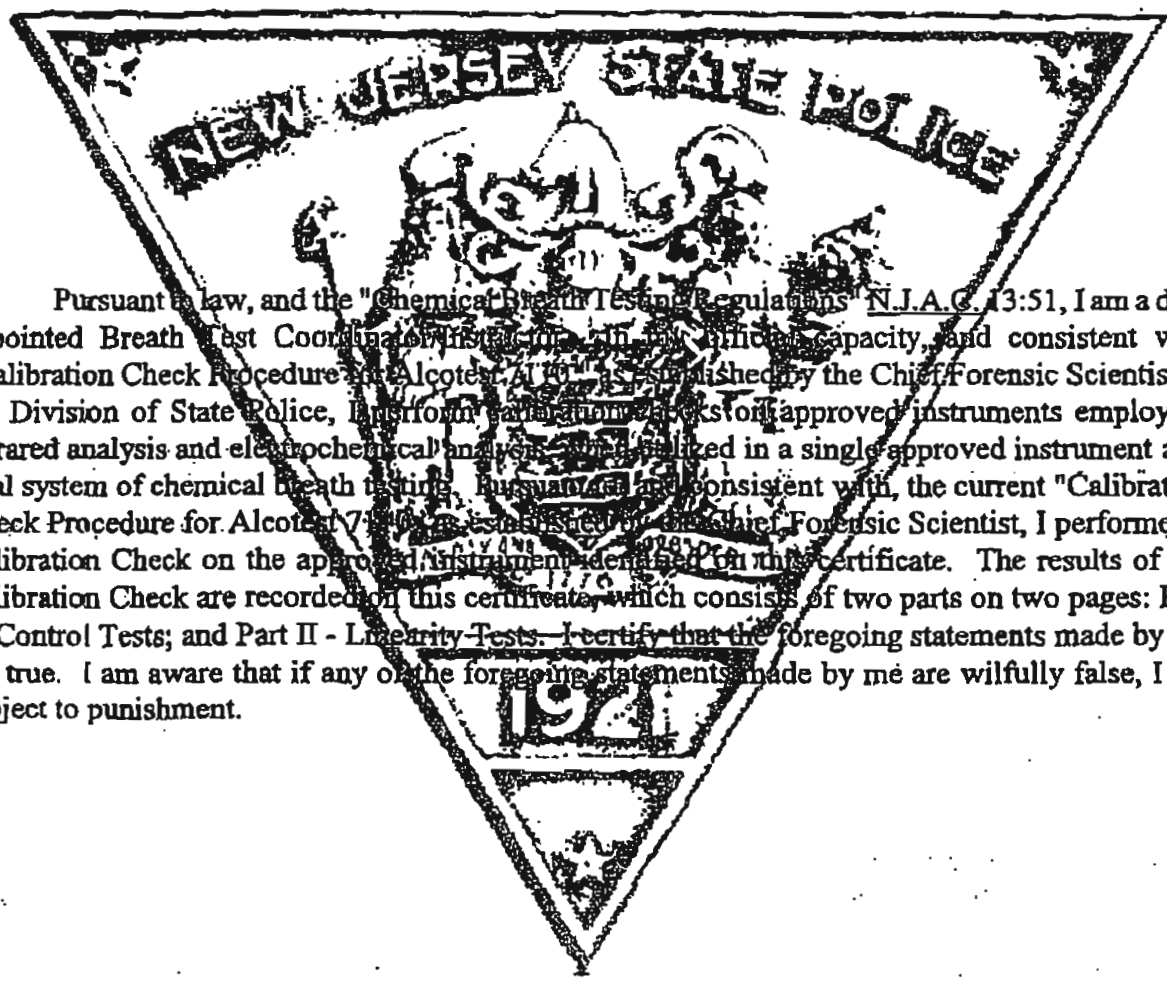

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis which are utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00458	Calib. Date: 03/28/2011
Certification File No.:	00459	Calib. No.: 00017
Linearity File No.:	00429	Cert. Date: 03/28/2011
Solution File No.:	00456	Cert. No.: 00010
Sequential File No.:	00459	Lin. Date: 01/05/2011
		Lin. No.: 00009
		Soln. Date: 03/21/2011
		Soln. No.: 00105
		File Date: 03/28/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	10F080	Expires: 06/14/2012
		Bottle No.: 0371

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:48S	34.0°C	*** TEST PASSED ***
Control 1 EC	0.099%	12:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:49S	34.0°C	*** TEST PASSED ***
Control 2 EC	0.099%	12:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:50S	34.0°C	*** TEST PASSED ***
Control 3 EC	0.099%	12:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:52S	34.0°C	*** TEST PASSED ***

All tests within acceptable tolerance.

Coordinator

Last Name: DELANOCE

Signature: *[Handwritten Signature]*

No. 6027

Date: 03/28/2011

Pursuant to law, and the "Chemical Breath Test Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Inspector in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I performed calibration checks on approved instruments employing infrared analysis and electrochemical analysis which are utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00458 **Calib. Date:** 03/28/2011 **Calib. No.:** 00017
Certification File No.: 00459 **Cert. Date:** 03/28/2011 **Cert. No.:** 00010
Linearity File No.: 00460 **Lin. Date:** 03/28/2011 **Lin. No.:** 00010
Solution File No.: 00456 **Soln. Date:** 03/21/2011 **Soln. No.:** 00105
Sequential File No.: 00460 **File Date:** 03/28/2011

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0196
Control Solution %: 0.040% **Expires:** 01/12/2012
Solution Control Lot: 10A073 **Bottle No.:** 0042

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0203
Control Solution %: 0.080% **Expires:** 01/15/2012
Solution Control Lot: 10A074 **Bottle No.:** 1031

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWE S3-0205
Control Solution %: 0.160% **Expires:** 01/21/2012
Solution Control Lot: 10A075 **Bottle No.:** 0842

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:07S	14:07D	
Control 1 EC	0.039%	13:07S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	13:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:09S		
Control 2 EC	0.039%	13:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	13:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:10S		
Control 3 EC	0.078%	13:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	13:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:12S		
Control 4 EC	0.078%	13:13S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.078%	13:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14S		
Control 5 EC	0.155%	13:15S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.156%	13:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16S		
Control 6 EC	0.156%	13:17S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.158%	13:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18S	14:18D gsp	

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Joseph Dellanoce #6027

Badge No.: 6027

Date: 03/28/2011

DEPARTMENT OF
Justice and Public Safety

Joseph S. Dellanoce
 New Jersey State Police

is challenged and competent to conduct professional duties as a member according to CHAPTER 102 OF
 TITLE 17B OF THE STATUTES OF THE STATE OF NEW JERSEY AND TO CHAPTER 102 OF
 TITLE 17B OF THE STATUTES OF THE STATE OF NEW JERSEY AS AMENDED BY CHAPTER 7110 OF TITLE 17B
 AS AMENDED TO EXTEND THE AUTHORITY OF THE BOARD OF EXAMINERS TO REVOKE LICENSES OF
 PROFESSIONALS IN THE STATE OF NEW JERSEY.

29th day of March

FIVE

[Signature]
 SUPERVISOR
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2/5/07	GC PA	C. P. [Signature]
2. 12/7/09	DC PA	[Signature]
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2010 (REV. 12/04)

DEPARTMENT OF
Traffic and Public Safety
What is to be certified that

Joseph S. Dellanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT THE FOLLOWING COURSE AND TO INSTRUCT IN THE
 THE LAWS OF NEW JERSEY IN THE OPERATION OF THE Breath Test Coordinator/Instructor
 A METHOD TO DEVELOPE INSTRUCTIONAL
 COVERED UNDER MY NAME AT THE OFFICE NEW JERSEY POLICE

14th DAY OF January

THE COURSE IS FOR EIGHT

[Signature]
 ATTORNEY GENERAL
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>12/17/09</u>	<u>OC.PA</u>	<u>Adam Standa</u>
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

DEPARTMENT OF
Fire and Public Safety

This is to certify that
Joseph B. Ballanocè
New Jersey State Police

IS QUALIFIED AND COMPETENT TO PERFORM THE SPECIAL DUTY AS QUALIFIED PURSUANT TO CHAPTER
143 OF TITLE 17 AND OF PART OF TITLE 17 OF THE STATUTES OF THE STATE OF NEW JERSEY
A METHOD TO DETERMINE DRUG CONCENTRATION IN BREATH BY MEANS OF A BREATHALYZER

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 13th day of Dec
TWO THOUSAND AND 01

Car. P. Kelly
SUPERINTENDENT
NEW JERSEY STATE POLICE

J. P. J.
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES: 8/30 - 9/3/99

Refresher Course		
DATE	PLACE	INSTRUCTOR
1. <u>12/12/01</u>	<u>A.G.T.C.</u>	<u>Potter</u>
2. <u>2-28-07</u>	<u>CPA</u>	<u>C. P. J.</u>
3. <u>10-3-09</u>	<u>ACTE</u>	<u>Ch. Stanley</u>
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

SP-2938 (Rev. 4/00)



JOHN S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
PO BOX 080
TRENTON, NJ 08625-0080

ANNE MILGRAM
Attorney General

January 14, 2008

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -
Trooper Joseph S. Dellanoce #6027

Dear Colonel Fuentes:

Pursuant to the provisions of *N.J.A.C.* 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A.* 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Trooper Joseph S. Dellanoce #6027, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,


Anne Milgram
Attorney General

jk
c. Trooper Joseph S. Dellanoce #6027, Alcohol/Drug Test Unit, Division of State Police
Lt. Mark Kolodzieski, Unit Head, Alcohol/Drug Test Unit, Division of State Police



20074



CERTIFICATE

This is to certify that


Joseph S. Dellanoce #6027

has successfully completed the two day Draeger Safety
Diagnostics, Inc. Operator Training and Preventive
Maintenance Course on the New Jersey specific
Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train
and certify Operators in the proper use and operation as
well as perform Preventive Maintenance on the New Jersey
specific Alcotest® 7110 MKIII-C.

Date: 4/12/2007

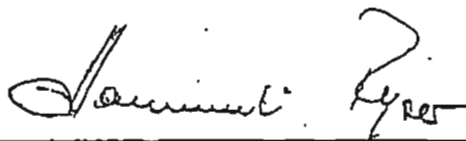

Instructor: Hansueli Ryser

Dräger



Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWAP2-016

February 7, 2011

February 7, 2012

Probe Value

107

Dräger Safety Diagnostics, Inc.
Technical Service Department





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7058
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

PAULA T. DOW
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

HRIS CHRISTIE
 Governor

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.


MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/2/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19A073


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0481 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 12, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

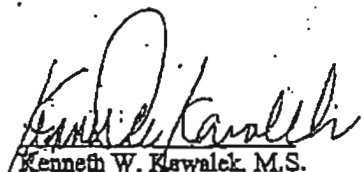
 Kenneth W. Kowalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.


 Notary

Linda L. Desantis
 Notary Public, New Jersey
 Commission Expires 8-17-14





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

PAULA T. DOW
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

HRIS CHRISTIE
 Governor

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/3/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A074

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0954 to 0.0958 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 15, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek
 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.

Linda L. DiStasio
 Notary.

Linda L. DiStasio
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CIRIS CHRISTIE
 Governor

PAULA T. DOW
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 7/8/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10F080

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1197 to 0.1207 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 14, 2012.


As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 5th day of July, 2010.

Dora R. Fuentes
 Notary



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 West Trenton NJ 08628-0068
 (609) 882-2000

PAULA T. DOW
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CHRIS CHRISTIE
 Governor

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 2/4/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A075


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1913 to 0.1919 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 21, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalick, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.


 Notary

Linda L. Desantis
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWE 53-0196

Certification Date

Technician

Re-Certification Due Date

2/28/11

JM

2/28/12



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK II A

Other: _____

Serial Number:

DDWES3-0203

Certification Date

Technician

Re-Certification Due Date

February 7, 2011

DM

February 7, 2012



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDWES3-0205

Certification Date

Technician

Re-Certification Due Date

February 7, 2011

DM

February 7, 2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00017
Calibration File No.:	00458	Cert. Date:	03/28/2011
Certification File No.:	00459	Lin. Date:	03/28/2011
Linearity File No.:	00460	Soln. Date:	03/28/2011
Solution File No.:	00461	File Date:	03/28/2011
Sequential File No.:	00461		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	10F079	Expires:	06/10/2012
		Bottle No.:	1093

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:25S	15:25D	
Control 1 EC	0.099%	14:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:26S		
Control 2 EC	0.099%	14:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:27S		
Control 3 EC	0.099%	14:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:29S	15:29D	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP2-293,10

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: *J. Dellanoce*

Badge No.: 6027

Date: 03/28/2011



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Attorney General

KIM GUADAGNO
 Lt. Governor

COLONEL JOSEPH R. FUENTI
 Superintendent

**CERTIFICATION OF ANALYSIS
 0.10 PERCENT BREATHE ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATHE ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 7/7/2010

BREATHE ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10FV79


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1183 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 10, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 20th day of July, 2010.


 Notary

Linda L. Mufantus
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Print on Recycled Paper and Recyclable

