

Municipality: NORTH FIELD

Alcotest Ser.#: ARWM-0022
08-04-08

ALCOTEST CHECKLIST

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R..
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXA 53-0005
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWJ P2-157
- 4. **Digital Temperature Measuring System Report of Calibration.**
- 5.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDWA P2-016
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
 - A. 0.04% Solution. 07A 041
 - B. 0.08% Solution. 07A 042
 - C. 0.10% Solution. 07B045
 - D. 0.16% Solution. 07A 043
- 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - A. 0.04% used in Calibration/Linearity Testing. DDWE 53-0196
 - B. 0.08% used in Calibration/Linearity Testing. DDWE 53-0203
 - C. 0.10% used in Calibration/Linearity Testing DDXA 53-0005
[Same as instrument's CU34 unit].
 - D. 0.16% used in Calibration/Linearity Testing. DDWE 53-0205
- 8.
 - A. New Standard Solution Report - following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 07B046
 - D. Alcotest card of operator/coordinator who completed change.

TJRP

Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


07-25-08

SERIAL NUMBER:

ARWM-0022

Draeger Safety Diagnostics, Inc.





Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXAS3-0005

Certification Date

Technician

Re-Certification Due Date

08-18-08

JS

08-18-09

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWTPR-157

08-18-08


08-18-09

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department

JS



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDXA 53-0005

Certification Date

Technician

Re-Certification Due Date

Nov. 13/2007

TG

Nov. 13/2008

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due.

DDWJP2-157

11.13.07

11.13.08

Probe Value

100

Draeger Safety Diagnostics, Inc.
Technical Service Department

Ertco-Hart Digital Temperature Measuring System

REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature

verification Serial Number: HH41301316 / HH41303176 / MERCURY THERMOMETER


Digital Units Serial Number: A23730

Probe Serial Number: 773623

Certification Date: 02-13-08

Next Certification Due: 02-13-09

At 34.00 °C digital unit displays 34.07 °C

Draeger Safety Diagnostics, Inc. Technician: 

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00212 Calib. Date: 08/04/2008 Calib. No.: 00009
Certification File No.: 00213 Cert. Date: 08/04/2008 Cert. No.: 00005
Linearity File No.: 00180 Lin. Date: 04/07/2008 Lin. No.: 00004
Solution File No.: 00210 Soln. Date: 07/25/2008 Soln. No.: 00050
Sequential File No.: 00213 File Date: 08/04/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 02/22/2009
Solution Control Lot: 07B045 Bottle No.: 0886

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:00D		
Control 1 EC	0.099%	15:00D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:00D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:01D		
Control 2 EC	0.099%	15:01D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:01D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:02D		
Control 3 EC	0.100%	15:03D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:03D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03D		

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
Signature: Tpc JSD # 6027 Badge No.: 6027
Date: 08/04/2008

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00212 Calib. Date: 08/04/2008 Calib. No.: 00009
Certification File No.: 00213 Cert. Date: 08/04/2008 Cert. No.: 00005
Linearity File No.: 00214 Lin. Date: 08/04/2008 Lin. No.: 00005
Solution File No.: 00210 Soln. Date: 07/25/2008 Soln. No.: 00050
Sequential File No.: 00214 File Date: 08/04/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0196
Control Solution %: 0.040% Expires: 01/26/2009
Solution Control Lot: 07A041 Bottle No.: 0019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0203
Control Solution %: 0.080% Expires: 01/26/2009
Solution Control Lot: 07A042 Bottle No.: 0598

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0205
Control Solution %: 0.160% Expires: 01/26/2009
Solution Control Lot: 07A043 Bottle No.: 0281

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:20D		
Control 1 EC	0.040%	15:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	15:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:22D		
Control 2 EC	0.040%	15:23D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	15:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:24D		
Control 3 EC	0.080%	15:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	15:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:26D		
Control 4 EC	0.079%	15:27D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	15:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:28D		
Control 5 EC	0.159%	15:29D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	15:29D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:30D		
Control 6 EC	0.159%	15:31D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.160%	15:31D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:32D		

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: _____

J. Dellanoce #6027

Badge No.: 6027

Date: 08/04/2008

DEPARTMENT OF
Law and Public Safety
 This is to certify that

Joseph S. Dellanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL-BREATH ANALYSES PURSUANT TO CHAPTER 10 OF
 THE LAWS OF 1964 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
 A METHOD TO DETERMINE INTOXICATION.
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND Five


 SUPERINTENDENT
 NEW JERSEY STATE POLICE


 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	2/15/07	CCPA	C. POTER
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

DEPARTMENT OF
Health and Public Safety

This is to certify that
Joseph S. Dellanoce
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT MEDICAL BREATH ANALYSES PURSUANT TO CHAPTER
143 OF THE LAWS OF 1949 IN THE OPERATION OF THE Breathalyzer
A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 13th DAY OF Dec.
TWO THOUSAND AND 01

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES: 8/30 - 9/3/99

Refresher Course		
DATE	PLACE	INSTRUCTOR
1. <u>12/12/01</u>	<u>A.G.P.C.</u>	<u>Rotter</u>
2. <u>2-2-03</u>	<u>CPA</u>	<u>C. Rotter</u>
3. <u>10-3-05</u>	<u>ACTC</u>	<u>Ch. Stamba</u>
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

SP-293B (Rev. 4/00)

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-016

Certification date:

04.04.08

Next Certification due:

04.04.09

Probe Value

106

Draeger Safety Diagnostics, Inc.
Technical Service Department





RON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
W857 TRENTON NJ 08628-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A041

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 29th day of March, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





RON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A042

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0965 to 0.0972 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungarc

Ajit R. Tungarc
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 29th day of March, 2007.

Linda L. DeSantis
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





IN S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08626-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 04/04/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07B045

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1227 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 22, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 20th day of April, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer





RON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A043

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1932 to 0.1938 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Linda L. DeSantis
My Commission
Expires Aug. 17, 2008

Ajit R. Tungare
Ajit R. Tungare
Chief Forensic Scientist
Division of State Police


Sworn to and subscribed before me this 29th day of March, 2007.

Linda L. DeSantis
Notary



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Draeger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWE 53-0196

Certification Date


Technician

Re-Certification Due Date

02-13-08

VE

02-13-09



Draeger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0203

Certification Date


Technician

Re-Certification Due Date

02-13-08

[Signature]

02-13-09



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWE53-0205

Certification Date

Technician

Re-Certification Due Date

02-13-08

AE

02-13-09

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: NORTHFIELD POLICE DEPT. Serial No.: ARWM-0022
Calibration File No.: 00212 Calib. Date: 08/04/2008 Calib. No.: 00009
Certification File No.: 00179 Cert. Date: 04/07/2008 Cert. No.: 00004
Linearity File No.: 00180 Lin. Date: 04/07/2008 Lin. No.: 00004
Solution File No.: 00210 Soln. Date: 07/25/2008 Soln. No.: 00050
Sequential File No.: 00212 File Date: 08/04/2008


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 02/22/2009
Solution Control Lot: 07B045 Bottle No.: 0886

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
Signature: Joe Dellanoce #6027 Badge No.: 6027
Date: 08/04/2008

*Black Key Temperature Probe Serial# DDWAP2-016 *pro*

*Ertco-Hart Digital Temperature Measuring System Serial# A23730 *pro*

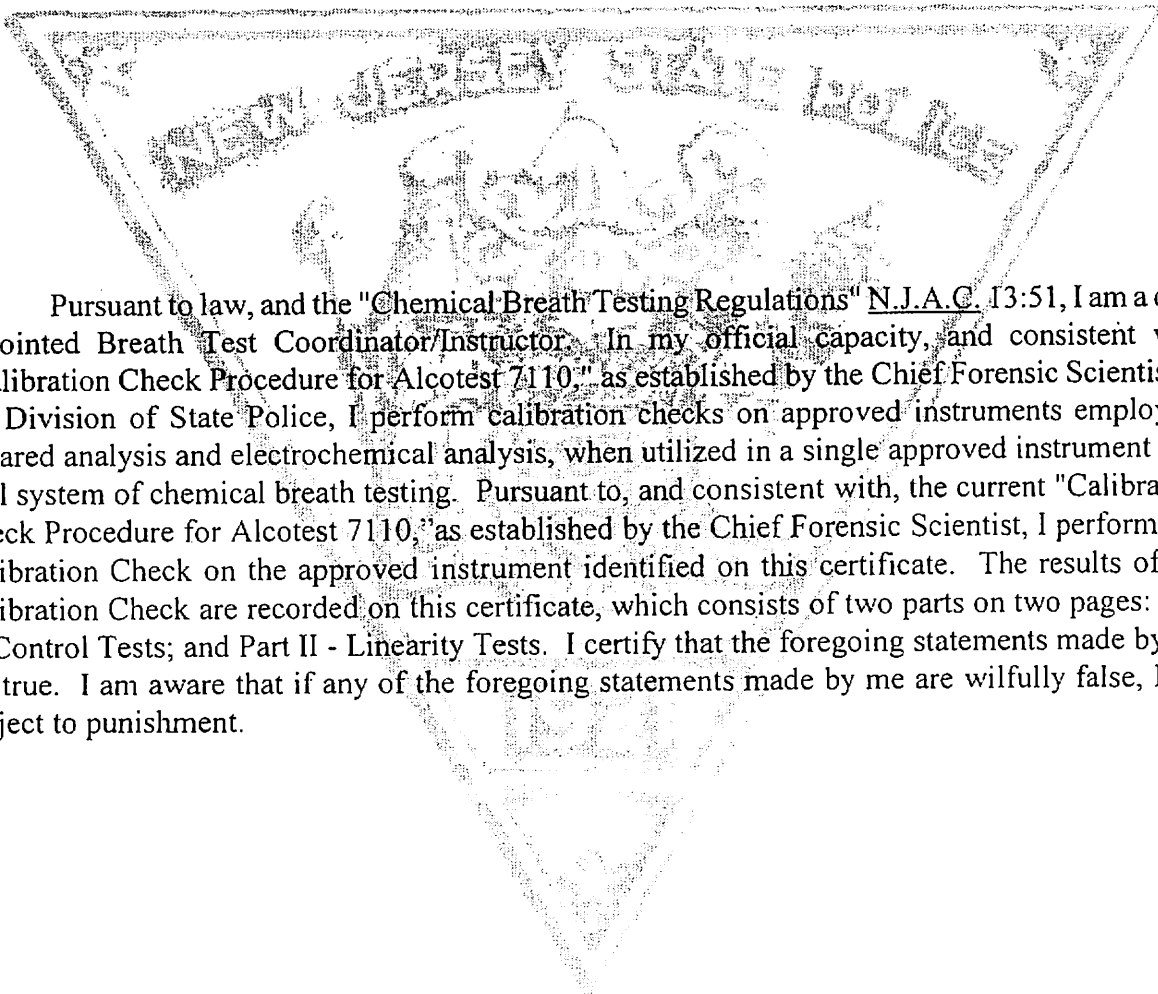

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00212 Calib. Date: 08/04/2008 Calib. No.: 00009
Certification File No.: 00213 Cert. Date: 08/04/2008 Cert. No.: 00005
Linearity File No.: 00214 Lin. Date: 08/04/2008 Lin. No.: 00005
Solution File No.: 00215 Soln. Date: 08/04/2008 Soln. No.: 00051
Sequential File No.: 00215 File Date: 08/04/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 04/24/2009
Solution Control Lot: 07B046 Bottle No.: 0286

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:40D		
Control 1 EC	0.102%	16:41D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:41D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:41D		
Control 2 EC	0.102%	16:42D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:42D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:43D		
Control 3 EC	0.101%	16:43D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:43D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:44D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWTP2-157₂₅₀

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tpr. J.D. # 6027

Badge No.: 6027

Date: 08/04/2008



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE Box 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 06/28/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07B046

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 24, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 13th day of July, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2008

