

ALCOTEST CHECKLIST

Municipality: LONGPORT

Alcotest Ser. #: ARXA-0067

County: ATLANTIC

Date of Calibration: 01-14-2020

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC 53-0154

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWA P2-177

4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 191 959 016

5. **NIST - Traceable Digital Thermometer Readings.**

6. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDXK P2-396

7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/>	A.	0.04% Solution.	<u>18240</u>
<input checked="" type="checkbox"/>	B.	0.08% Solution.	<u>18250</u>
<input checked="" type="checkbox"/>	C.	0.10% Solution.	<u>18220</u>
<input checked="" type="checkbox"/>	D.	0.16% Solution.	<u>18260</u>

8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

<input checked="" type="checkbox"/>	A.	0.04% used in Calibration/Linearity Testing	<u>DDWE 53-0206</u>
<input checked="" type="checkbox"/>	B.	0.08% used in Calibration/Linearity Testing	<u>DDWF 53-0218</u>
<input checked="" type="checkbox"/>	C.	0.10% used in Calibration/Linearity Testing. [Same as CU34 unit on instrument.]	
<input checked="" type="checkbox"/>	D.	0.16% used in Calibration/Linearity Testing	<u>DDWJ 53-0334</u>

9. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 19110
 D. Alcotest card of operator/coordinator who completed change.

Dreger

Alcotest® 7110 MKII-C

CERTIFICATE OF ACCURACY

This is to certify that the model 7110 MKII-C has been tested for accuracy against known standards and the following results were obtained: **Accuracy: 99.99%**
The accuracy of the instrument is within the limits specified in the manufacturer's specifications.
The manufacturer recommends a re-verification of this instrument within 12 months of the calibration date shown on this certificate, according to the State Specifications.

Certification Date:

1-10-14

SERIAL NUMBER:

AK 28-01167

Dreger Safety Diagnostics, Inc.

BL

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDXCS3-0154

Certification Date:

10-29-19

Technician:

BS

Re-Certification Due Date:

10-29-20

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWAP2-177

Certification Date:

10-29-19

Next Certification Due:

10-29-20

Probe Value:

104

Draeger, Inc.

BS



Calibration complies with ISO/IEC 17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177835

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 191959016

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	20 Apr 2019	1000424560
Thermistor Module	A27129	10 Jan 2020	1000436202
Temperature Calibration Bath	A73332		
Temperature Probe	3039	08 May 2019	6-B7F4L-20-1
Temperature Calibration Bath	A79341		
Temperature Probe	5394	29 Jan 2020	B9124038
Temperature Calibration Bath	B16388		
Temperature Probe	5267	28 Jan 2020	B9124036

Certificate Information:

Technician: 104

Procedure: CAL-06

Cal Date: 13 Feb 2019

Cal Due Date: 13 Feb 2021

Test Conditions: -38.85%RH 24.21°C 1023mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	0.000	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.000	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.000	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.001	100.004	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±[(Max-Min)/2]; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Aaron Justice

Aaron Justice, Technical Manager

Note:

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01, Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RvA, International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177835

Traceable® Certificate of Calibration for Digital Thermometer

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01
Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

TR. 1 DAVID M. NAPOLITANO
Name

7237
Badge No.

Location:

LONGPORT POLICE
Agency

ARXA-0067
Alcotest Serial No.

Equipment:

191 959 016
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDWE 53-0206	0729 S	0831 S	34.0 °C
0.08%	DDWF 53-0218	0729 S	0831 S	34.0 °C
0.10%	DDXC 53-0154	0729 S	0832 S	34.0 °C
0.16%	DDWT 53-0334	0729 S	0832 S	34.0 °C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius ± 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

J. D. [Signature] 7237
Coordinator's Signature

1.14.20
Date

Alcotest 7110 Calibration Record


Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00893 Calib. Date: 01/14/2020 Calib. No.: 00036
Certification File No.: 00877 Cert. Date: 07/22/2019 Cert. No.: 00029
Linearity File No.: 00878 Lin. Date: 07/22/2019 Lin. No.: 00029
Solution File No.: 00892 Soln. Date: 11/28/2019 Soln. No.: 00235
Sequential File No.: 00893 File Date: 01/14/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 07/23/2020
Solution Control Lot: 18220 Bottle No.: 0203

Coordinator

Last Name: NAPOLITANO First Name: DAVID MI: M.
Signature: *David Napolitano* 7237 Badge No.: 7237
Date: 01/14/2020

*Black Key Temperature Probe Serial.....# DDXK P2-396 (2)
*Digital NIST Temperature Measuring System Serial.....# 191 959 016 (2)

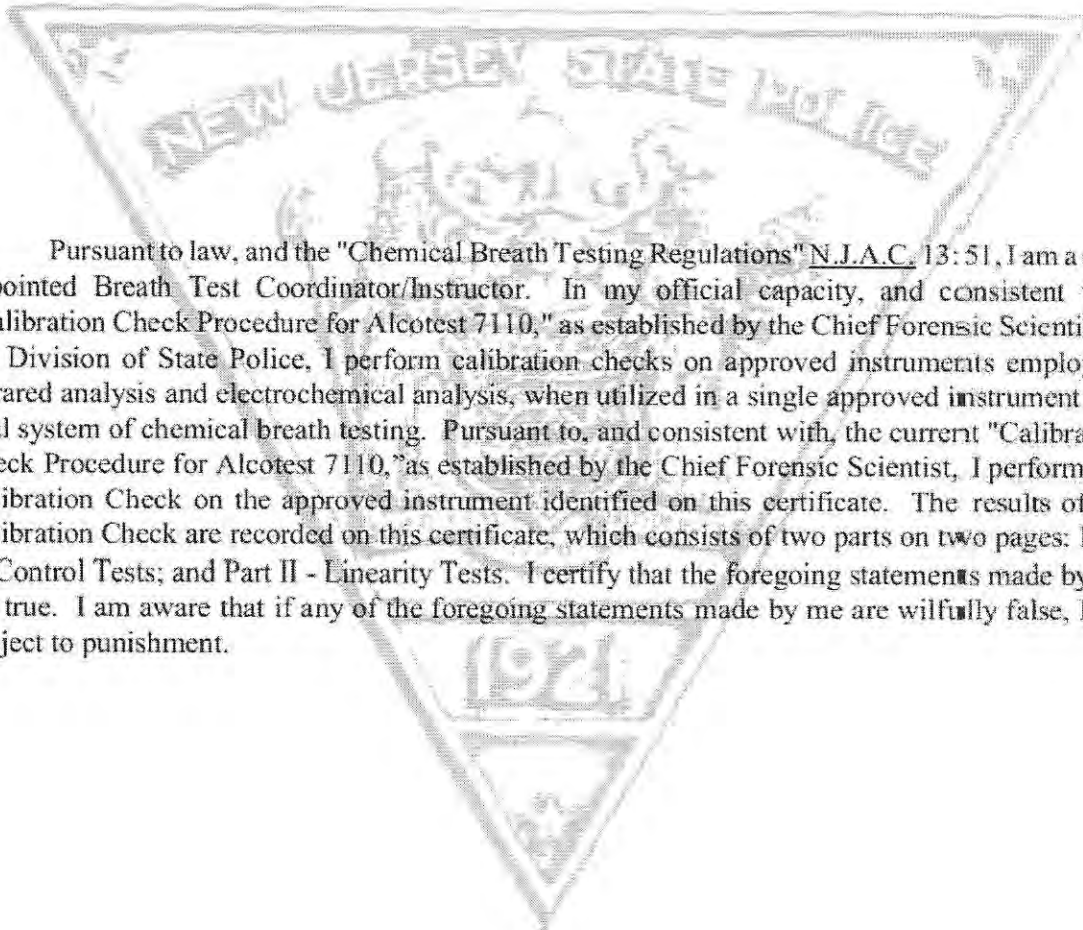

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00893 Calib. Date: 01/14/2020 Calib. No.: 00036
Certification File No.: 00894 Cert. Date: 01/14/2020 Cert. No.: 00030
Linearity File No.: 00878 Lin. Date: 07/22/2019 Lin. No.: 00029
Solution File No.: 00892 Soln. Date: 11/28/2019 Soln. No.: 00235
Sequential File No.: 00894 File Date: 01/14/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 07/23/2020
Solution Control Lot: 18220 Bottle No.: 0203

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:40S		
Control 1 EC	0.099%	08:40S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:41S		
Control 2 EC	0.099%	08:42S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:42S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:43S		
Control 3 EC	0.098%	08:43S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:43S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:44S		

All tests within acceptable tolerance.

Coordinator

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature: *David Napolitano* 7237

Badge No.: 7237

Date: 01/14/2020

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00893 Calib. Date: 01/14/2020 Calib. No.: 00036
Certification File No.: 00894 Cert. Date: 01/14/2020 Cert. No.: 00030
Linearity File No.: 00895 Lin. Date: 01/14/2020 Lin. No.: 00030
Solution File No.: 00892 Soln. Date: 11/28/2019 Soln. No.: 00235
Sequential File No.: 00895 File Date: 01/14/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0206
Control Solution %: 0.040% Expires: 07/31/2020
Solution Control Lot: 18240 Bottle No.: 0136

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0218
Control Solution %: 0.080% Expires: 08/06/2020
Solution Control Lot: 18250 Bottle No.: 0329

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0334
Control Solution %: 0.160% Expires: 08/21/2020
Solution Control Lot: 18260 Bottle No.: 0437

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:05S		
Control 1 EC	0.041%	09:05S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.038%	09:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:07S		
Control 2 EC	0.040%	09:08S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.039%	09:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:09S		
Control 3 EC	0.081%	09:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11S		
Control 4 EC	0.080%	09:12S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14S		
Control 5 EC	0.158%	09:15S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.158%	09:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16S		
Control 6 EC	0.158%	09:17S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.157%	09:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18S		

All tests within acceptable tolerance.


Coordinator

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature: _____

 7237

Badge No.: 7237

Date: 01/14/2020

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

David M. Napolitano

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Akotec 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 9th DAY OF October TWO THOUSAND AND Eighteen

[Signature]
COLONEL
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 01/18)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

David M. Napolitano
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Akotec 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 7th DAY OF October TWO THOUSAND AND Ten

[Signature]
SARJEANT-MAJOR
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 6/30/12	CAPE MAY P.A.	Adam Stankis
2. 11/6/14	GLPS	Adam Stankis
3. 6/23/16	CMPS	Adam Stankis
4. 1/16/18	LAKE HUDGETT	Adam Stankis
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 03/10)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL,
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/28/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0486 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 31, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaoui]

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29th day of August, 2018.
[Mary Elizabeth McLaughlin]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
WEST TRENTON, NJ 08628-0068
(609) 852-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/30/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0976 to 0.0987 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 06, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 4th day of September, 2018.
Notary [Signature]

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 832-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 07/31/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1210 to 0.1233 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaoie]

Ali M. Alaoie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of August, 2018.
[Mary Elizabeth McLaughlin signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/13/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1938 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15th day of September 2018.
Mary E. McLaughlin
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDWES3-0206

Certification Date:

7-19-19

Technician:

BS

Re-Certification Due Date:

7-19-20

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDWFS3-0218

Certification Date:

7-19-19

Technician:

BS

Re-Certification Due Date:

7-19-20

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDW) 53-0334

Certification Date:

7-19-19

Technician:

BS

Re-Certification Due Date:

7-19-20

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKPa-396

Certification Date:

7-18-19

Next Certification Due:

7-18-20

Probe Value:

104

Draeger, Inc.

BS



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor
SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General
PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 04/30/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19110

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 09, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 2nd day of May, 2019.
Notary



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

