



**Dräger**safety

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDUNP2-235

Certification date:

03/09/2006

Next Certification due:

03/09/2007

Probe Value

102

Draeger Safety Diagnostics, Inc.  
Technical Service Department

*Ant Dy*

# Alcotest 7110 Calibration Record

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00004 Calib. Date: 04/14/2006 Calib. No.: 00002  
Certification File No.: 00000 Cert. Date: --/--/---- Cert. No.: 00000  
Linearity File No.: 00000 Lin. Date: --/--/---- Lin. No.: 00000  
Solution File No.: 00002 Soln. Date: 03/09/2006 Soln. No.: 00001  
Sequential File No.: 00004 File Date: 04/14/2006

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135  
Control Solution %: 0.100% Expires: 11/29/2007  
Solution Control Lot: 05K021 Bottle No.: 0259

## Coordinator

Last Name: STANKS First Name: ADAM MI: N  
Signature: TPR. I Adam N. Stank #5403 Badge No.: 5403  
Date: 04/14/2006

BLACK KEY TEMPERATURE PROBE SERIAL NUMBER: DDUNP2-235 *ams*

ERTCO - HART DIGITAL TEMPERATURE MEASURING SYSTEM  
SERIAL NUMBER: A18522 *ams*

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00004 Calib. Date: 04/14/2006 Calib. No.: 00002  
Certification File No.: 00005 Cert. Date: 04/14/2006 Cert. No.: 00001  
Linearity File No.: 00000 Lin. Date: --/--/---- Lin. No.: 00000  
Solution File No.: 00002 Soln. Date: 03/09/2006 Soln. No.: 00001  
Sequential File No.: 00005 File Date: 04/14/2006

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135  
Control Solution %: 0.100% Expires: 11/29/2007  
Solution Control Lot: 05K021 Bottle No.: 0259

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:12D		
Control 1 EC	0.099%	12:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:13D		
Control 2 EC	0.099%	12:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:14D		
Control 3 EC	0.099%	12:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15D		

All tests within acceptable tolerance.

### Coordinator

Last Name: STANKS First Name: ADAM MI: N  
Signature: TPR I Adam N Stanks # 5403 Badge No.: 5403  
Date: 04/14/2006

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE		
Calibration File No.:	00004	Calib. Date:	04/14/2006
Certification File No.:	00005	Cert. Date:	04/14/2006
Linearity File No.:	00006	Lin. Date:	04/14/2006
Solution File No.:	00002	Soln. Date:	03/09/2006
Sequential File No.:	00006	File Date:	04/14/2006
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.040%	Serial No.:	DDWE S3-0196
Solution Control Lot:	05C015	Expires:	03/09/2007
		Bottle No.:	0069
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.080%	Serial No.:	DDWE S3-0203
Solution Control Lot:	04F007	Expires:	06/08/2006
		Bottle No.:	0057
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.160%	Serial No.:	DDWE S3-0205
Solution Control Lot:	05C016	Expires:	03/09/2007
		Bottle No.:	0054

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:30D		
Control 1 EC	0.040%	12:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	12:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		
Control 2 EC	0.040%	12:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	12:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		
Control 3 EC	0.079%	12:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	12:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:36D		
Control 4 EC	0.079%	12:36D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.076%	12:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37D		
Control 5 EC	0.159%	12:38D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.158%	12:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:39D		
Control 6 EC	0.159%	12:40D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.158%	12:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41D		

All tests within acceptable tolerance.

**Coordinator**

Last Name: STANKS

First Name: ADAM

MI: N

Signature: TPR. I Adam N. Stank #5403


Badge No.: 5403

Date: 04/14/2006

DEPARTMENT OF  
*Law and Public Safety*  
 This is to certify that

**ADAM N. STANKS**  
**NEW JERSEY STATE POLICE**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF  
 THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIIC**  
 A METHOD TO DETERMINE INTOXICATION.  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF December

TWO THOUSAND AND **FOUR**  
  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	11/21/06	Sayreville PD	S. J. [Signature]
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			


DEPARTMENT OF  
*Law and Public Safety*  
This is to certify that


ADAM N. STANKS

NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIIC**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF December

TWO THOUSAND AND **FOUR**

  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 06/03)

## Ertco-Hart Digital Temperature Measuring System

### REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature verification Serial Number: 303176

Digital Units Serial Number: A18522

Probe Serial Number: 557904

Certification Date: 02/28/2006

Next Certification Due: 02/28/2007

At 34.00 °C digital unit displays 33.98 °C

Draeger Safety Diagnostics, Inc. Technician: Cent Dly

**Dräger**safety

**ALCOTEST® 7110 TEMPERATURE PROBE**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDW 14P2-199

Certification date:

03/08/2006

Next Certification due:

03/08/2007


Probe Value

103

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

Curt Rly





Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34  
 Model: MARK IIA  
 Other: \_\_\_\_\_

Serial Number:

DDWE 53-0196

Certification Date


MAR 09 2006

Technician

DB

Re-Certification Due Date

MAR 09 2007



**Dräger**safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWE 53-0203

Certification Date

MAR 09 2006

Technician

DB

Re-Certification Due Date

MAR 09 2007

USED TO CALIBRATE MACHINE



**Draeger**safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34  
 Model: MARK IIA  
 Other: \_\_\_\_\_

Serial Number:

DDWE 53-0205

Certification Date

MAR 09 2006

Technician

DB

Re-Certification Due Date

MAR 09 2007



**Dräger**safety

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDUNP2-235

Certification date:

03/09/2006

Next Certification due:

03/09/2007

Probe Value

102

Draeger Safety Diagnostics, Inc.  
Technical Service Department

Ant Dly

## Ertco-Hart Digital Temperature Measuring System

### REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature verification Serial Number: 303176

Digital Units Serial Number: A18522

Probe Serial Number: 557904

Certification Date: 02/28/2006

Next Certification Due: 02/28/2007

At 34.00 °C digital unit displays 33.98 °C

Draeger Safety Diagnostics, Inc. Technician: Cent Dely



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

RICHARD J. CODEY
Acting Governor

PETER C. HARVEY
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 4/18/05

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 05C015

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0483 to 0.0484 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 9, 2007.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Thomas A. Brettell

Thomas A. Brettell, Ph.D.
Forensic Laboratory Director
Division of State Police

Sworn to and subscribed before me this 14th day of June, 2005.

Handwritten signature of Linda L. DeSantis
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

RICHARD J. CODEY
Acting Governor

PETER C. HARVEY
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 4/18/05

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 04F007

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0958 to 0.0963 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 8, 2006.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Thomas A. Brettell

Thomas A. Brettell, Ph.D.
Forensic Laboratory Director
Division of State Police

Sworn to and subscribed before me this 14th day of June, 2005.

Handwritten signature of Linda L. DeSantis
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

RICHARD J. CODEY  
Acting Governor

PETER C. HARVEY  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 12/12/05

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 05K021

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1208 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 29, 2007.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Thomas A. Brettell*  
Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 20th day of December, 2005.

*Linda L. DeSantis*  
Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009







State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

RICHARD J. CODEY  
Acting Governor

PETER C. HARVEY  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 4/18/05

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 05C016

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1942 to 0.1946 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 9, 2007.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 14<sup>th</sup> day of June, 2005.

  
Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009




DEPARTMENT OF  
**Law and Public Safety**  
This is to certify that

ADAM N. STANKS

NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIHC**  
A METHOD TO DETERMINE INTOXICATION.  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF December

TWO THOUSAND AND **FOUR**

  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11/21/06	SAYREVILLE PD	S. J. [Signature]
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		



State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

JON S. CORZINE  
Governor

ZULIMA V. FARBER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 3/02/06

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 06B023

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1214 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 10, 2008.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 16<sup>th</sup> day of March, 2006.

Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009



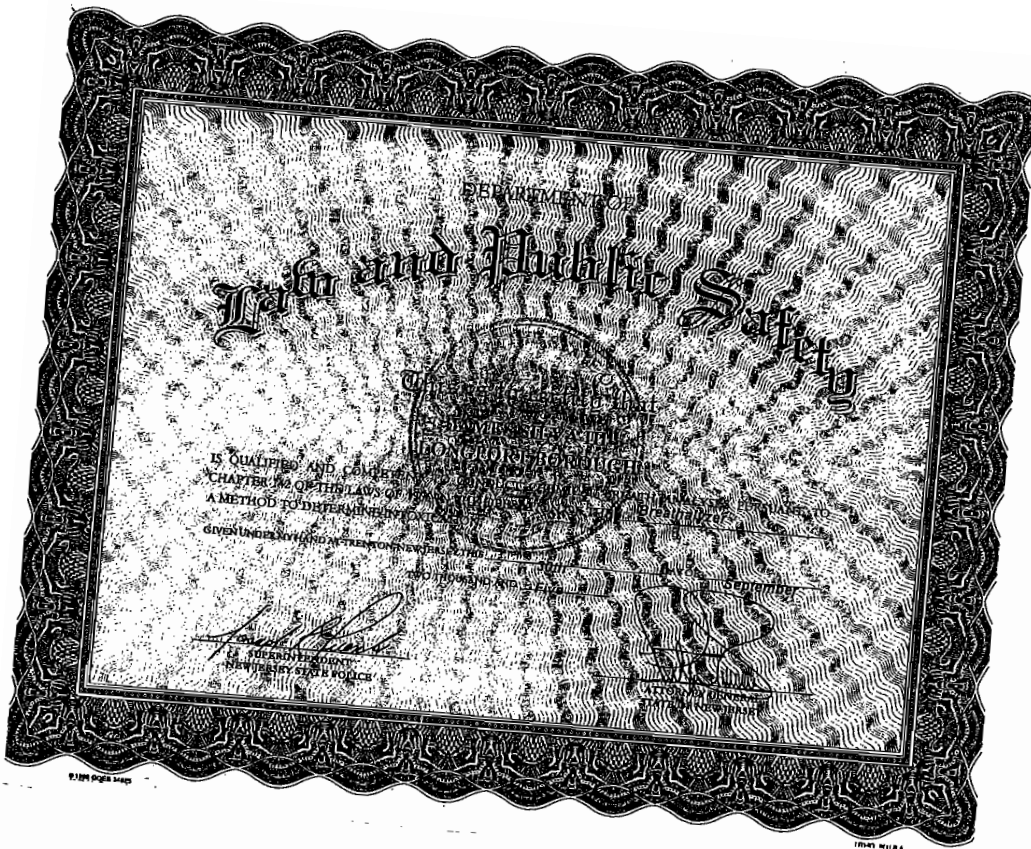

DEPARTMENT OF  
**Public and Public Safety**  
 This is to certify that

**James F. Silva III**  
**Longport Boro**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL URINE ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOHET 7110 MKIII-C** A METHOD TO DETERMINE INTOXICATION. GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 17th DAY OF March

TWO THOUSAND AND SIX

*Joseph P. ...*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*Julian V. ...*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY


**Certificate of Training**

This is to certify that

**James F. Silva III**

has successfully completed practitioner training in the use of  
**Horizontal Gaze Nystagmus**  
**Improved Sobriety Test Procedures**  
 as set forth by the National Highway Traffic Safety Administration

*[Signature]* Director, Division of Highway Traffic Safety  
*[Signature]* Instructor



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXCS3-0154

Certification Date

Technician

Re-Certification Due Date

11/13/2006

CRD

11/13/2007

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWAP2-177

11/13/2006

11/13/2007

Probe Value

104

Draeger Safety Diagnostics, Inc.  
Technical Service Department

CRD



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

Jon S. Corzine
Governor

ZULIMA V. PARBER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drazer Safety, Inc. ANALYSIS DATE: 3/02/06

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 06B023

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1214 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 10, 2008.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Thomas A. Brettell

Thomas A. Brettell, Ph.D.
Forensic Laboratory Director
Division of State Police

Sworn to and subscribed before me this 16th day of March, 2006.

[Signature]
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

RICHARD J. CODEY  
Acting Governor

PETER C. HARVEY  
Attorney General

COLONEL JOSEPH R. PUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 12/12/05

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 05K021

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1208 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 29, 2007.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Thomas A. Brettell*  
Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 28<sup>th</sup> day of December, 2005.

*Linda L. DeSantis*  
Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

JON S. CORZINE  
Governor

ZULIMA V. FARRER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.

**ANALYSIS DATE:** 3/17/06

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 06B026

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0477 to 0.0479 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 25, 2008.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 10<sup>th</sup> day of April, 2006.

  
Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009







State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

JON S. CORZINE  
Governor

ZULIMA V. FARBER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.

**ANALYSIS DATE:** 3/17/06

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 06B024

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0956 to 0.0959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 24, 2008.


As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 10<sup>th</sup> day of April, 2006.

  
Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

JON S. CORZINE  
Governor

ZULIMA V. FARBER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 3/17/06

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 06B025

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1916 to 0.1929 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 25, 2008.

As Forensic Laboratory Director of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Thomas A. Brettell, Ph.D.  
Forensic Laboratory Director  
Division of State Police

Sworn to and subscribed before me this 10<sup>th</sup> day of April, 2006.

Notary


Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009



DEPARTMENT OF  
*Law and Public Safety*  
This is to certify that

**ADAM N. STANKS**  
**NEW JERSEY STATE POLICE**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 143 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIIIIC  
A METHOD TO DETERMINE INTOXICATION.  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF December

TWO THOUSAND AND FOUR  
  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11/21/06	SPRINGVILLE P.D.	S. J. [Signature]
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

DEPARTMENT OF  
**Law and Public Safety**  
 This is to certify that

Adam N. Stanks

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE Breathalyzer METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF APR.  
 ONE THOUSAND NINE HUNDRED AND 97

Carla Williams  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

Peter Vermeir  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

1	DATE	Refresher Course		INSTRUCTOR
		PLACE		
1	4-26-88	ACTC		RM Janczon
2	10/12/01	OCPA		D. Janczon
3	9-3-03	ACTC		RM Janczon
4	7-18-05	ACTC		C. Potter
5	3-2-07	OCPA		C. Potter
6				
7				
8				
9				

SP-293B