

ALCOTEST CHECKLIST

Municipality: LONGPORT

Alcotest Ser. #: ARXA-0067

County: ATLANTIC

Date of Calibration: 07-19-2023

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC 53-0154
3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWA P2-177
4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 221473067
5. **NIST - Traceable Digital Thermometer Readings.**
6.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDMB P1-0119
7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>22250</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>22270</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>22230</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>22290</u>
8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

<input checked="" type="checkbox"/> A.	0.04% used in Calibration/Linearity Testing.	<u>DDXD 53-0187</u>
<input checked="" type="checkbox"/> B.	0.08% used in Calibration/Linearity Testing.	<u>DDRK 53-0006</u>
<input checked="" type="checkbox"/> C.	0.10% used in Calibration/Linearity Testing. [Same as CU34 unit on instrument.]	
<input checked="" type="checkbox"/> D.	0.16% used in Calibration/Linearity Testing.	<u>DDCB-0001</u>
9.
 - A. New Standard Solution Report following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 23110
 - D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest[®] 7110 MKII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKII-C is compliant as a mobile and nonmobile EBT with 49 FR 48884, 48 FR 48864 and 53 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

1-10-14

SERIAL NUMBER:

ARXA-07107

Dräger Safety Diagnostics, Inc.

BC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDXCS3-0154

Certification Date:

1-2-23

Technician:

DH/ MB

Re-Certification Due Date:

1-2-24

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWAP2-177

Certification Date:

1-2-23

Next Certification Due:

1-2-24

Probe Value:

107

Draeger, Inc.

DH/ MB



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-13326328

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 221473067

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Temperature Probe	128	09 Jul 2022	15-D4F0Q-40-1
Thermistor Module	A17118	08 Jul 2022	1000469276
Temperature Calibration Bath	A45240		
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Thermistor Module	B96381	18 Aug 2022	1000470702
Temperature Probe	5392	04 Aug 2022	4500006080
Temperature Probe	5398	24 Aug 2022	4500006081
Thermistor Module	B96382	08 Oct 2022	1000472708
Temperature Probe	5410	20 Oct 2022	4500006780

Certificate Information:

Technician: 299

Procedure: CAL-06

Cal Date: 25 Apr 2022

Cal Due Date: 25 Apr 2024

Test Conditions: 58.46%RH 23.43°C 1017mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	-0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.000	25.001	Y	24.95	25.05	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.001	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		100.001	100.003	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement: (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ± U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Marisa Elms

Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained, Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1760.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-13326328

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 26 Apr 2022

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

TPR. II William F. Widener
Name

7817
Badge No.

Location:

Longport Police
Agency

ARXA-0067
Alcotest Serial No.

Equipment:

221 473 067
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDXD S3-0187	11:12 D	12:15 D	33.9°C
0.08%	DDRK S3-0006	11:12 D	12:16 D	34.0°C
0.10%	DDXC S3-0154	11:12 D	12:17 D	33.9°C
0.16%	DDCB-0001	11:12 D	12:18 D	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

TPR. II Wm F. Widener #7817
Coordinator's Signature

07/19/2023
Date

Alcotest 7110 Calibration Record


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE		
Calibration File No.:	00989	Calib. Date:	07/19/2023
Certification File No.:	00980	Cert. Date:	03/01/2023
Linearity File No.:	00981	Lin. Date:	03/01/2023
Solution File No.:	00986	Soln. Date:	06/22/2023
Sequential File No.:	00989	File Date:	07/19/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0154
Solution Control Lot:	22230	Expires:	06/28/2024
		Bottle No.:	1472

Coordinator

Last Name: WIDENER First Name: WILLIAM MI: F
Signature: Ter. J. Wm. F. Widener #7817 Badge No.: 7817
Date: 07/19/2023

*Black Key Temperature Probe Serial.....# DDMBP1-0119 (WFW)

*Digital NIST Temperature Measuring System Serial.....# 221 473 067 (WFW)

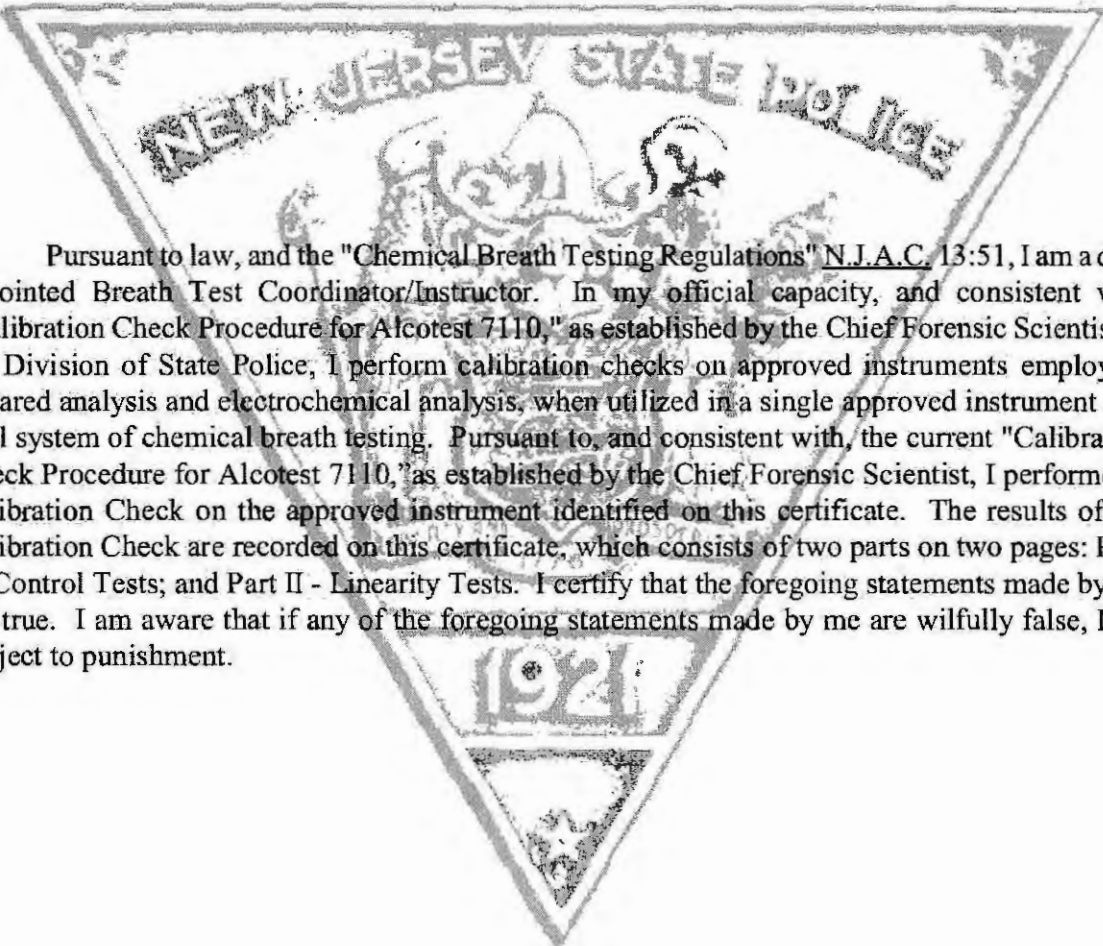

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE		
Calibration File No.:	00989	Calib. Date:	07/19/2023
Certification File No.:	00990	Cert. Date:	07/19/2023
Linearity File No.:	00981	Lin. Date:	03/01/2023
Solution File No.:	00986	Soln. Date:	06/22/2023
Sequential File No.:	00990	File Date:	07/19/2023
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0154
Solution Control Lot:	22230	Expires:	06/28/2024
		Bottle No.:	1472

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:29D		
Control 1 EC	0.101%	12:30D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:30D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 2 EC	0.099%	12:31D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:31D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		
Control 3 EC	0.099%	12:33D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:33D		


All tests within acceptable tolerance.

Coordinator

Last Name: WIDENER

First Name: WILLIAM

MI: F

Signature:  #7817

Badge No.: 7817

Date: 07/19/2023

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00989 Calib. Date: 07/19/2023 Calib. No.: 00044
Certification File No.: 00990 Cert. Date: 07/19/2023 Cert. No.: 00038
Linearity File No.: 00991 Lin. Date: 07/19/2023 Lin. No.: 00038
Solution File No.: 00986 Soln. Date: 06/22/2023 Soln. No.: 00279
Sequential File No.: 00991 File Date: 07/19/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0187
Control Solution %: 0.040% Expires: 07/19/2024
Solution Control Lot: 22250 Bottle No.: 0624

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0006
Control Solution %: 0.080% Expires: 07/28/2024
Solution Control Lot: 22270 Bottle No.: 0617

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCB-0001
Control Solution %: 0.160% Expires: 08/04/2024
Solution Control Lot: 22290 Bottle No.: 0195

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:48D		
Control 1 EC	0.041%	12:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	12:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:50D		
Control 2 EC	0.041%	12:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	12:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:52D		
Control 3 EC	0.082%	12:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.081%	12:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:55D		
Control 4 EC	0.081%	12:55D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	12:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:57D		
Control 5 EC	0.159%	12:58D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.158%	12:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:59D		
Control 6 EC	0.158%	13:00D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.159%	13:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:02D		

All tests within acceptable tolerance.

Coordinator

Last Name: WIDENER

First Name: WILLIAM

MI: F

Signature: Tr. J. W. Widener #7817

Badge No.: 7817

Date: 07/19/2023

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

William F. Widener III
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE A METHOD TO DETERMINE INTOXICATION, GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 19th DAY OF August SIXTEEN

L. P. [Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12/3/18	Green	Adrian [Signature]
2. 9-8-20	ACCC	Winton
3. 2-7-22	ACCC	[Signature]
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2330 (Rev. 08/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

William F. Widener

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7119 MKIII-C A METHOD TO DETERMINE INTOXICATION, GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 1st DAY OF March THIRTY AND Twenty Three

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2330 (Rev. 10/22)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 842-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/17/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0483 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110822
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/18/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0967 to 0.0983 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 28, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/20/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1194 to 0.1212 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 27 day of July, 2022.

Notary



KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission #: 60110822
My Commission Expires 0/13/2024

NOTARY PUBLIC OF NEW JERSEY
Commission #: 60110822
My Commission Expires 0/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor
SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General
COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/22/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1924 to 0.1948 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 4, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 01/31/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249, 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDXDS3-0187

Certification Date:

5-22-23

Technician:

DH / MB

Re-Certification Due Date:

5-22-24

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249, 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDRKS3-0006

Certification Date:

5-22-23

Technician:

DH / MB

Re-Certification Due Date:

5-22-24

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDCB-0001

Certification Date:
5-22-23

Technician:
DH / MB

Re-Certification Due Date:
5-22-24

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:
DDMBP1-0119

Certification Date:
5-30-23

Next Certification Due:
5-30-24

Probe Value:
104

Draeger, Inc.

DH / MB

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00989	Calib. Date: 07/19/2023
Certification File No.:	00990	Calib. No.: 00044
Linearity File No.:	00991	Cert. Date: 07/19/2023
Solution File No.:	00992	Cert. No.: 00038
Sequential File No.:	00992	Lin. Date: 07/19/2023
		Lin. No.: 00038
		Soln. Date: 07/19/2023
		Soln. No.: 00280
		File Date: 07/19/2023
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	23110	Expires: 04/12/2025
		Bottle No.: 0671

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:10D		
Control 1 EC	0.103%	14:11D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	14:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:12D		
Control 2 EC	0.102%	14:12D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	14:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:13D		
Control 3 EC	0.101%	14:14D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-177 (WFW)

Changed By:

Last Name: WIDENER	First Name: WILLIAM	MI: F
Signature: <u>W.F. Widener #7817</u>	Badge No.: 7817	Date: 07/19/2023



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 05/15/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23110

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1204 to 0.1215 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 12, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 19 day of May, 2023.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

