

ALCOTEST CHECKLIST

Municipality: LONGPORT Alcotest Ser.#: ARXA-0067

County: ATLANTIC Date of Calibration: 08-18-09

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R..
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC S3-0154
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWA P2-177
- 4. **Digital Temperature Measuring System Report of Calibration.**
- 5.
 - A. Alcotest 7110 Calibration Record
 - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 - D. **Alcotest Card** of operator/coordinator who performed tests.
 - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDWA P2-016
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
 - A. 0.04% Solution. 08 F 054
 - B. 0.08% Solution. 08 F 055
 - C. 0.10% Solution. 08 G 056
 - D. 0.16% Solution. 08 G 057
- 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
 - A. 0.04% used in Calibration/Linearity Testing DDWE S3-0196
 - B. 0.08% used in Calibration/Linearity Testing DDWE S3-0203
 - C. 0.10% used in Calibration/Linearity Testing DDXC S3-0154
[Same as instrument's CU34 unit].
 - D. 0.16% used in Calibration/Linearity Testing DDWE S3-0205
- 8.
 - A. New Standard Solution Report - following Calibration.
 - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 - C. Certificate of Analysis 0.10% solution for same.
Lot #: 08 B 050
 - D. Alcotest card of operator/coordinator who completed change.

RJP

Dräger safety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


SERIAL NUMBER:

03/09/2000

ARXA - 0067

Draeger Safety Diagnostics, Inc.
Durango, CO

Ante Dely



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXC 53-0154

Certification Date

Technician

Re-Certification Due Date

JAN. 22/2008

TS

JAN. 22/2009

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWAP2-177

01-22-08

01-22-09

Probe Value

104

Draeger Safety Diagnostics, Inc.
Technical Service Department



Calibration
Certificate No. 1750.01

Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NC SL Z540-1



Cert. No.: 4000-2035927

Traceable® Certificate of Calibration for Digital Thermometer

Instrument Identification:

Model: 61220-601 S/N: 80637585 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Probe	149	3/06/09	A82225037-3
Thermistor Module	A27129	8/22/09	1000248949
Temperature Calibration Bath TC218	A73332		
Temperature Calibration Bath TC155	93139		
Thermistor Module	A27129	8/22/09	1000248949
Temperature Probe	157	5/28/09	A8519038-4

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 11/18/08 Cal Due: 11/18/10
Test Conditions: 25.0°C 34.0 %RH 1031 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±uc	TUR
°C		N.A.		0.001	-0.002	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.001	25.003	Y	24.951	25.051	0.013	3.8:1
°C		N.A.		60.001	59.998	Y	59.951	60.051	0.018	2.8:1
°C		N.A.		100.001	100.001	Y	99.951	100.051	0.013	3.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Date=MM/DD/YY.

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2000 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-AQ-HOU.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00343 Calib. Date: 08/18/2009 Calib. No.: 00007
Certification File No.: 00285 Cert. Date: 02/23/2009 Cert. No.: 00005
Linearity File No.: 00286 Lin. Date: 02/23/2009 Lin. No.: 00005
Solution File No.: 00341 Soln. Date: 08/14/2009 Soln. No.: 00073
Sequential File No.: 00343 File Date: 08/18/2009


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 07/02/2010
Solution Control Lot: 08G056 Bottle No.: 0023

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
Signature: Joe Dellanoce # 6027 Badge No.: 6027
Date: 08/18/2009

*Black Key Temperature Probe Serial.....# DDWAP2-016 *gso*

*Digital NIST Temperature Measuring System Serial.....# 80637585 *gso*

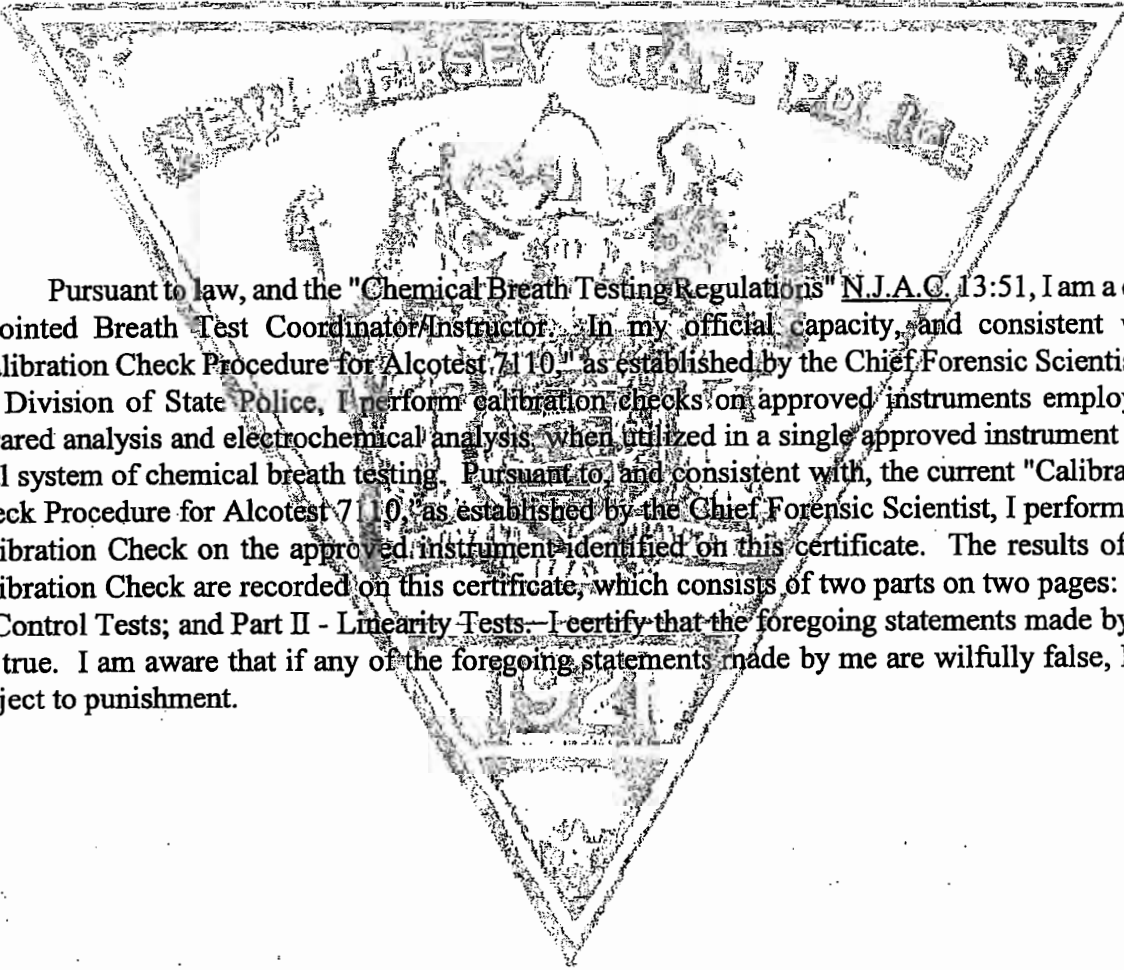

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00343 **Calib. Date:** 08/18/2009 **Calib. No.:** 00007
Certification File No.: 00344 **Cert. Date:** 08/18/2009 **Cert. No.:** 00006
Linearity File No.: 00286 **Lin. Date:** 02/23/2009 **Lin. No.:** 00005
Solution File No.: 00341 **Soln. Date:** 08/14/2009 **Soln. No.:** 00073
Sequential File No.: 00344 **File Date:** 08/18/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDXC S3-0154
Control Solution %: 0.100% **Expires:** 07/02/2010
Solution Control Lot: 08G056 **Bottle No.:** 0023

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:52D		
Control 1 EC	0.099%	12:53D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:54D		
Control 2 EC	0.099%	12:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:55D		
Control 3 EC	0.099%	12:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:56D		

All tests within acceptable tolerance.

Coordinator
Last Name: DEL ANOCE First Name: JOSEPH
Signature: Tpr. J. Del Anoce # 6027 Badge: 107697 Date: 08/18/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00343 Calib. Date: 08/18/2009 Calib. No.: 00007
Certification File No.: 00344 Cert. Date: 08/18/2009 Cert. No.: 00006
Linearity File No.: 00345 Lin. Date: 08/18/2009 Lin. No.: 00006
Solution File No.: 00341 Soln. Date: 08/14/2009 Soln. No.: 00073
Sequential File No.: 00345 File Date: 08/18/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0196
Control Solution %: 0.040% Expires: 06/26/2010
Solution Control Lot: 08F054 Bottle No.: 1184

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0203
Control Solution %: 0.080% Expires: 06/28/2010
Solution Control Lot: 08F055 Bottle No.: 0143

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0205
Control Solution %: 0.160% Expires: 07/07/2010
Solution Control Lot: 08G057 Bottle No.: 0706

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:11D		
Control 1 EC	0.041%	13:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	13:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:13D		
Control 2 EC	0.040%	13:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	13:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:15D		
Control 3 EC	0.079%	13:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	13:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		
Control 4 EC	0.080%	13:18D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	13:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19D		
Control 5 EC	0.161%	13:20D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.161%	13:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21D		
Control 6 EC	0.160%	13:22D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.160%	13:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:23D		

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tpr. II [Signature] # 6027


Badge No.: 6027


Date: 08/18/2009

DEPARTMENT OF
Law and Public Safety

Joseph S. Dellanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT EMERGENCY TRAINING AND EVALUATE PERFORMANCE TO CHAPTER 10 OF
 THE LAWS OF 1984 IN THE OPERATION OF THE Atedtest 7110 MTCII-C
 A METHOD TO DETERMINE INDETERMINATE
 DETERMINED BY HAND AT TELEVISION, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND

 SERGEANT JOSEPH S. DELLANOCE
 NEW JERSEY STATE POLICE

FIVE

 ATTORNEY GENERAL
 STATE OF NEW JERSEY

11

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2/15/07	CCPA	C. P. [Signature]
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 12/04)

DEPARTMENT OF
Traffic and Public Safety

This is to certify that
Joseph S. Dallanocce
New Jersey State Police

IS QUALIFIED AND COMPETENT TO INSTRUCT AND ANALYZE PULSANT TO CHAPTER
111 OF THE LAWS OF 1944 OF THE OPERATION OF THE Breathalyzer
A METHOD TO DETERMINE INTOXICATION

CIVIL UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 13th DAY OF Dec
TWO THOUSAND AND 01

Cum F. Kelly
SUPERINTENDENT
NEW JERSEY STATE POLICE

John P. ...
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES: 8/30 - 9/3/99

Refresher Course

	DATE	PLACE	INSTRUCTOR
1.	<u>12/12/01</u>	<u>A.G.P.C.</u>	<u>Porter</u>
2.	<u>2-20-03</u>	<u>6/2/04</u>	<u>C. Porter</u>
3.	<u>10/3-03</u>	<u>ACTE</u>	<u>C. Stambic</u>
4.			
5.			
6.			
7.			
8.			
9.			

SP-293B (Rev. 4/00)

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDNAPR-016

Certification date:

02/23/2009

Next Certification due:

02/03/2010

Probe Value

106

Dräger Safety Diagnostics, Inc.
Technical Service Department

[Signature]



JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR PREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 07/16/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F054

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0487 to 0.0493 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary
JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/25/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F055

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0977 to 0.0984 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/24/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G056

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1227 to 0.1236 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 2, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 13th day of August, 2008.

Notary

Linda L. DeSantis
 My Commission
 Expires Aug. 17, 2009





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G057

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1956 to 0.1959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





Draegersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 24912/1994 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWE53-0196

Certification Date

Technician

Re-Certification Due Date

02-03-09

[Signature]

02-03-10



Draeger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWE 53-0203

Certification Date

02.03.09

Technician

Re-Certification Due Date

02.03.10



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0205

Certification Date

Technician

Re-Certification Due Date

02-03-09

[Signature]

02-03-10

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00343 **Calib. Date:** 08/18/2009 **Calib. No.:** 00007
Certification File No.: 00344 **Cert. Date:** 08/18/2009 **Cert. No.:** 00006
Linearity File No.: 00345 **Lin. Date:** 08/18/2009 **Lin. No.:** 00006
Solution File No.: 00346 **Soln. Date:** 08/18/2009 **Soln. No.:** 00074
Sequential File No.: 00346 **File Date:** 08/18/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDXC S3-0154
Control Solution %: 0.100% **Expires:** 02/13/2010
Solution Control Lot: 08B050 **Bottle No.:** 0349

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:30D		
Control 1 EC	0.102%	14:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:31D		
Control 2 EC	0.101%	14:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:33D		
Control 3 EC	0.100%	14:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWAP2-177 *js*

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: *Tpr. II JS #6027*

Badge No.: 6027

Date: 08/18/2009



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

**CERTIFICATION OF ANALYSIS
 0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 03/14/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08B050

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1229 to 0.1234 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 13, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 31 st day of March, 2008.

Simon L. DeSantis

NOTARY
 Simon L. DeSantis
 My Commission
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

RECEIPT

Table with 2 columns: RECEIVED FROM: (Name) and AGENCY: (Name and Address). Includes details for Steve Dellanoce and New Jersey State Police - Alcohol Drug Testing Unit.

DESCRIPTION AND LIST OF PROPERTY:

- 1. One CD-R Memory Download Disc created on this day from Alcotest serial # ARXA-0067 marked NON-REDACTED to be maintained by your Agency for safe keeping for REFERENCE PURPOSES ONLY.
2. One CD-R Memory Download Disc created on this day from Alcotest serial # ARXA-0067 marked REDACTED to be maintained by your Agency to be copied for DISCOVERY PURPOSES if/when court ordered.

(PLACE "X" IN APPROPRIATE SPACE)

RECEIVED: As Evidence For Safekeeping X On Loan

Table with 3 columns: DATE (8/18/09), STATION / UNIT / AGENCY NAME (mike mailer), and SIGNATURE (unavailable). Includes AGENCY: Longport P.D.

